
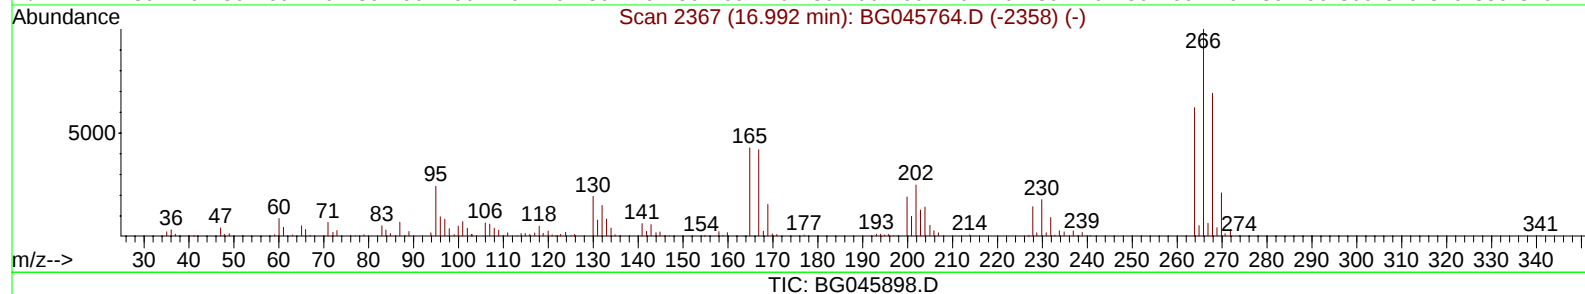
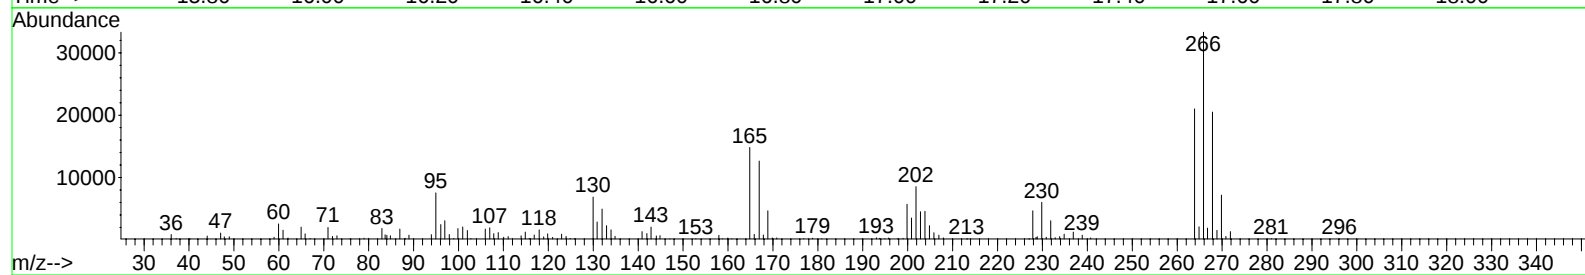


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070120\
Data File : BG045898.D
Acq On : 1 Jul 2020 9:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 01 19:02:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 01 14:59:28 2020
Response via : Initial Calibration

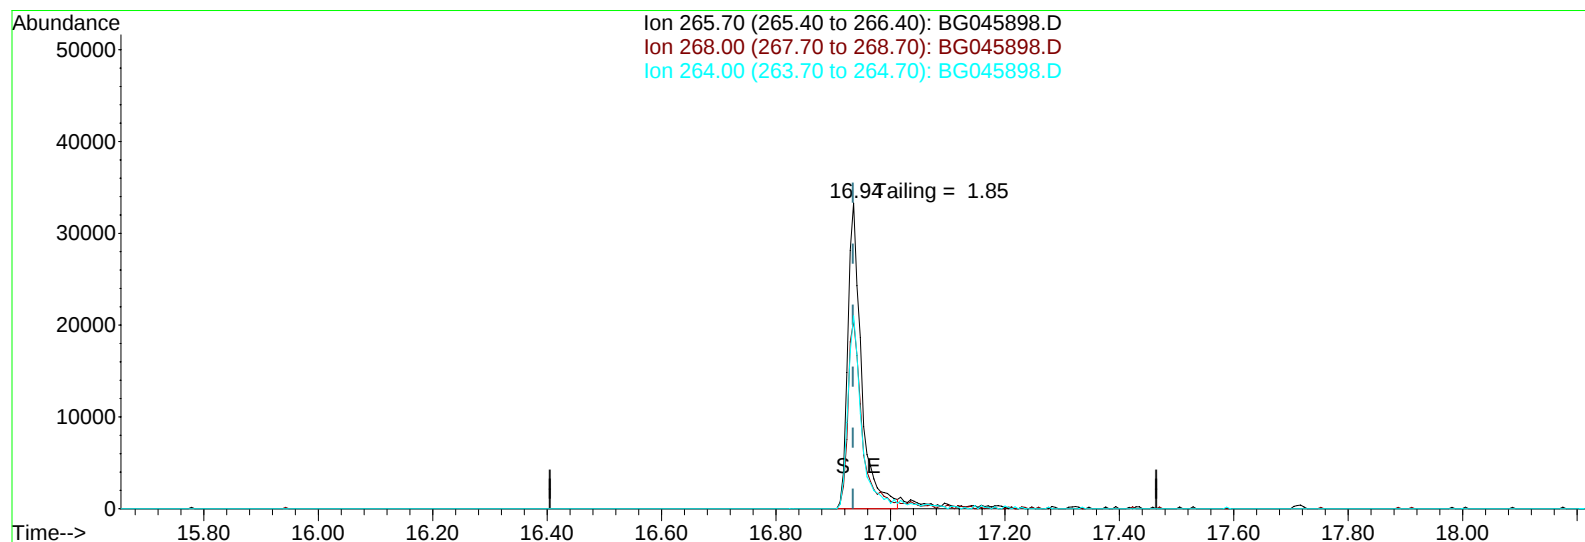

(70) Pentachlorophenol (C)




16.936min (+0.001) 18297.91ng

response 56564

Ion	Exp%	Act%
265.70	100	100
268.00	62.00	61.54
264.00	61.00	63.08
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070120\
 Data File : BG045898.D
 Acq On : 1 Jul 2020 9:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 01 19:02:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 01 14:59:28 2020
 Response via : Initial Calibration

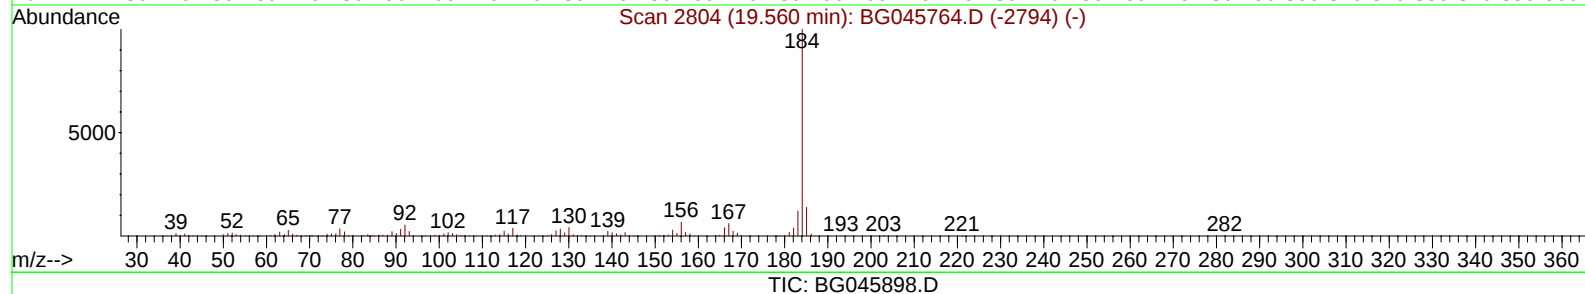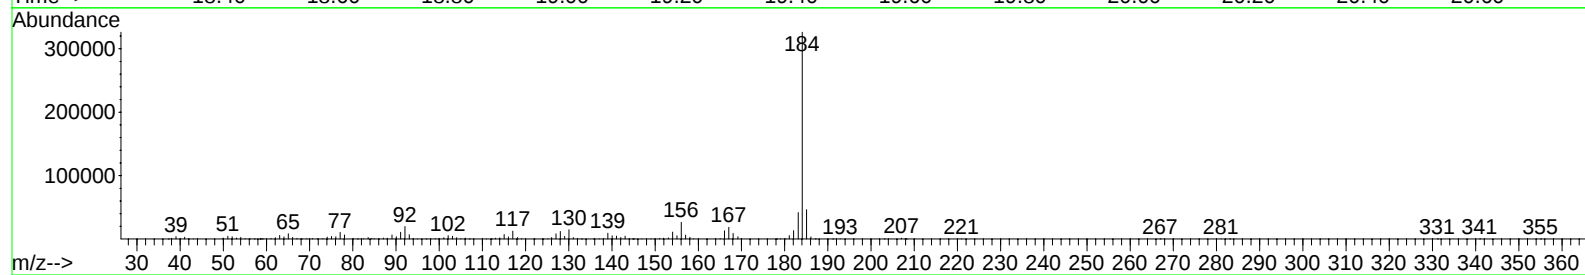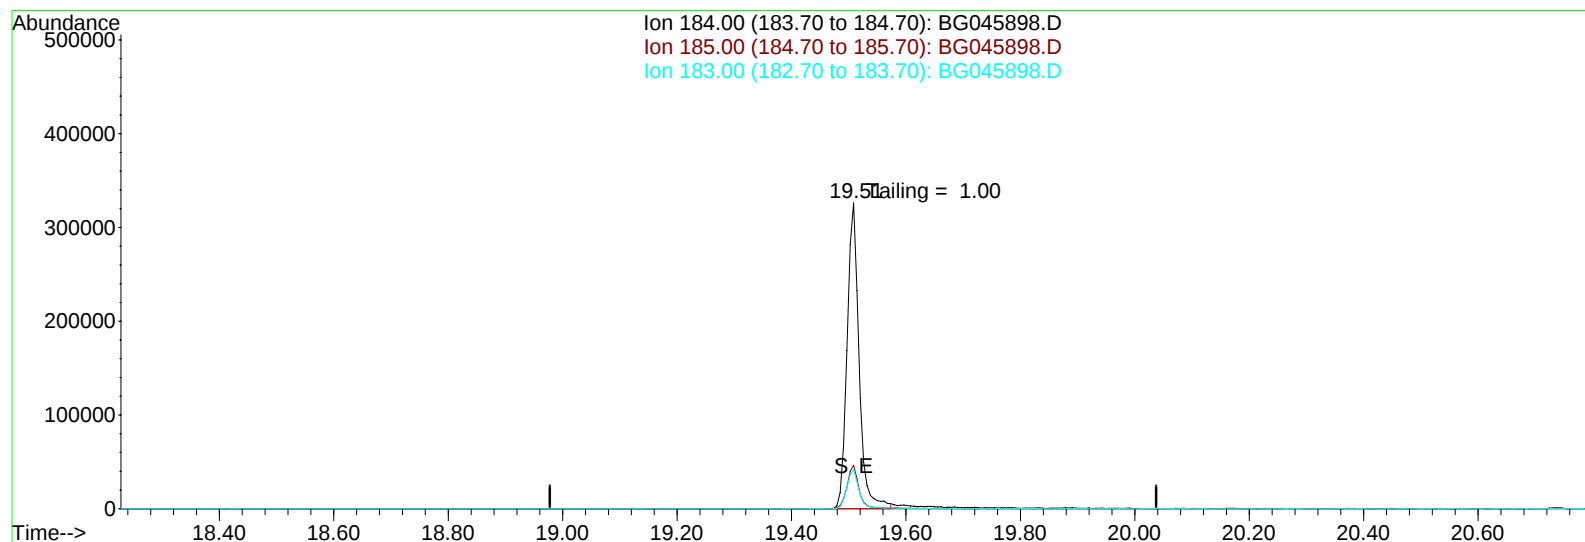

(77) Benzidine

19.507min (-19.507) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	14.50	0.00#
183.00	13.00	0.00#
0.00	0.00	0.00