


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070120\
 Data File : BG045898.D
 Acq On : 1 Jul 2020 9:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 02 14:02:29 2020

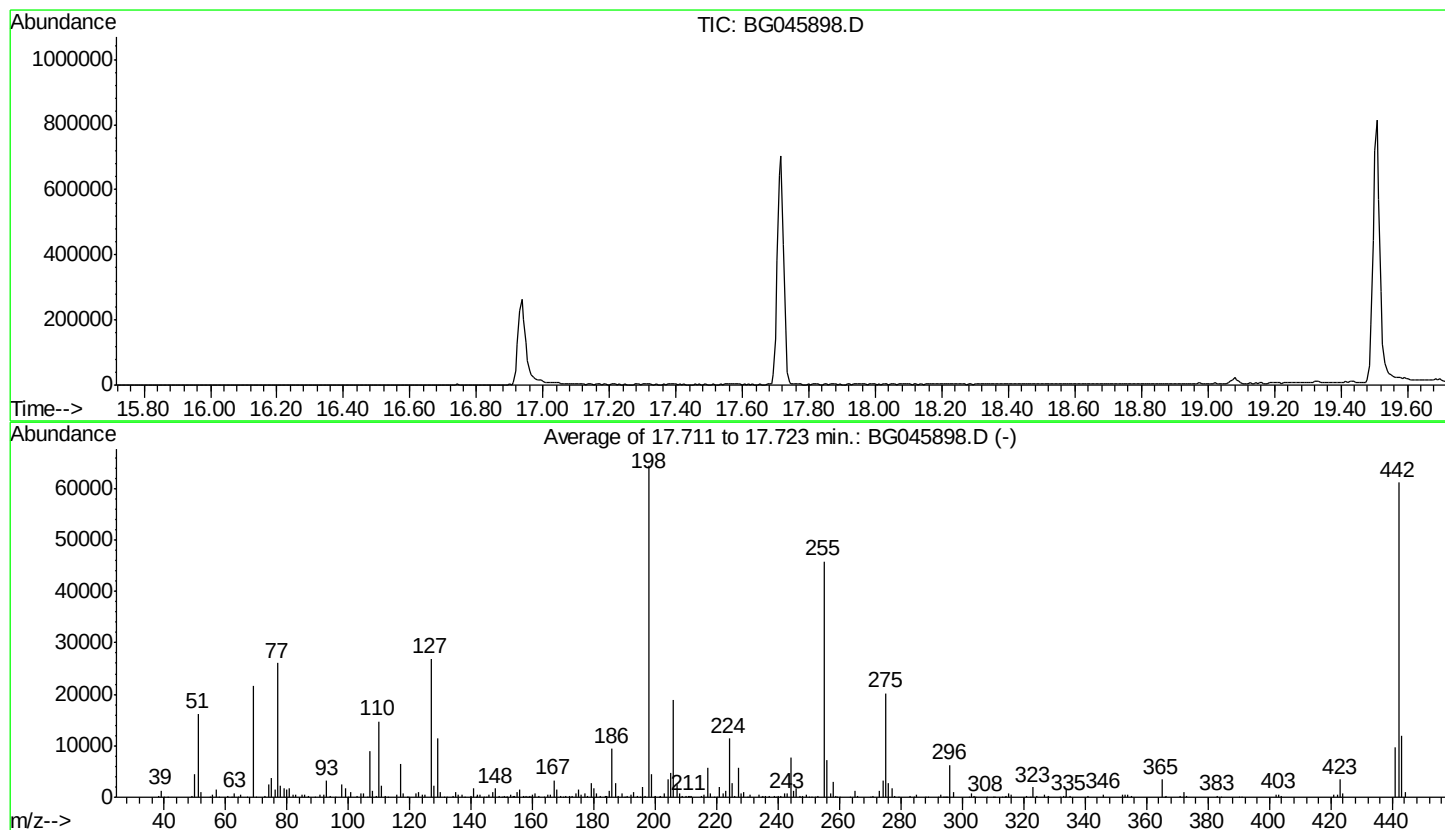

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.2	16205	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.6	21613	PASS
70	69	0.00	2	0.6	126	PASS
127	198	10	80	41.8	26936	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64410	PASS
199	198	5	9	6.8	4376	PASS
275	198	10	60	31.4	20193	PASS
365	198	1	100	5.3	3427	PASS
441	198	0.01	100	14.9	9593	PASS
442	198	50	100	94.8	61072	PASS
443	442	15	24	19.6	11977	PASS