




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070124\
Data File : BG061817.D
Acq On : 1 Jul 2024 18:09
Operator : MA/JU
Sample : PB161627BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK627

Manual IntegrationsAPPROVED

Quant Time: Jul 01 22:40:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 27 12:23:53 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/02/2024
Supervised By :mohammad ahmed 07/04/2024

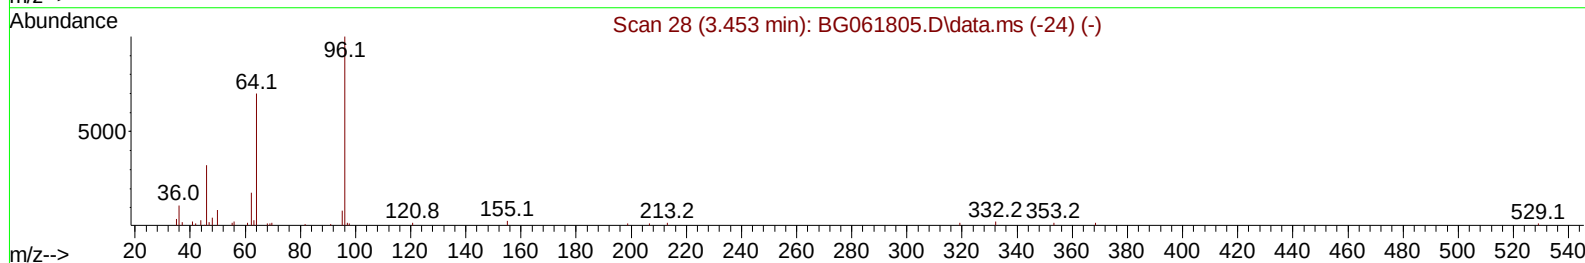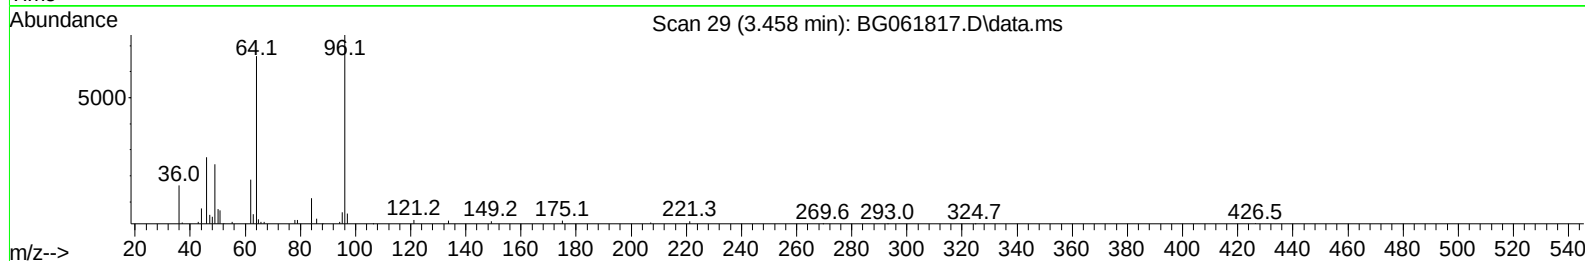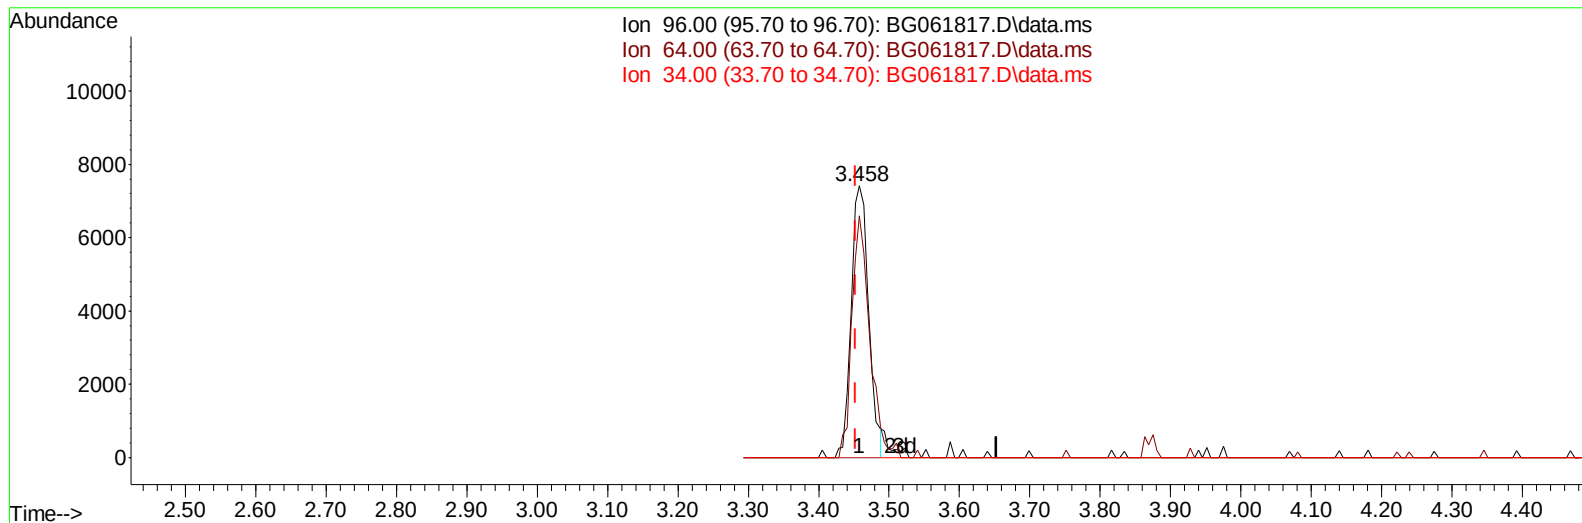

TIC: BG061817.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.458min (+ 0.005) 5.83 ng/uL

response 12682

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	65.50	89.02#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070124\
Data File : BG061817.D
Acq On : 1 Jul 2024 18:09
Operator : MA/JU
Sample : PB161627BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK627

Manual IntegrationsAPPROVED

Quant Time: Jul 01 22:40:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 27 12:23:53 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/02/2024
Supervised By :mohammad ahmed 07/04/2024

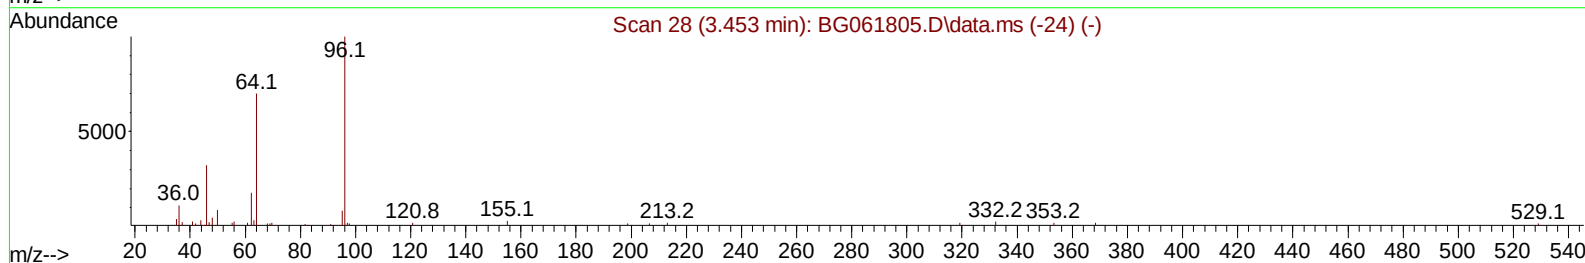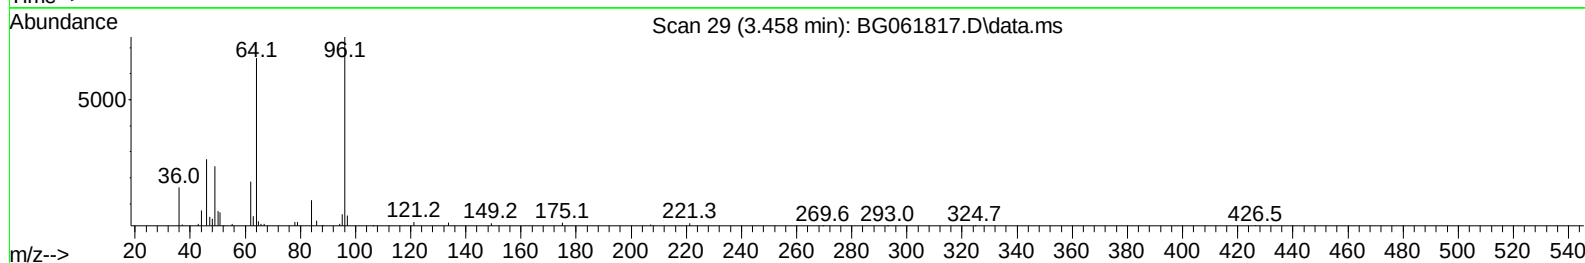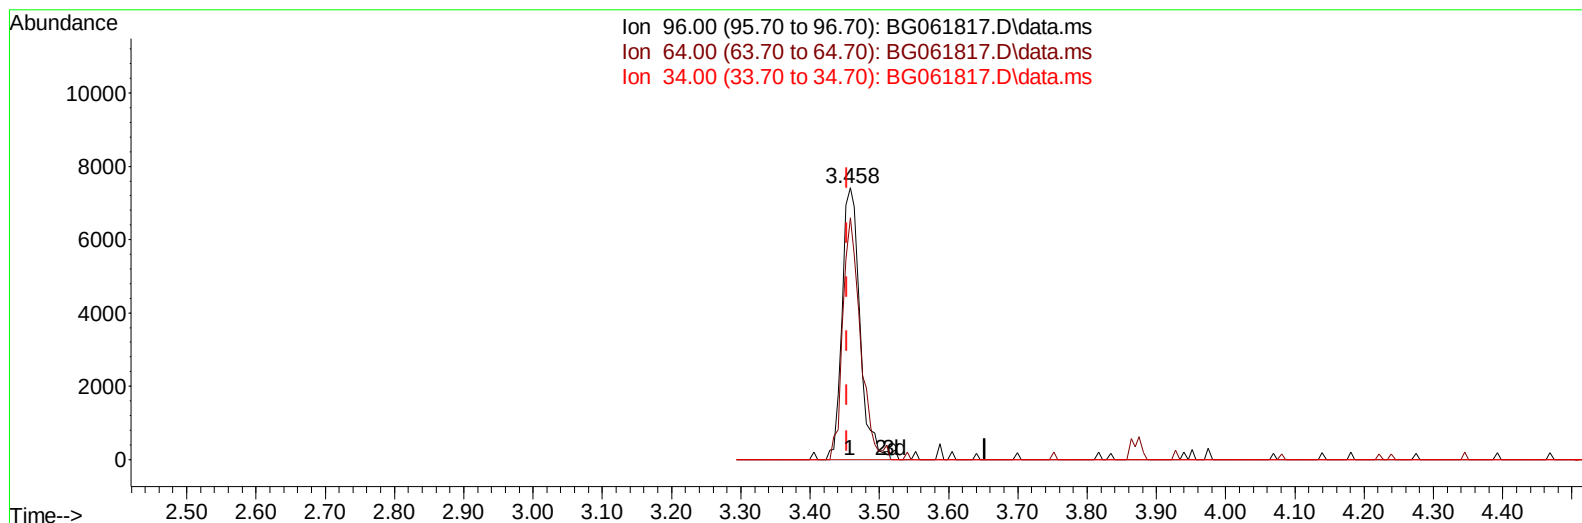

TIC: BG061817.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.458min (+ 0.005) 6.08 ng/uL m

response 13221

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	65.50	89.02#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070124\
 Data File : BG061817.D
 Acq On : 1 Jul 2024 18:09
 Operator : MA/JU
 Sample : PB161627BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK627

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/02/2024
 Supervised By :mohammad ahmed 07/04/2024

Quant Time: Jul 01 22:43:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 27 12:23:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.058	152	78570	20.000	ng/ul	0.00
20) Naphthalene-d8	10.867	136	369691	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.680	164	254119	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.430	188	553668	20.000	ng/ul	0.00
79) Chrysene-d12	21.690	240	439656	20.000	ng/ul	0.00
88) Perylene-d12	24.903	264	523973	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.458	96	13221m	6.079	ng/uL	0.00
4) Pyridine-d5	3.875	84	196264	29.846	ng/ul	0.00
7) Phenol-d5	7.207	99	257307	30.167	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.383	67	151070	28.412	ng/ul	0.00
11) 2-Chlorophenol-d4	7.583	132	175104	29.916	ng/ul	0.00
15) 4-Methylphenol-d8	8.752	113	192056	29.126	ng/ul	0.00
21) Nitrobenzene-d5	9.222	128	90873	36.202	ng/ul	0.00
24) 2-Nitrophenol-d4	9.939	143	104578	41.135	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.485	165	190413	31.631	ng/ul	0.00
31) 4-Chloroaniline-d4	10.996	131	265146	29.092	ng/ul	0.00
46) Dimethylphthalate-d6	14.087	166	598181	30.589	ng/ul	0.00
49) Acenaphthylene-d8	14.380	160	670223	31.273	ng/ul	0.00
54) 4-Nitrophenol-d4	14.868	143	94170	28.039	ng/ul	0.00
60) Fluorene-d10	15.673	176	536396	31.332	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.779	200	61192	25.846	ng/ul	0.00
73) Anthracene-d10	17.524	188	796188	31.504	ng/ul	0.00
81) Pyrene-d10	19.809	212	855406	34.832	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.686	264	828992	33.126	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070124\
Data File : BG061817.D
Acq On : 1 Jul 2024 18:09
Operator : MA/JU
Sample : PB161627BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK627

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/02/2024
Supervised By :mohammad ahmed 07/04/2024

Quant Time: Jul 01 22:43:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 27 12:23:53 2024
Response via : Initial Calibration

