




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070124\
Data File : BG061830.D
Acq On : 2 Jul 2024 2:58
Operator : MA/JU
Sample : P2962-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0T75

Manual IntegrationsAPPROVED

Quant Time: Jul 02 03:43:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 27 12:23:53 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/02/2024
Supervised By :mohammad ahmed 07/04/2024

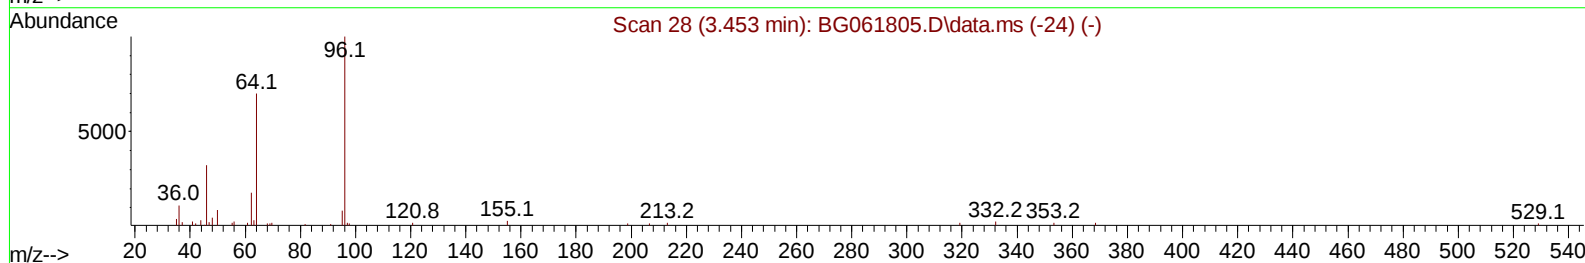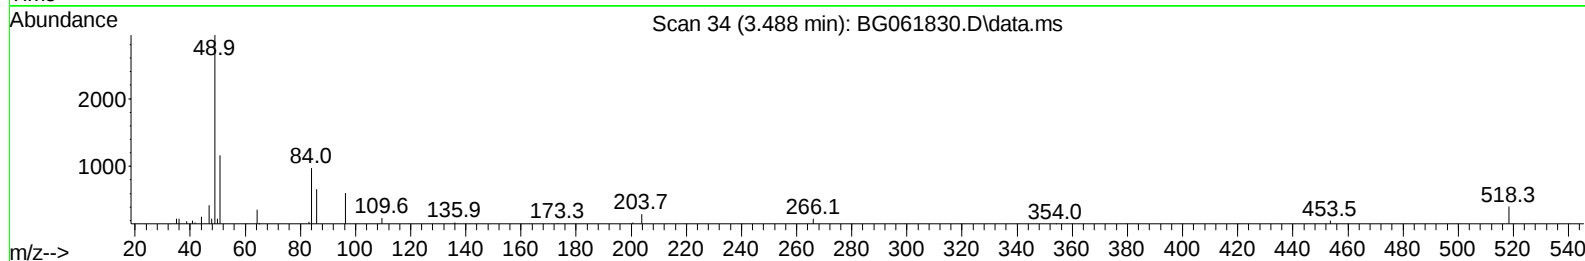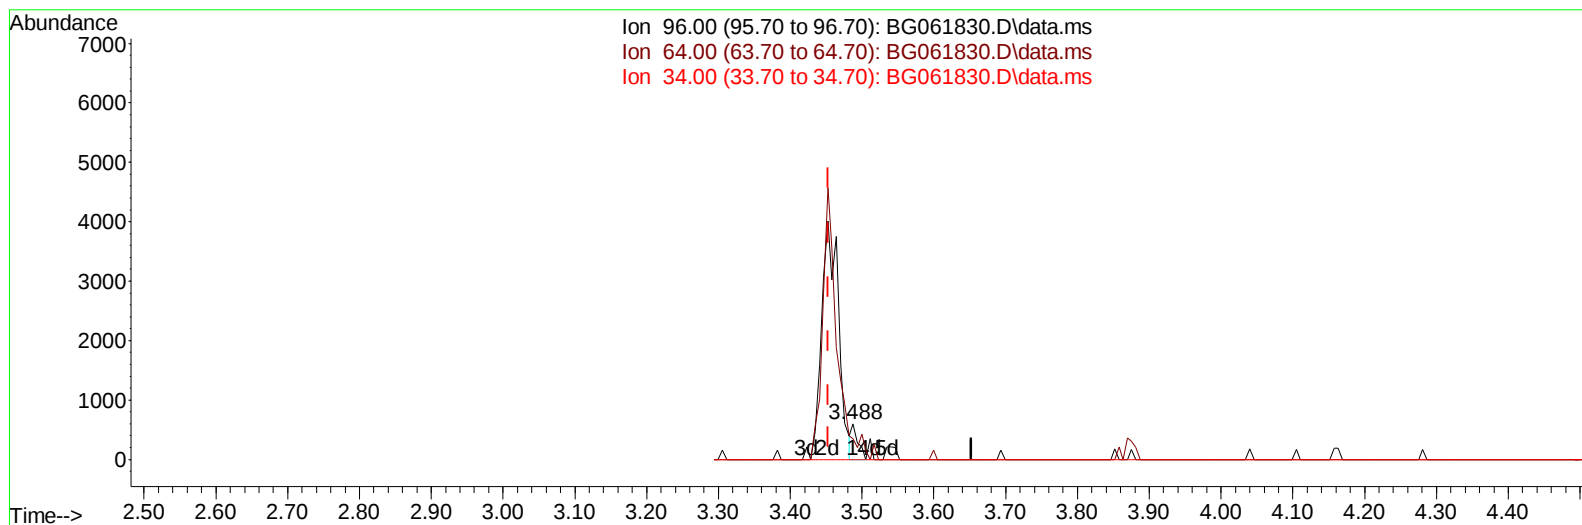

TIC: BG061830.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.488min (+ 0.035) 0.18 ng/uL

response 386

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	65.50	59.04
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070124\
 Data File : BG061830.D
 Acq On : 2 Jul 2024 2:58
 Operator : MA/JU
 Sample : P2962-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0T75

Manual IntegrationsAPPROVED

Quant Time: Jul 02 03:43:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 27 12:23:53 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/02/2024
 Supervised By :mohammad ahmed 07/04/2024

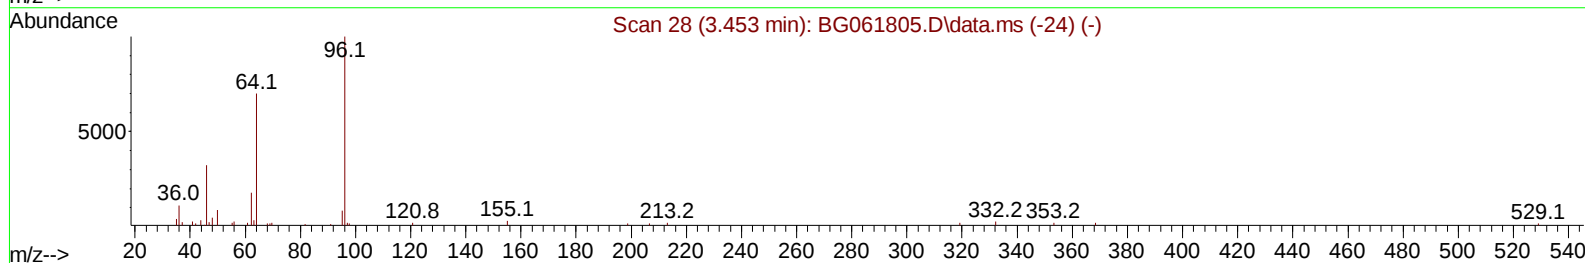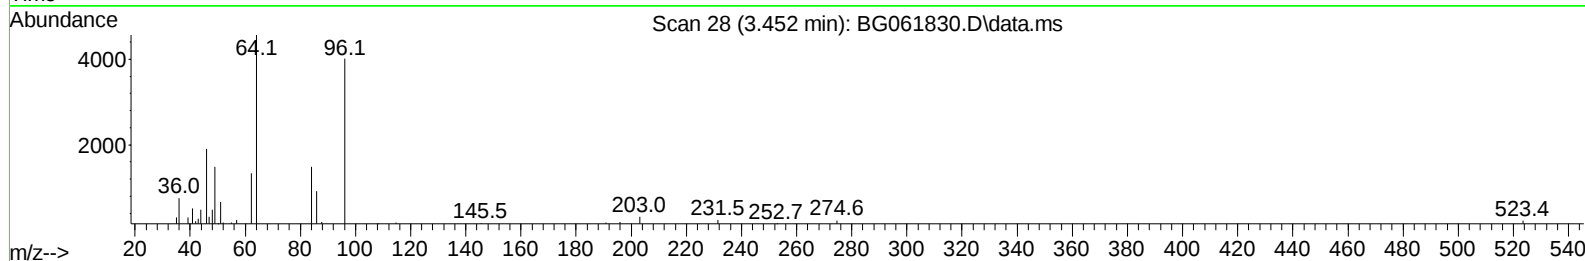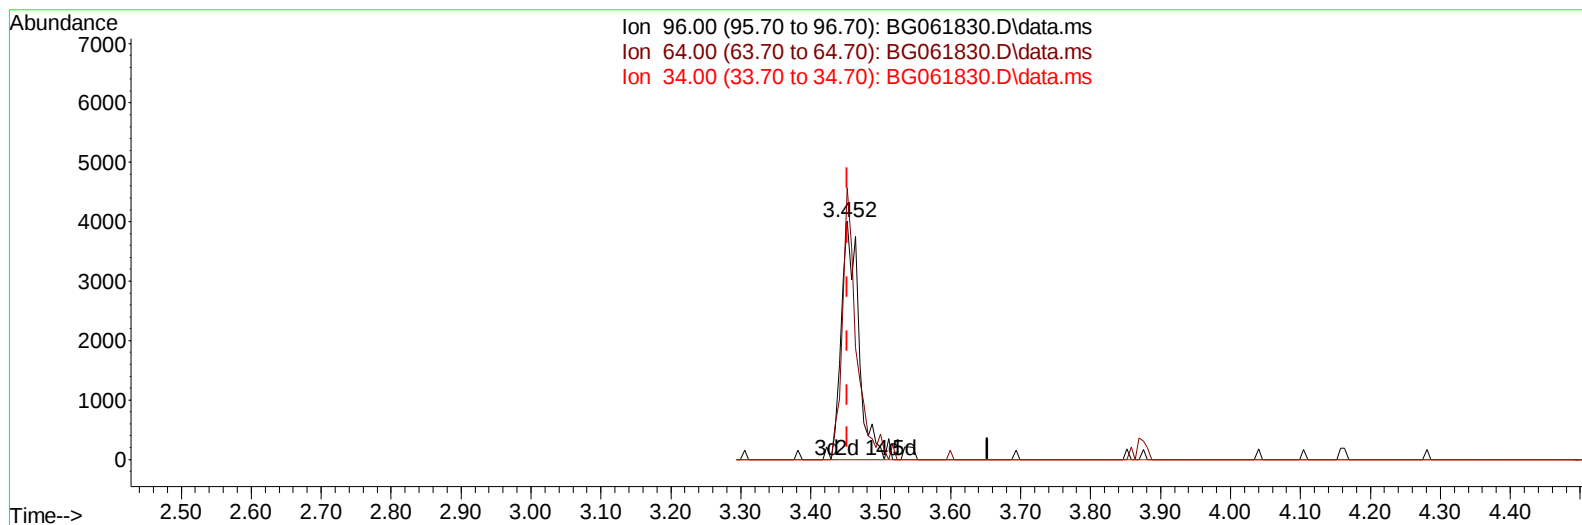

TIC: BG061830.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.452min (-0.000) 3.21 ng/uL m

response 6915

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	65.50	113.91#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070124\
 Data File : BG061830.D
 Acq On : 2 Jul 2024 2:58
 Operator : MA/JU
 Sample : P2962-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0T75

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/02/2024
 Supervised By :mohammad ahmed 07/04/2024

Quant Time: Jul 02 03:44:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 27 12:23:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.053	152	77804	20.000	ng/ul	0.00
20) Naphthalene-d8	10.861	136	375509	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.680	164	250355	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.424	188	556696	20.000	ng/ul	0.00
79) Chrysene-d12	21.684	240	446336	20.000	ng/ul	0.00
88) Perylene-d12	24.898	264	520572	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.452	96	6915m	3.211	ng/uL	0.00
4) Pyridine-d5	3.875	84	112560	17.285	ng/ul	0.00
7) Phenol-d5	7.201	99	168186	19.912	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.377	67	104569	19.860	ng/ul	0.00
11) 2-Chlorophenol-d4	7.583	132	118030	20.364	ng/ul	0.00
15) 4-Methylphenol-d8	8.752	113	134762	20.639	ng/ul	0.00
21) Nitrobenzene-d5	9.216	128	61416	24.088	ng/ul	0.00
24) 2-Nitrophenol-d4	9.939	143	72440	28.052	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.479	165	132435	21.659	ng/ul	0.00
31) 4-Chloroaniline-d4	10.996	131	186384	20.133	ng/ul	0.00
46) Dimethylphthalate-d6	14.087	166	438659	22.769	ng/ul	0.00
49) Acenaphthylene-d8	14.381	160	481343	22.798	ng/ul	0.00
54) 4-Nitrophenol-d4	14.863	143	65679	19.850	ng/ul	0.00
60) Fluorene-d10	15.673	176	388437	23.031	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.779	200	39148	16.445	ng/ul	0.00
73) Anthracene-d10	17.524	188	603528	23.751	ng/ul	0.00
81) Pyrene-d10	19.804	212	651313	26.124	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.675	264	621329	24.990	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070124\
Data File : BG061830.D
Acq On : 2 Jul 2024 2:58
Operator : MA/JU
Sample : P2962-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0T75

Manual IntegrationsAPPROVED

Quant Time: Jul 02 03:44:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 27 12:23:53 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/02/2024
Supervised By :mohammad ahmed 07/04/2024

