

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070124\
 Data File : BG061827.D
 Acq On : 2 Jul 2024 00:56
 Operator : MA/JU
 Sample : P2962-20
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0T98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061827.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.456	24	28	34	rVB3	15343	22399	1.50%	0.117%
2	3.726	69	74	79	rBV	27828	47793	3.21%	0.250%
3	3.873	96	99	113	rVV	155684	295722	19.86%	1.544%
4	4.214	155	157	162	rVB3	5577	6453	0.43%	0.034%
5	4.543	210	213	215	rVB4	3768	3502	0.24%	0.018%
6	4.590	220	221	224	rVB3	4215	3702	0.25%	0.019%
7	4.784	250	254	258	rVB3	4259	4796	0.32%	0.025%
8	5.130	307	313	317	rBV4	8617	15513	1.04%	0.081%
9	5.371	350	354	357	rVB4	2737	4393	0.30%	0.023%
10	6.117	475	481	488	rVB4	12029	21105	1.42%	0.110%
11	6.300	510	512	513	rBV2	4822	3641	0.24%	0.019%
12	6.352	518	521	523	rBV4	3624	4620	0.31%	0.024%
13	6.881	605	611	613	rBV4	2699	4163	0.28%	0.022%
14	7.063	639	642	646	rVB6	3185	4298	0.29%	0.022%
15	7.204	657	666	672	rBV	267458	480900	32.30%	2.511%
16	7.381	688	696	702	rVV	177293	306761	20.60%	1.602%
17	7.475	710	712	715	rBV2	3858	3254	0.22%	0.017%
18	7.504	715	717	723	rVB2	2727	3583	0.24%	0.019%
19	7.580	723	730	736	rBV2	250307	431617	28.99%	2.254%
20	7.633	736	739	742	rVB2	11740	15353	1.03%	0.080%
21	7.898	780	784	786	rVB3	2971	3425	0.23%	0.018%
22	7.939	788	791	794	rBV4	3110	4216	0.28%	0.022%
23	8.056	804	811	817	rBV2	283835	494182	33.19%	2.580%
24	8.103	817	819	824	rVB5	5237	7535	0.51%	0.039%
25	8.750	922	929	940	rVB	327297	566599	38.06%	2.958%
26	9.167	996	1000	1002	rBV3	2713	3282	0.22%	0.017%
27	9.220	1002	1009	1017	rVV	252925	456397	30.65%	2.383%
28	9.355	1029	1032	1035	rBV	4778	6181	0.42%	0.032%
29	9.555	1063	1066	1069	rBV3	3832	4202	0.28%	0.022%
30	9.766	1097	1102	1109	rVV3	23812	42526	2.86%	0.222%
31	9.942	1124	1132	1139	rBV	219044	399180	26.81%	2.084%
32	10.095	1153	1158	1161	rBV	1851	3460	0.23%	0.018%
33	10.160	1164	1169	1172	rBV4	4244	8088	0.54%	0.042%
34	10.289	1189	1191	1193	rVB3	4259	3601	0.24%	0.019%
35	10.312	1193	1195	1196	rBV	4695	3433	0.23%	0.018%
36	10.477	1216	1223	1232	rBV2	336150	574598	38.59%	3.000%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070124\
 Data File : BG061827.D
 Acq On : 2 Jul 2024 00:56
 Operator : MA/JU
 Sample : P2962-20
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COT98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

37	10.865	1281	1289	1297	rBV	441035	764667	51.36%	3.992%
38	10.994	1302	1311	1319	rBV	343816	619307	41.60%	3.233%
39	11.329	1365	1368	1371	rBV2	3049	3564	0.24%	0.019%
40	11.382	1371	1377	1386	rBV6	12459	23155	1.56%	0.121%
41	11.464	1389	1391	1393	rBV2	4531	4574	0.31%	0.024%
42	11.558	1404	1407	1408	rBV2	3273	3291	0.22%	0.017%
43	11.593	1408	1413	1420	rVV3	52862	98549	6.62%	0.515%
44	12.334	1536	1539	1542	rVB2	2721	3562	0.24%	0.019%
45	12.445	1551	1558	1563	rBV4	5450	11884	0.80%	0.062%
46	12.586	1580	1582	1586	rVV2	3363	3507	0.24%	0.018%
47	12.616	1586	1587	1592	rVV3	2979	3787	0.25%	0.020%
48	13.027	1654	1657	1659	rBV2	3254	4279	0.29%	0.022%
49	13.285	1698	1701	1707	rVV4	3345	6960	0.47%	0.036%
50	13.350	1711	1712	1717	rVV3	2390	3320	0.22%	0.017%
51	13.497	1732	1737	1740	rVV	5473	7020	0.47%	0.037%
52	13.791	1784	1787	1790	rVB3	2851	3448	0.23%	0.018%
53	14.085	1830	1837	1846	rBV	600047	858253	57.65%	4.481%
54	14.320	1873	1877	1880	rBV4	9126	12866	0.86%	0.067%
55	14.378	1880	1887	1895	rVB2	623771	988791	66.41%	5.163%
56	14.684	1931	1939	1945	rBV	680996	1041947	69.98%	5.440%
57	14.866	1963	1970	1977	rBV	307121	492241	33.06%	2.570%
58	14.954	1984	1985	1987	rBV2	4916	3237	0.22%	0.017%
59	15.048	2000	2001	2005	rBV2	3888	4147	0.28%	0.022%
60	15.089	2005	2008	2011	rVV3	3698	5246	0.35%	0.027%
61	15.465	2070	2072	2077	rBV5	3557	6039	0.41%	0.032%
62	15.518	2077	2081	2083	rVB4	6056	5830	0.39%	0.030%
63	15.548	2085	2086	2089	rBV2	4912	4946	0.33%	0.026%
64	15.624	2096	2099	2101	rBV2	3397	3646	0.24%	0.019%
65	15.671	2101	2107	2115	rVB	817319	1219576	81.91%	6.368%
66	15.730	2115	2117	2120	rBV4	2742	3735	0.25%	0.020%
67	15.783	2120	2126	2131	rBV2	159240	239739	16.10%	1.252%
68	15.877	2139	2142	2143	rBV2	4000	4801	0.32%	0.025%
69	16.023	2163	2167	2168	rBV3	3548	3884	0.26%	0.020%
70	16.041	2168	2170	2173	rVV3	4434	3666	0.25%	0.019%
71	16.082	2175	2177	2180	rVV3	4375	3477	0.23%	0.018%
72	16.376	2224	2227	2232	rVB4	7309	10465	0.70%	0.055%
73	16.452	2238	2240	2242	rVB3	4449	3305	0.22%	0.017%
74	16.540	2253	2255	2259	rBV5	3722	5440	0.37%	0.028%
75	17.011	2334	2335	2338	rBV	3692	3567	0.24%	0.019%
76	17.169	2361	2362	2365	rBV3	4710	3921	0.26%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070124\
 Data File : BG061827.D
 Acq On : 2 Jul 2024 00:56
 Operator : MA/JU
 Sample : P2962-20
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0T98

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

77	17.328	2386	2389	2390	rBV2	3220	3285	0.22%	0.017%
78	17.381	2395	2398	2399	rBV2	4253	3504	0.24%	0.018%
79	17.428	2399	2406	2415	rVB	836074	1247930	83.82%	6.516%
80	17.522	2415	2422	2430	rBV2	863580	1348447	90.57%	7.040%
81	17.598	2432	2435	2440	rVB8	5745	8494	0.57%	0.044%
82	17.669	2442	2447	2450	rBV7	11823	19037	1.28%	0.099%
83	17.774	2461	2465	2466	rBV3	3518	3361	0.23%	0.018%
84	17.921	2486	2490	2491	rBV4	3842	4771	0.32%	0.025%
85	18.086	2517	2518	2521	rVB2	8738	4573	0.31%	0.024%
86	18.133	2524	2526	2527	rVB2	6856	3832	0.26%	0.020%
87	18.150	2527	2529	2530	rBV2	4413	3749	0.25%	0.020%
88	18.303	2552	2555	2560	rBV6	21044	31391	2.11%	0.164%
89	18.421	2573	2575	2579	rBV3	4435	3231	0.22%	0.017%
90	18.491	2585	2587	2590	rBV4	4003	5975	0.40%	0.031%
91	19.132	2694	2696	2697	rBV2	5067	3235	0.22%	0.017%
92	19.443	2745	2749	2753	rBV3	14650	23598	1.58%	0.123%
93	19.496	2756	2758	2760	rVB3	7733	5732	0.38%	0.030%
94	19.719	2794	2796	2801	rBV5	12570	19487	1.31%	0.102%
95	19.807	2804	2811	2817	rBV	1027073	1488845	100.00%	7.773%
96	20.130	2865	2866	2868	rVB2	10478	5124	0.34%	0.027%
97	21.335	3067	3071	3076	rBV	103948	137794	9.26%	0.719%
98	21.682	3124	3130	3140	rBV2	727098	1210353	81.29%	6.319%
99	24.672	3631	3639	3652	rVB2	527338	1435968	96.45%	7.497%
100	24.901	3670	3678	3695	rVB	474897	1369143	91.96%	7.148%




Sum of corrected areas: 19152971

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070124\
Data File : BG061827.D
Acq On : 2 Jul 2024 00:56
Operator : MA/JU
Sample : P2962-20
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0T98

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

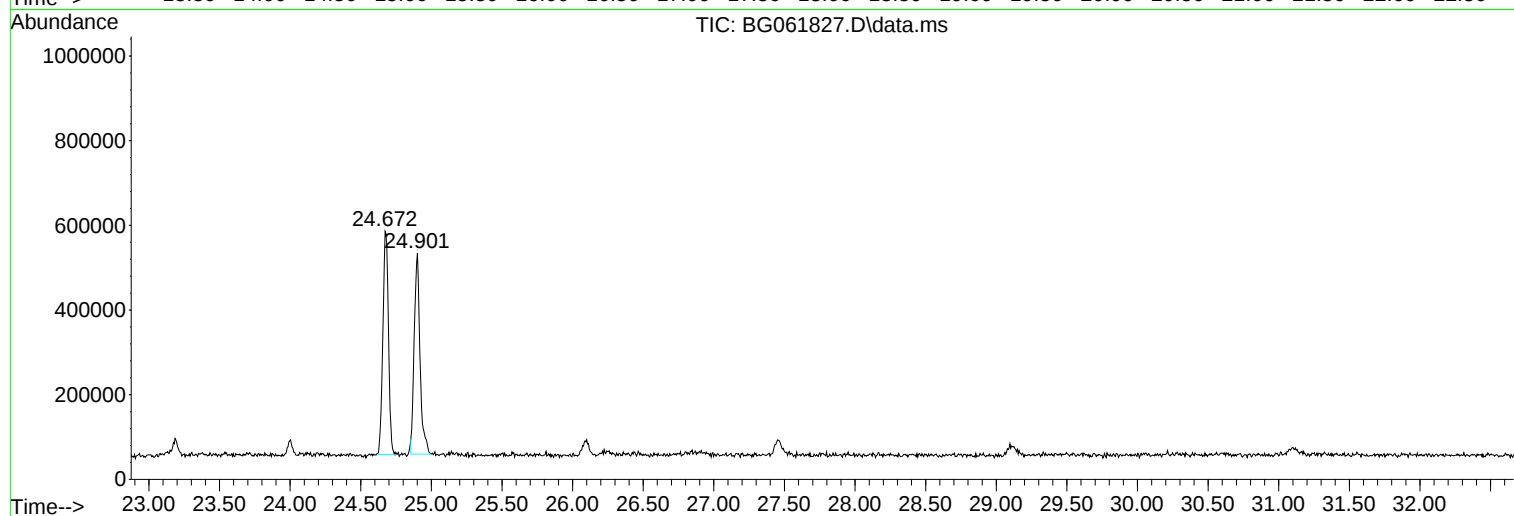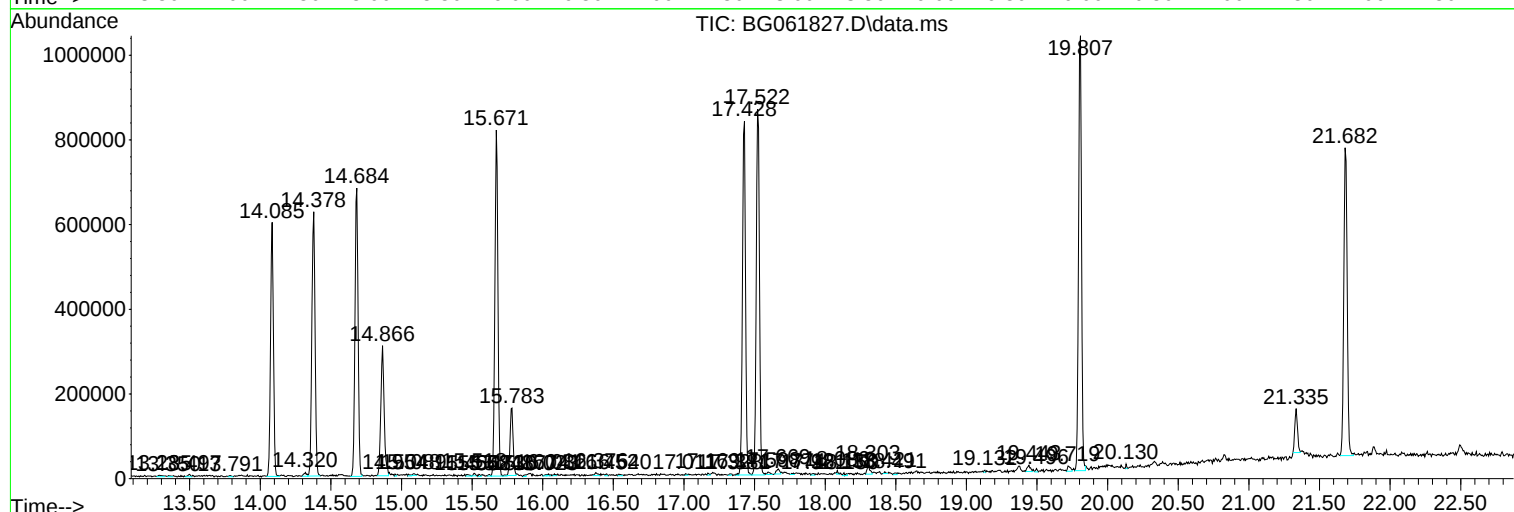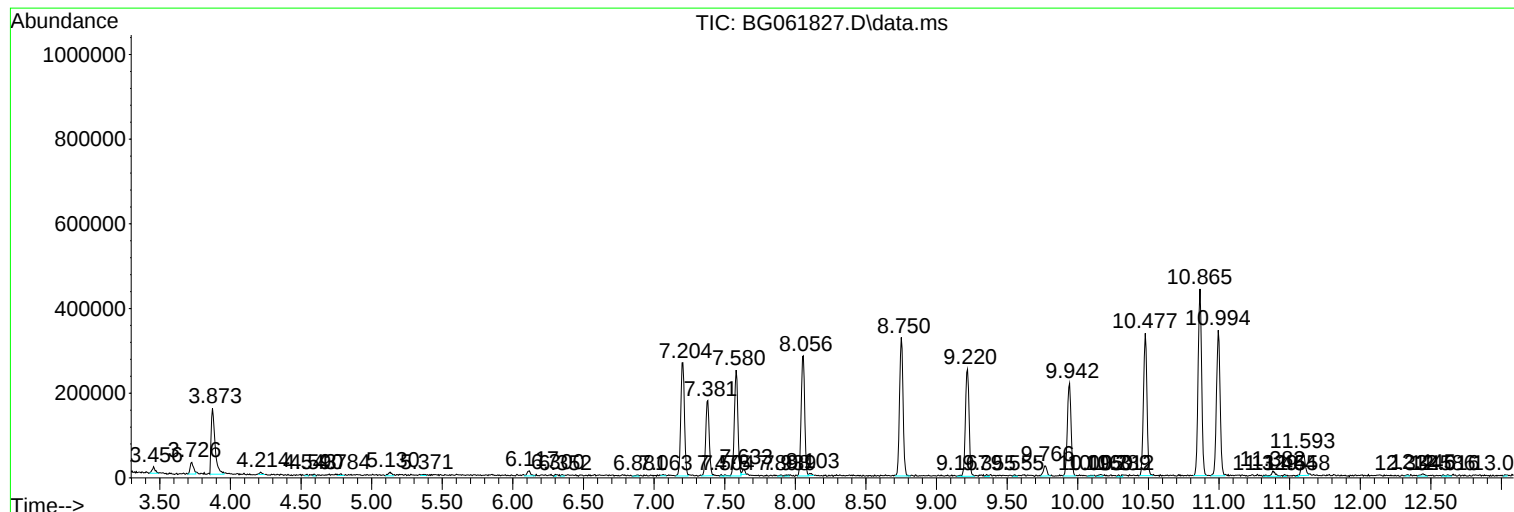

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070124\
Data File : BG061827.D
Acq On : 2 Jul 2024 00:56
Operator : MA/JU
Sample : P2962-20
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COT98










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Phenoxypropan-2-ol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.593	2.58 ng/ul	98549	Naphthalene-d8	10.865

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Phenoxypropan-2-ol	152	C9H12O2	000770-35-4	95
2			1-Phenoxypropan-2-ol	152	C9H12O2	000770-35-4	94
3			1-Phenoxypropan-2-ol	152	C9H12O2	000770-35-4	90
4			1-Phenoxypropan-2-ol	152	C9H12O2	000770-35-4	90
5			1-Propanol, 3-phenoxy-	152	C9H12O2	006180-61-6	78

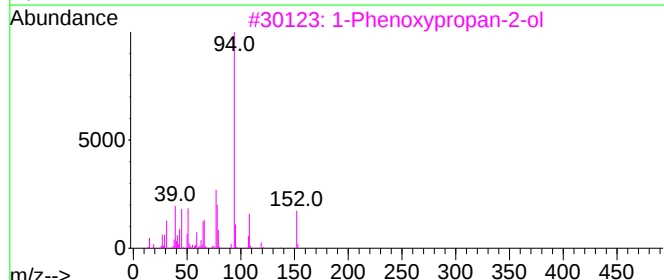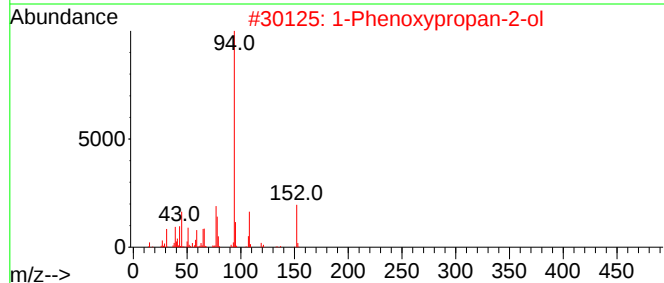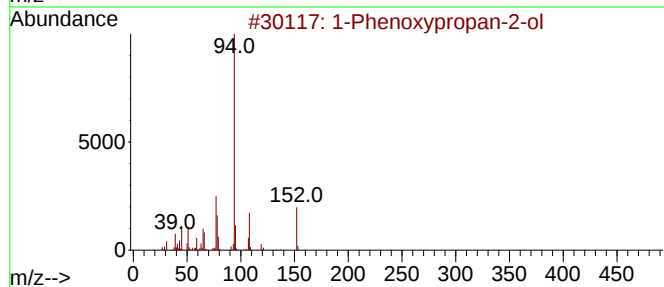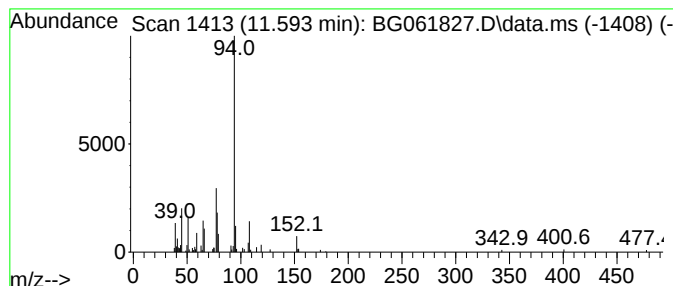

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070124\
Data File : BG061827.D
Acq On : 2 Jul 2024 00:56
Operator : MA/JU
Sample : P2962-20
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COT98










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Cyclic21.335 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.335	2.28 ng/ul	137794	Chrysene-d12	21.682

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclotetracosane	336	C24H48	000297-03-0	96
2			5-Octadecene, (E)-	252	C18H36	007206-21-5	91
3			Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	87
4			Trichloroacetic acid, tetradecyl...	358	C16H29Cl3O2	074339-52-9	83
5			1-Tetracosene	336	C24H48	010192-32-2	83

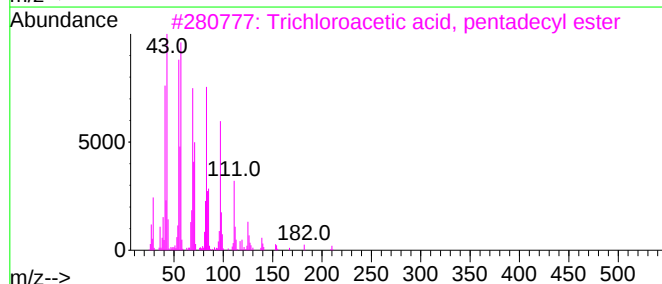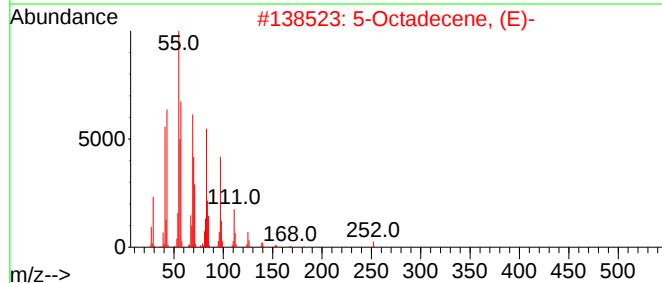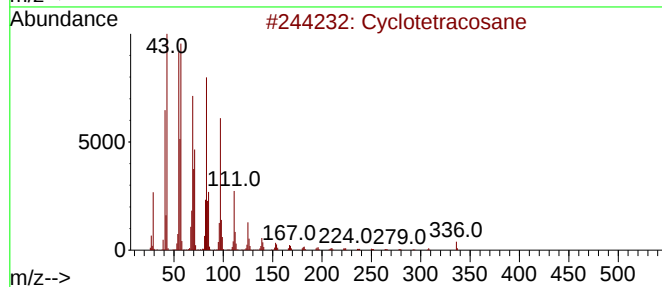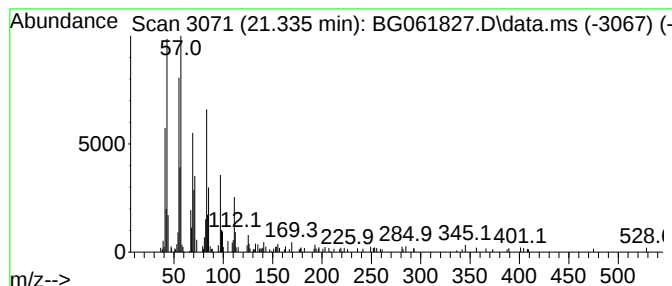

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070124\
Data File : BG061827.D
Acq On : 2 Jul 2024 00:56
Operator : MA/JU
Sample : P2962-20
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0T98

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Phenoxypropan...	11.593	2.6	ng/u1	98549	2	10.865	764667	20.0
(DEL) Alkane: C...	21.335	2.3	ng/u1	137794	5	21.682	1210350	20.0