

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070216\
 Data File : BG022814.D
 Acq On : 3 Jul 2016 4:28
 Operator : UM/SJ
 Sample : H3818-18
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHW7

Quant Time: Jul 04 00:43:20 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 04 00:41:24 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	164429	20.00	ng/ul	0.00
18) Naphthalene-d8	10.98	136	781821	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.80	164	622852	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.55	188	1476632	20.00	ng/ul	0.00
75) Chrysene-d12	21.85	240	1670261	20.00	ng/ul	0.00
83) Perylene-d12	25.23	264	1730353	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.54	96	5211	1.77	ng/uL	0.00
5) Phenol-d5	7.30	99	357447	20.67	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.48	67	237767	24.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	245193	21.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	292389	21.76	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	136443	21.89	ng/ul	0.00
22) 2-Nitrophenol-d4	10.05	143	152769	20.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	310782	19.76	ng/ul	0.00
29) 4-Chloroaniline-d4	11.11	131	373339	28.04	ng/ul	0.00
43) Dimethylphthalate-d6	14.19	166	1152933	22.78	ng/ul	0.00
46) Acenaphthylene-d8	14.49	160	1279036	22.06	ng/ul	0.00
51) 4-Nitrophenol-d4	14.99	143	154407	19.43	ng/ul	0.00
57) Fluorene-d10	15.79	176	1065767	22.23	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	176402	18.57	ng/ul	0.00
70) Anthracene-d10	17.65	188	1591439	23.19	ng/ul	0.00
76) Pyrene-d10	19.93	212	1888104	23.66	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.99	264	1956849	23.80	ng/ul	0.00

Target Compounds


						Ovalue
6) Phenol	7.33	94	19490	1.10	ng/ul#	37
44) Dimethylphthalate	14.24	163	630962	12.21	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070216\
Data File : BG022814.D
Acq On : 3 Jul 2016 4:28
Operator : UM/SJ
Sample : H3818-18
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDHW7

Quant Time: Jul 04 00:43:20 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 04 00:41:24 2016
Response via : Initial Calibration

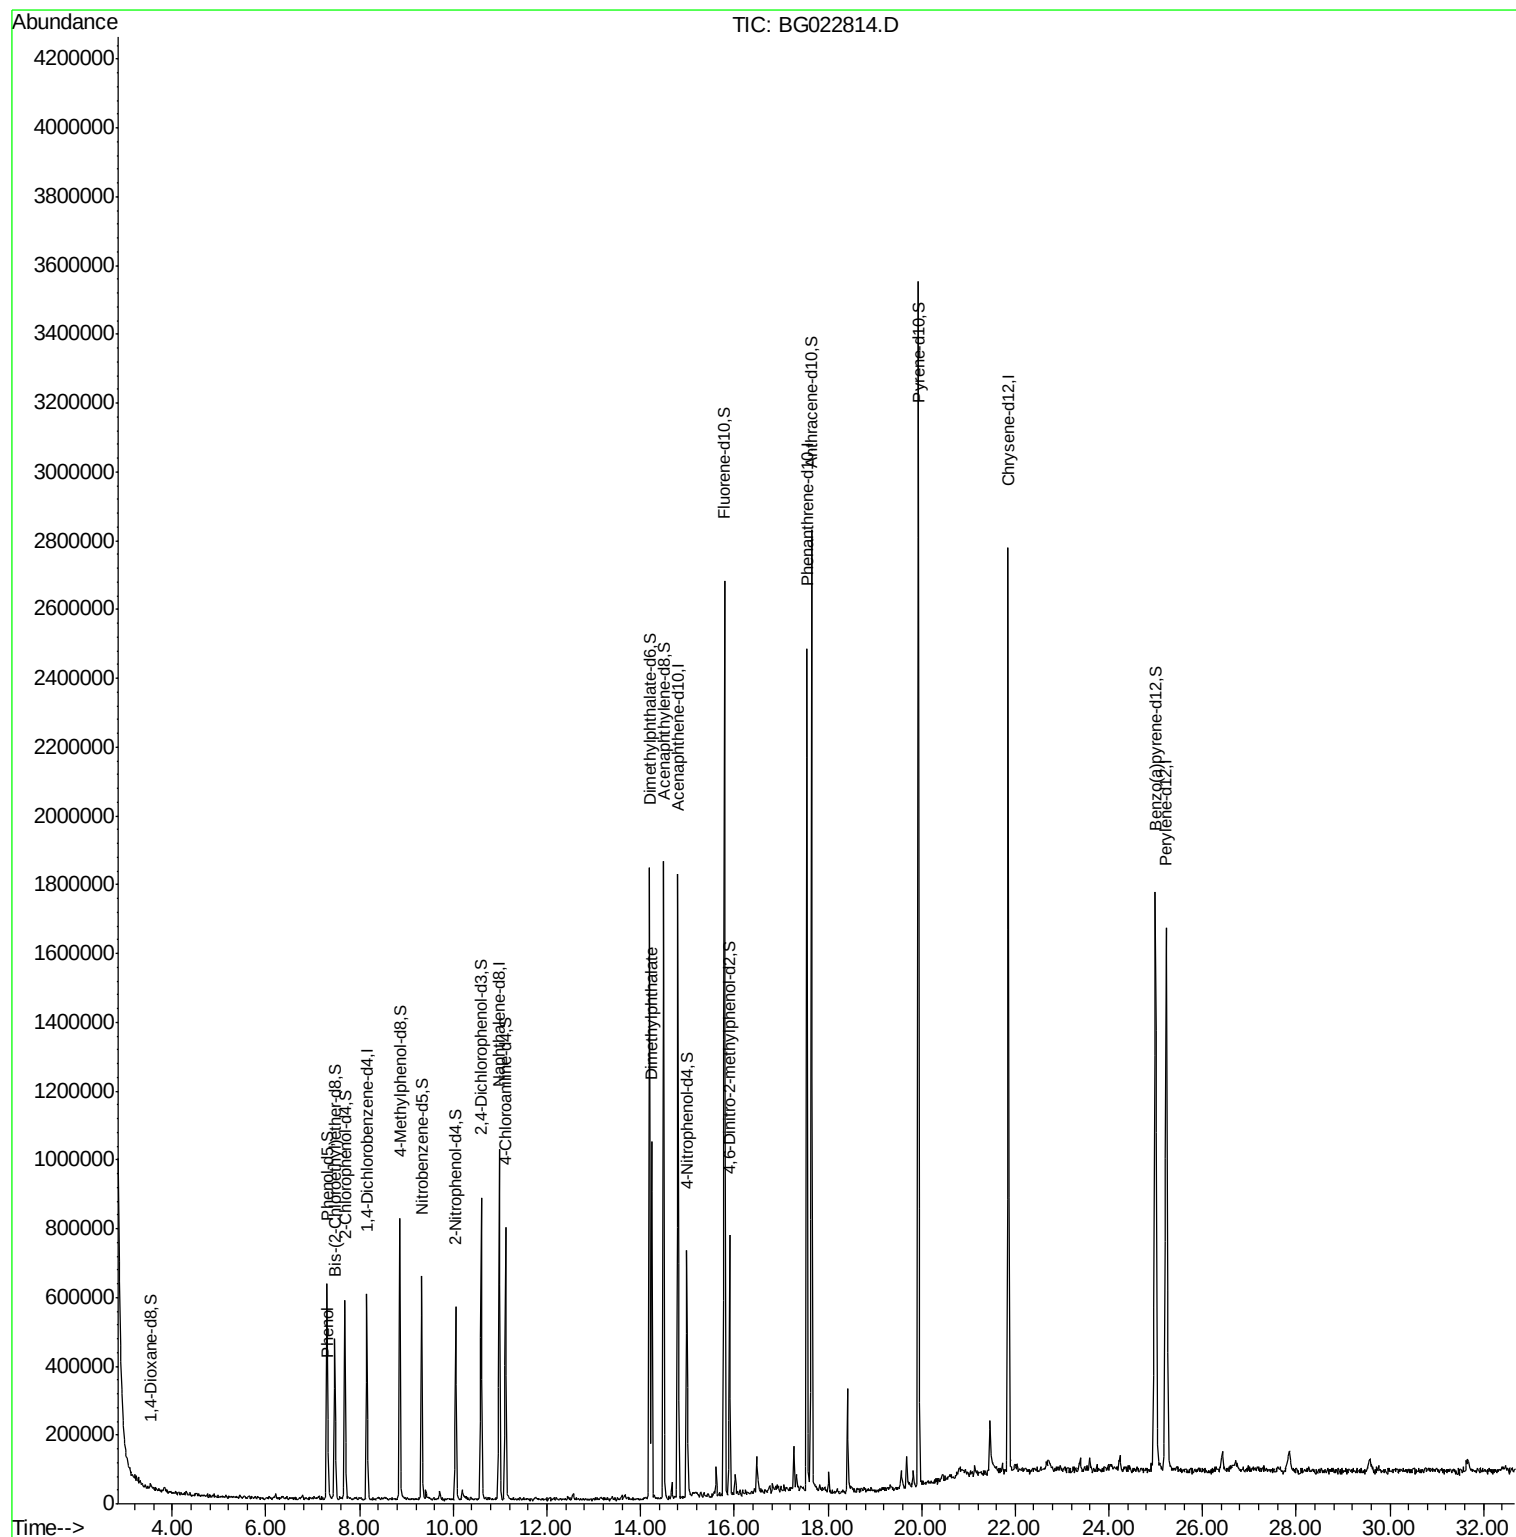

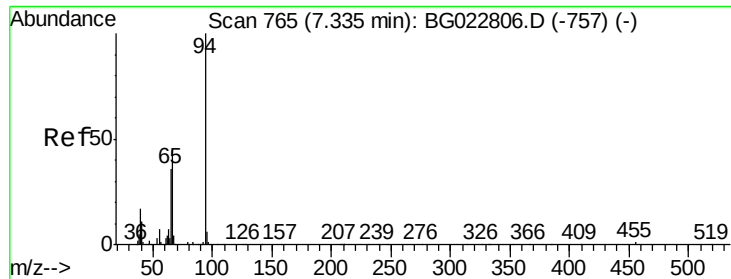

#6

Phenol

Concen: 1.10 ng/ul

RT: 7.33 min Scan# 764

Delta R.T. -0.01 min

Lab File: BG022814.D

Acq: 3 Jul 2016 4:28

Instrument :

BNA_G

ClientSampleId :

BDHW7


Tot Ion: 94 Resp: 19490

Ion Ratio Lower Upper




94 100

65 40.3 16.8 25.2#

66 69.8 22.6 33.8#

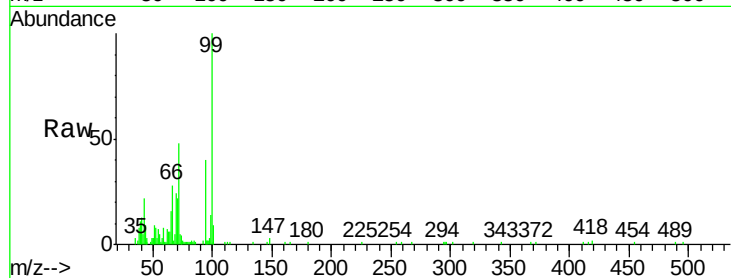

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

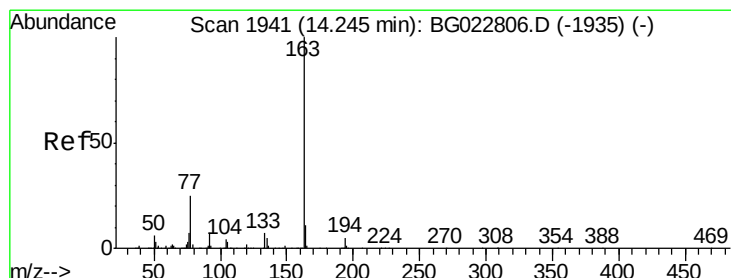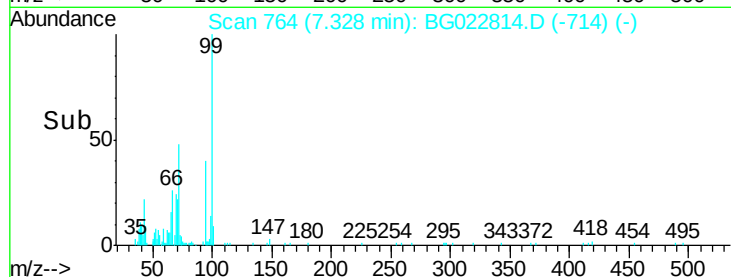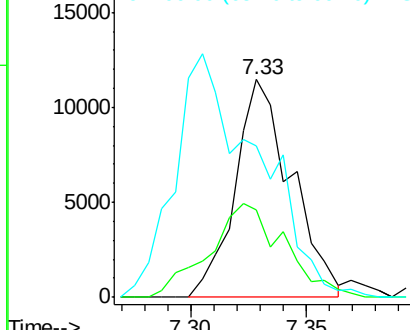

#44

Dimethylphthalate

Concen: 12.21 ng/ul

RT: 14.24 min Scan# 1940

Delta R.T. -0.01 min

Lab File: BG022814.D

Acq: 3 Jul 2016 4:28


Tgt Ion:163 Resp: 630962

Ion Ratio Lower Upper

163 100

194 4.7 3.4 5.2

164 11.4 8.8 13.2

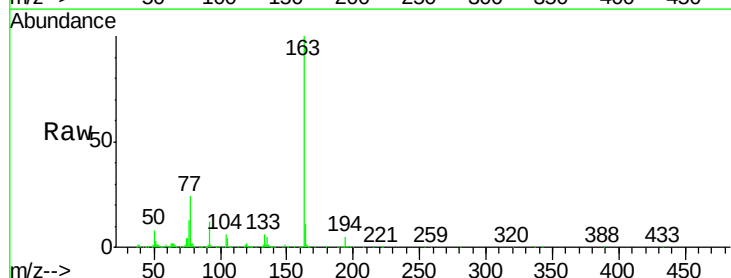

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

