

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA G\DATA\BG070216\
 Data File : BG022797.D
 Acq On : 2 Jul 2016 17:08
 Operator : UM/SJ
 Sample : H3752-15
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHM7

Manual Integration

Quant Time: Jul 03 01:20:49 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 03 00:31:55 2016
 Response via : Initial Calibration

APPROVED
 umangi
 7/5/2016 7:42:13 PM

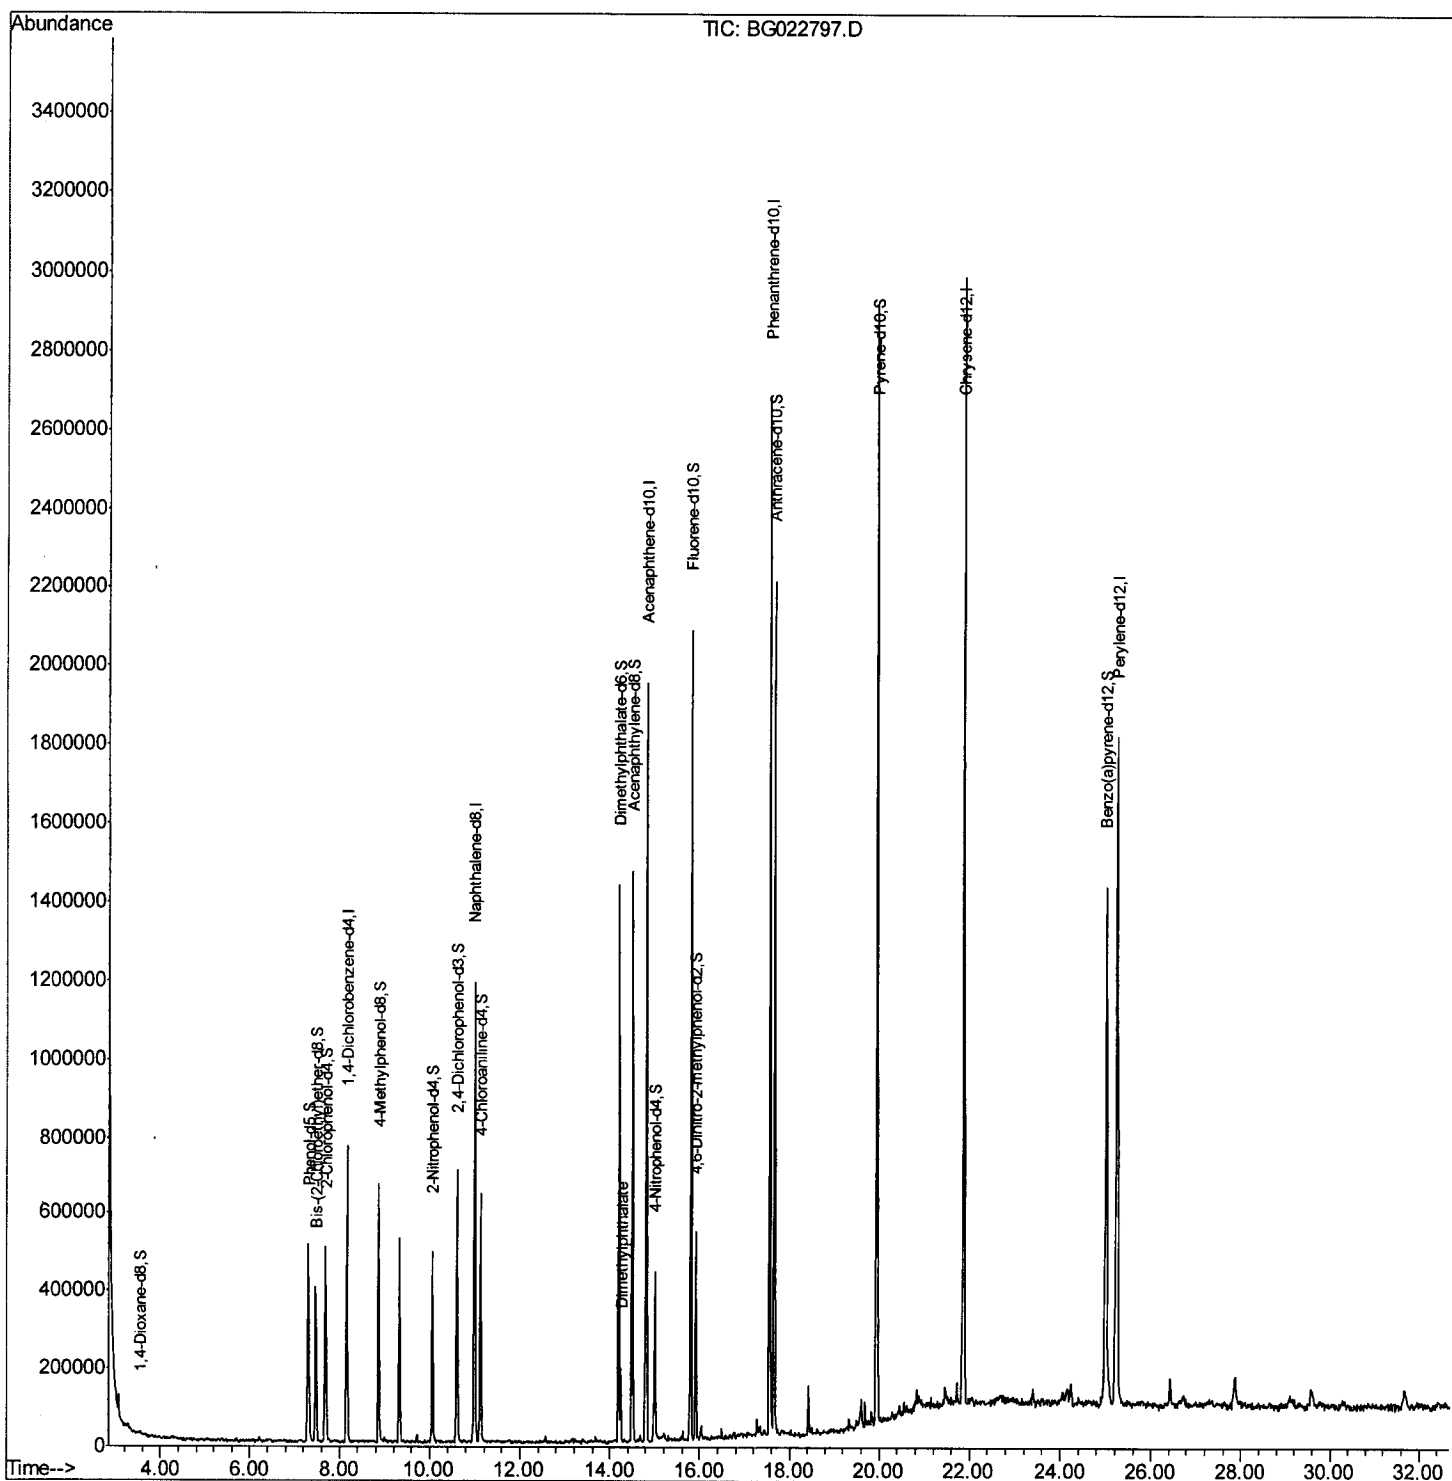

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA G\DATA\BG070216\
 Data File : BG022797.D
 Acq On : 2 Jul 2016 17:08
 Operator : UM/SJ
 Sample : H3752-15
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA G
 ClientSampleId :
 BDHM7

Manual Integration

umangi
 7/5/2016 7:42:13 PM

Quant Time: Jul 03 00:33:27 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 03 00:31:55 2016
 Response via : Initial Calibration

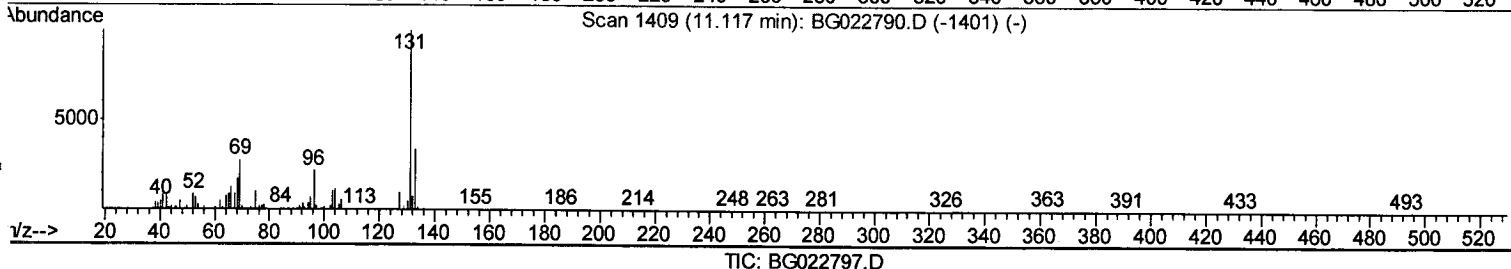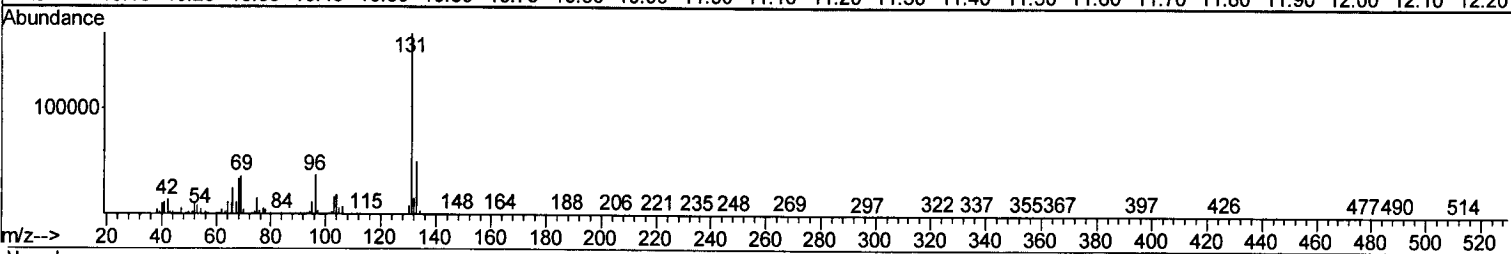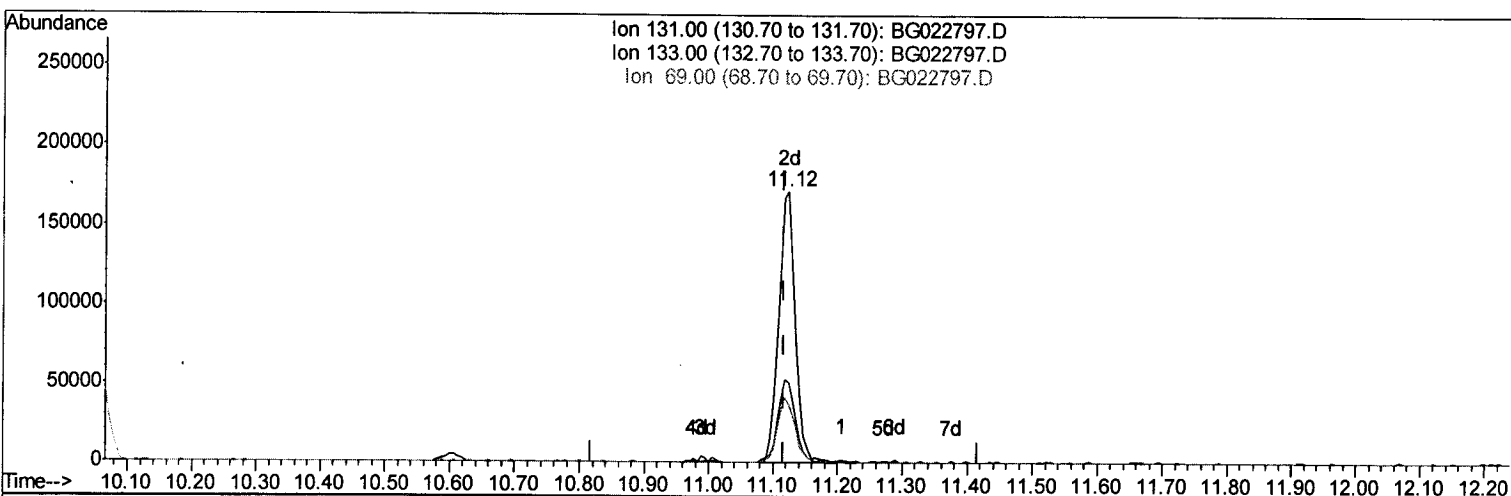

(29) 4-Chloroaniline-d4 (S)

11.123min (+0.006) 20.16ng/ul m U.M

response 311160

Ion	Exp%	Act%
131.00	100	100
133.00	33.10	29.35
69.00	15.40	21.44#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA G\DATA\BG070216\
Data File : BG022797.D
Acq On : 2 Jul 2016 17:08
Operator : UM/SJ
Sample : H3752-15
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDHM7

Quant Time: Jul 03 00:33:27 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 03 00:31:55 2016
Response via : Initial Calibration

Manual Integration

umangi
7/5/2016 7:42:13 PM

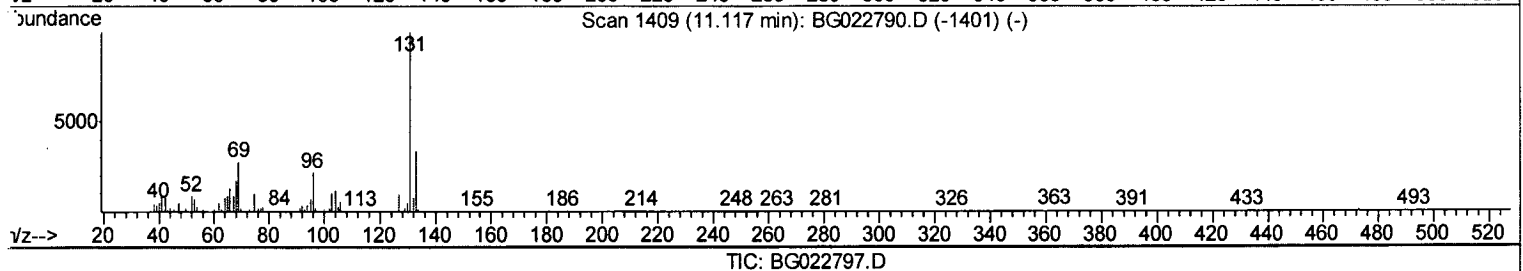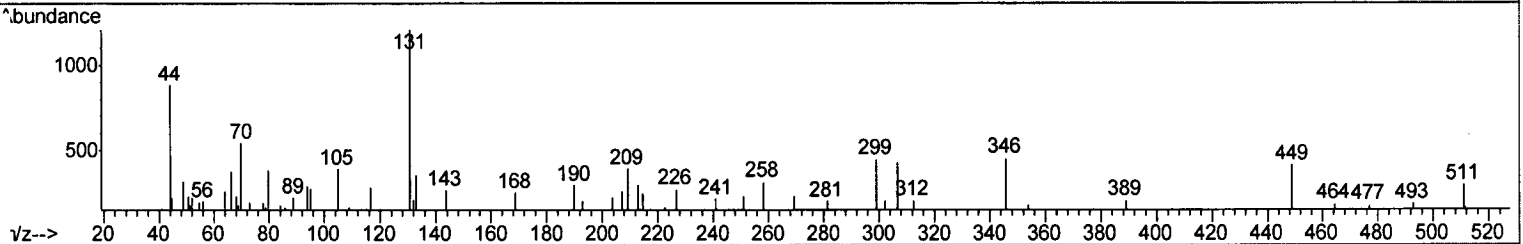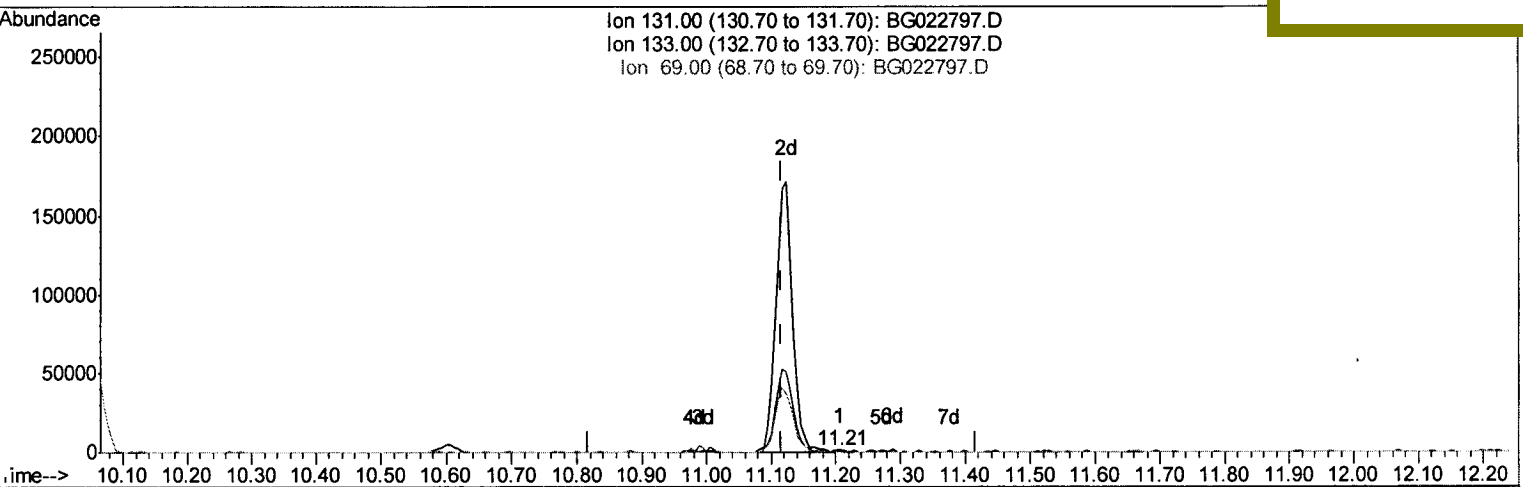

TIC: BG022797.D

(29) 4-Chloroaniline-d4 (S)

11.206min (+0.088) 0.06ng/ul

response 944

Ion	Exp%	Act%
131.00	100	100
133.00	33.10	29.26
69.00	15.40	15.04
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070216\
 Data File : BG022797.D
 Acq On : 2 Jul 2016 17:08
 Operator : UM/SJ
 Sample : H3752-15
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHM7

Manual Integration

umangi
 7/5/2016 7:42:13 PM

Quant Time: Jul 03 01:20:49 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 03 00:31:55 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	212586	20.00	ng/ul	0.00
18) Naphthalene-d8	10.99	136	906133	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.80	164	690857	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.56	188	1621786	20.00	ng/ul	0.00
75) Chrysene-d12	21.86	240	1835776	20.00	ng/ul	0.00
83) Perylene-d12	25.24	264	1949346	20.00	ng/ul	0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.54	96	4922	1.29	ng/uL	0.00
5) Phenol-d5	7.31	99	312523	13.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	204432	16.21	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	217152	14.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	231458	13.33	ng/ul	0.00
19) Nitrobenzene-d5	9.46	128	118	0.02	ng/ul	0.13
22) 2-Nitrophenol-d4	10.06	143	134588	15.44	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	264761	14.53	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	311160m	20.16	ng/ul	0.00
43) Dimethylphthalate-d6	14.20	166	925258	16.49	ng/ul	0.00
46) Acenaphthylene-d8	14.50	160	1039010	16.15	ng/ul	0.00
51) 4-Nitrophenol-d4	15.00	143	94690	10.75	ng/ul	0.00
57) Fluorene-d10	15.79	176	873520	16.43	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.91	200	119463	11.45	ng/ul	0.00
70) Anthracene-d10	17.66	188	1245612	16.52	ng/ul	0.00
76) Pyrene-d10	19.94	212	1532298	17.47	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.00	264	1514277	16.35	ng/ul	0.01

Target Compounds				Ovalue
44) Dimethylphthalate	14.24	163	111142	1.94 ng/ul# 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed