

Data Path : U:\HPCHEM1\BNA G\DATA\BG070216\
 Data File : BG022797.D
 Acq On : 2 Jul 2016 17:08
 Operator : UM/SJ
 Sample : H3752-15
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHM7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.891	177	179	182	rVB4	7639	7736	0.15%	0.015%
2	4.302	247	249	253	rBV4	6142	10100	0.20%	0.020%
3	4.419	267	269	271	rVB2	7210	5970	0.12%	0.012%
4	4.461	271	276	279	rVV5	5834	12247	0.24%	0.024%
5	4.508	283	284	286	rBV2	8849	6067	0.12%	0.012%
6	4.549	288	291	293	rVB3	5903	6756	0.13%	0.013%
7	4.672	309	312	314	rBV4	5843	6483	0.13%	0.013%
8	5.054	372	377	379	rBV3	7658	6917	0.13%	0.013%
9	5.213	402	404	406	rBV3	5443	6161	0.12%	0.012%
10	5.506	452	454	456	rBV3	6161	5805	0.11%	0.011%
11	5.712	486	489	490	rBV2	10072	6910	0.13%	0.013%
12	6.211	570	574	581	rBV5	12549	22271	0.43%	0.043%
13	6.358	596	599	603	rBV6	6452	9003	0.17%	0.017%
14	6.781	669	671	674	rVB3	8686	9439	0.18%	0.018%
15	6.822	674	678	680	rVB4	6484	7919	0.15%	0.015%
16	6.864	680	685	687	rBV4	3926	6386	0.12%	0.012%
17	6.958	700	701	706	rVB3	6693	5962	0.12%	0.012%
18	7.016	708	711	714	rBV2	4162	6047	0.12%	0.012%
19	7.110	723	727	729	rBV4	5871	7999	0.16%	0.016%
20	7.310	754	761	775	rVB	506533	1014492	19.71%	1.968%
21	7.475	780	789	800	rBV	397904	705903	13.71%	1.369%
22	7.686	817	825	834	rBV	502306	924693	17.96%	1.793%
23	7.827	846	849	850	rBV3	5008	5937	0.12%	0.012%
24	8.162	898	906	920	rBV	769504	1434911	27.88%	2.783%
25	8.391	943	945	950	rVB6	6131	9917	0.19%	0.019%
26	8.438	950	953	957	rBV4	5602	9547	0.19%	0.019%
27	8.526	964	968	971	rVB5	4795	6178	0.12%	0.012%
28	8.861	1018	1025	1036	rBV	666047	1207808	23.46%	2.343%
29	8.996	1044	1048	1049	rBV4	12281	12159	0.24%	0.024%
30	9.096	1063	1065	1068	rBV3	5618	7303	0.14%	0.014%
31	9.167	1073	1077	1080	rVB5	5171	8453	0.16%	0.016%
32	9.331	1097	1105	1116	rBV	525776	983947	19.12%	1.908%
33	9.725	1164	1172	1175	rBV4	23187	41784	0.81%	0.081%
34	9.784	1180	1182	1186	rVB3	5440	6038	0.12%	0.012%

Data Path : U:\HPCHEM1\BNA G\DATA\BG070216\
 Data File : BG022797.D
 Acq On : 2 Jul 2016 17:08
 Operator : UM/SJ
 Sample : H3752-15
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHM7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
 Title : SVOA CALIBRATION

35	10.060	1222	1229	1237	rBV	489655	900743	17.50%	1.747%
36	10.119	1237	1239	1244	rVB4	11412	11221	0.22%	0.022%
37	10.371	1280	1282	1286	rBV3	6331	9695	0.19%	0.019%
38	10.600	1311	1321	1333	rBV2	702633	1335638	25.95%	2.591%
39	10.753	1342	1347	1348	rBV3	8531	9174	0.18%	0.018%
40	10.841	1359	1362	1365	rBV2	5658	8630	0.17%	0.017%
41	10.988	1379	1387	1399	rBV	1183770	2105870	40.91%	4.084%
42	11.123	1402	1410	1420	rVV	637049	1182773	22.98%	2.294%
43	11.288	1433	1438	1439	rBV4	5049	7064	0.14%	0.014%
44	11.405	1453	1458	1461	rBV4	5381	7111	0.14%	0.014%
45	11.517	1474	1477	1480	rBV4	5062	8069	0.16%	0.016%
46	11.682	1501	1505	1507	rBV	4287	7053	0.14%	0.014%
47	11.752	1514	1517	1519	rBV2	7653	6715	0.13%	0.013%
48	11.899	1539	1542	1544	rVB2	8296	8306	0.16%	0.016%
49	11.987	1552	1557	1563	rBV7	5988	13149	0.26%	0.026%
50	12.210	1594	1595	1599	rVB4	6259	6828	0.13%	0.013%
51	12.451	1633	1636	1639	rBV4	8215	12539	0.24%	0.024%
52	12.563	1650	1655	1662	rVB4	19071	33996	0.66%	0.066%
53	12.657	1669	1671	1673	rBV	6295	6090	0.12%	0.012%
54	12.915	1711	1715	1716	rBV2	6111	7508	0.15%	0.015%
55	13.145	1752	1754	1757	rBV4	8196	11652	0.23%	0.023%
56	13.209	1763	1765	1767	rBV3	12864	8879	0.17%	0.017%
57	13.350	1786	1789	1790	rVB2	8689	7762	0.15%	0.015%
58	13.368	1790	1792	1794	rBV	7518	7582	0.15%	0.015%
59	13.397	1794	1797	1804	rVV8	12918	27088	0.53%	0.053%
60	13.509	1813	1816	1818	rBV4	6711	9191	0.18%	0.018%
61	13.597	1830	1831	1836	rVB5	6900	6995	0.14%	0.014%
62	13.679	1841	1845	1849	rVB5	15501	23001	0.45%	0.045%
63	13.949	1887	1891	1892	rVB3	5623	5900	0.11%	0.011%
64	13.973	1892	1895	1897	rBV2	8111	10501	0.20%	0.020%
65	14.032	1902	1905	1909	rVV4	4869	6972	0.14%	0.014%
66	14.196	1925	1933	1938	rBV	1429558	2172194	42.20%	4.213%
67	14.243	1938	1941	1946	rVV2	189892	268303	5.21%	0.520%
68	14.314	1949	1953	1954	rBV2	6494	7616	0.15%	0.015%
69	14.496	1977	1984	1993	rBV	1463015	2331119	45.29%	4.521%
70	14.678	2011	2015	2023	rVB5	18568	30689	0.60%	0.060%
71	14.807	2027	2037	2047	rBV2	1944896	3350508	65.09%	6.498%

Data Path : U:\HPCHEM1\BNA G\DATA\BG070216\
Data File : BG022797.D
Acq On : 2 Jul 2016 17:08
Operator : UM/SJ
Sample : H3752-15
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDHM7

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Title : SVOA CALIBRATION

72	14.995	2063	2069	2076	rBV2	435988	768687	14.93%	1.491%
73	15.295	2117	2120	2124	rBV6	15494	18690	0.36%	0.036%
74	15.360	2129	2131	2133	rVB3	7738	6962	0.14%	0.014%
75	15.454	2146	2147	2152	rBV5	9382	10597	0.21%	0.021%
76	15.624	2173	2176	2180	rVB3	25090	26486	0.51%	0.051%
77	15.794	2198	2205	2213	rBV	2073760	3223002	62.61%	6.251%
78	15.906	2218	2224	2231	rBV	533439	801563	15.57%	1.555%
79	16.041	2238	2247	2252	rBV5	37320	69425	1.35%	0.135%
80	16.253	2281	2283	2284	rBV2	11175	8796	0.17%	0.017%
81	16.329	2294	2296	2299	rBV4	7248	7891	0.15%	0.015%
82	16.435	2310	2314	2316	rBV4	9622	12689	0.25%	0.025%
83	16.488	2320	2323	2326	rBV5	26721	33598	0.65%	0.065%
84	16.670	2350	2354	2355	rBV3	8998	12142	0.24%	0.024%
85	17.069	2419	2422	2424	rBV4	12274	15962	0.31%	0.031%
86	17.187	2440	2442	2444	rBV3	7471	7349	0.14%	0.014%
87	17.287	2455	2459	2462	rBV2	38143	40723	0.79%	0.079%
88	17.557	2498	2505	2512	rBV2	2647547	4181316	81.23%	8.110%
89	17.657	2516	2522	2534	rVB2	2180787	3327170	64.64%	6.453%
90	18.303	2631	2632	2635	rBV3	9187	7513	0.15%	0.015%
91	18.421	2648	2652	2659	rBV3	127021	192540	3.74%	0.373%
92	19.002	2749	2751	2756	rBV6	10225	14480	0.28%	0.028%
93	19.226	2786	2789	2790	rBV3	13604	15029	0.29%	0.029%
94	19.602	2851	2853	2859	rVB	70491	85843	1.67%	0.166%
95	19.690	2864	2868	2874	rBV8	65256	101889	1.98%	0.198%
96	19.825	2888	2891	2897	rBV4	35901	68296	1.33%	0.132%
97	19.937	2904	2910	2921	rVB	2857698	4174461	81.10%	8.096%
98	21.858	3230	3237	3245	rBV2	2869265	5147353	100.00%	9.983%
99	25.001	3763	3772	3783	rBV2	1299224	3648191	70.88%	7.076%
100	25.242	3802	3813	3827	rVB2	1700943	5020959	97.54%	9.738%


Sum of corrected areas: 51558974

Data Path : U:\HPCHEM1\BNA G\DATA\BG070216\
Data File : BG022797.D
Acq On : 2 Jul 2016 17:08
Operator : UM/SJ
Sample : H3752-15
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDHM7

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

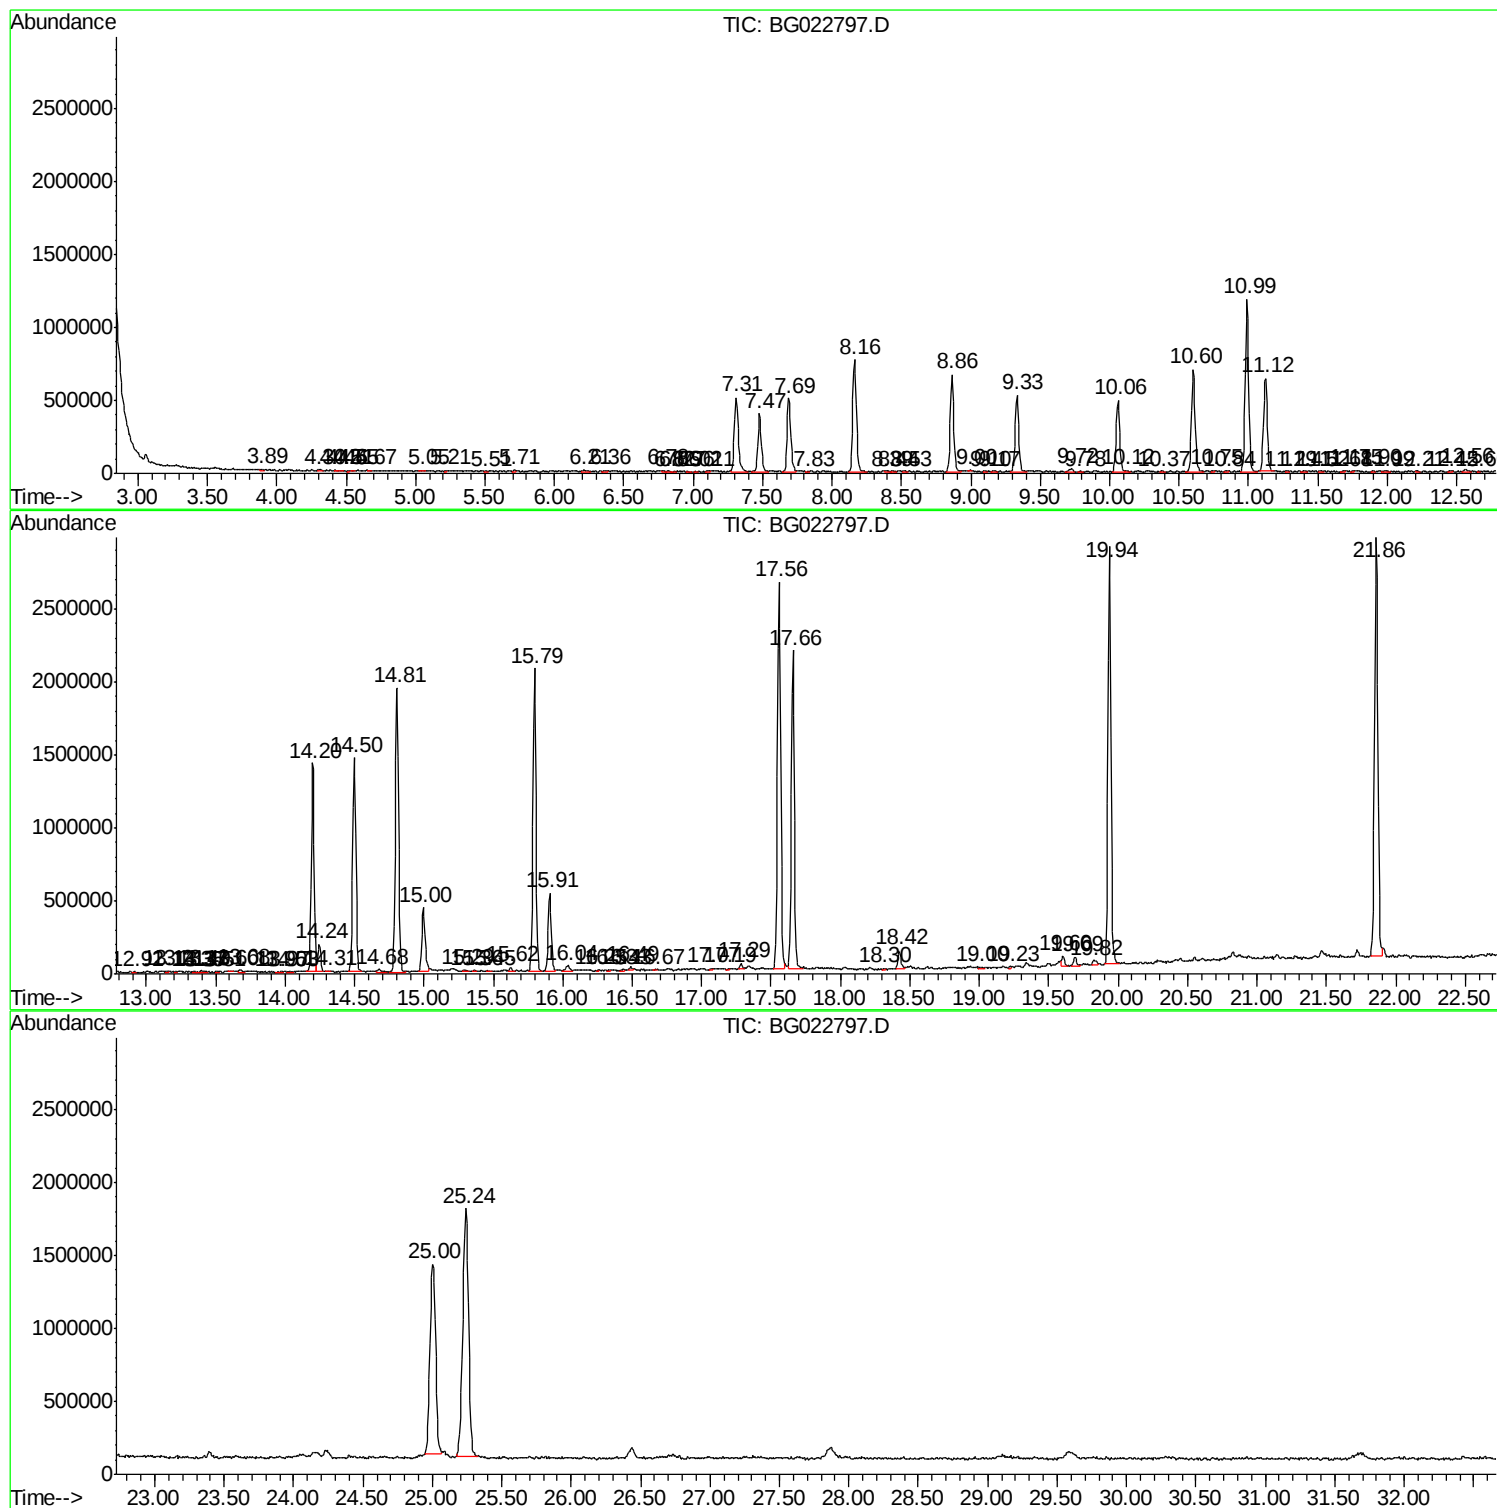

Data Path : U:\HPCHEM1\BNA_G\DATA\BG070216\
Data File : BG022797.D
Acq On : 2 Jul 2016 17:08
Operator : UM/SJ
Sample : H3752-15
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDHM7

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : U:\HPCHEM1\BNA_G\DATA\BG070216\
Data File : BG022797.D
Acq On : 2 Jul 2016 17:08
Operator : UM/SJ
Sample : H3752-15
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDHM7

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc