


Data Path : Z:\HPCHEM1\BNA_G\Data\BG070217\
 Data File : BG027811.D
 Acq On : 2 Jul 2017 9:17
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 28 19:26:37 2017

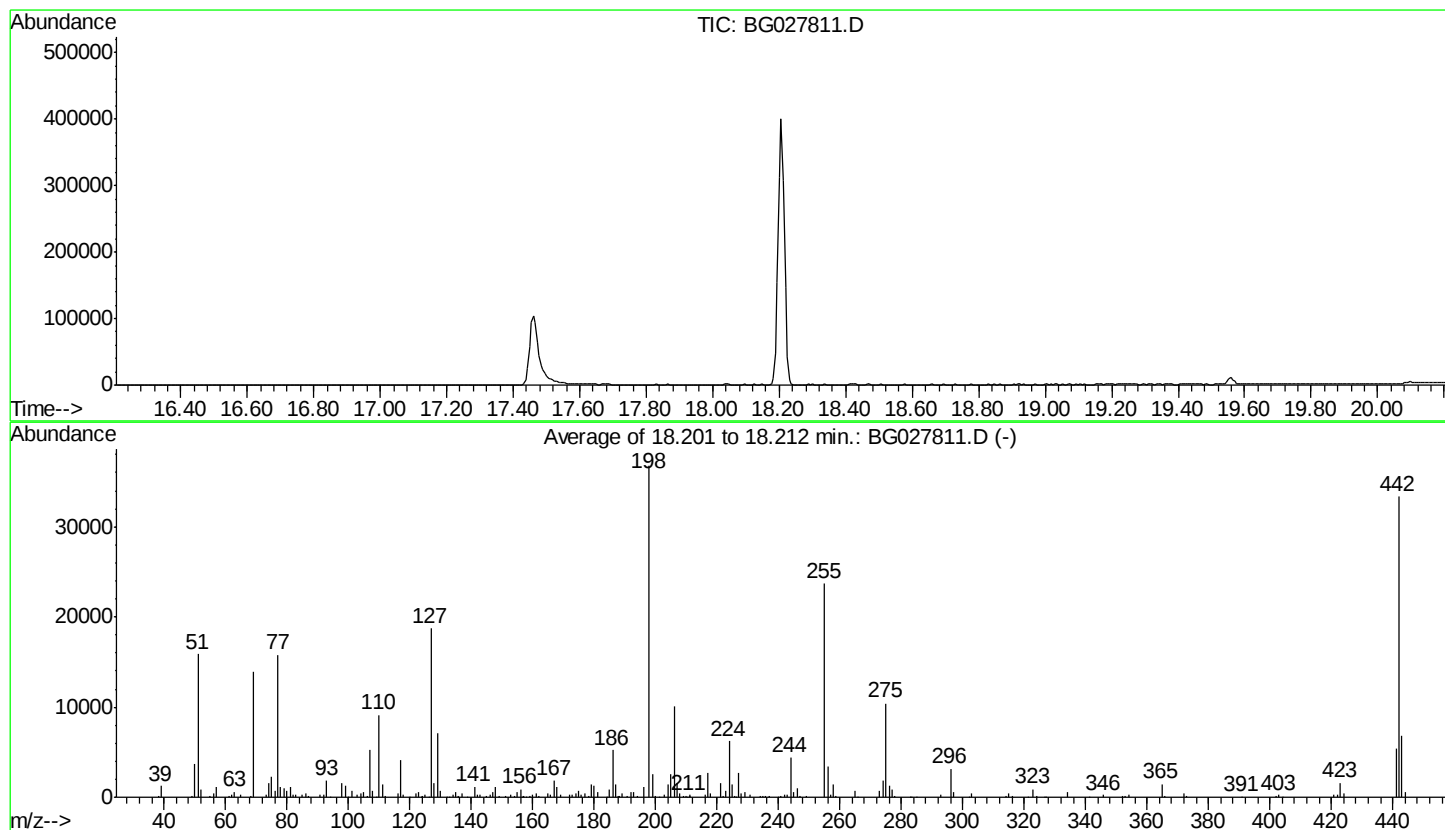

AutoFind: Scans 2436, 2437, 2438; Background Corrected with Scan 2430

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	15842	PASS
68	69	0.00	2	1.1	151	PASS
69	198	0.00	100	37.7	13856	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.9	18719	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	36784	PASS
199	198	5	9	6.9	2552	PASS
275	198	10	60	28.2	10380	PASS
365	198	1	100	3.9	1447	PASS
441	442	0.01	24	16.1	5371	PASS
442	198	50	100	90.5	33304	PASS
443	442	15	24	20.4	6794	PASS