
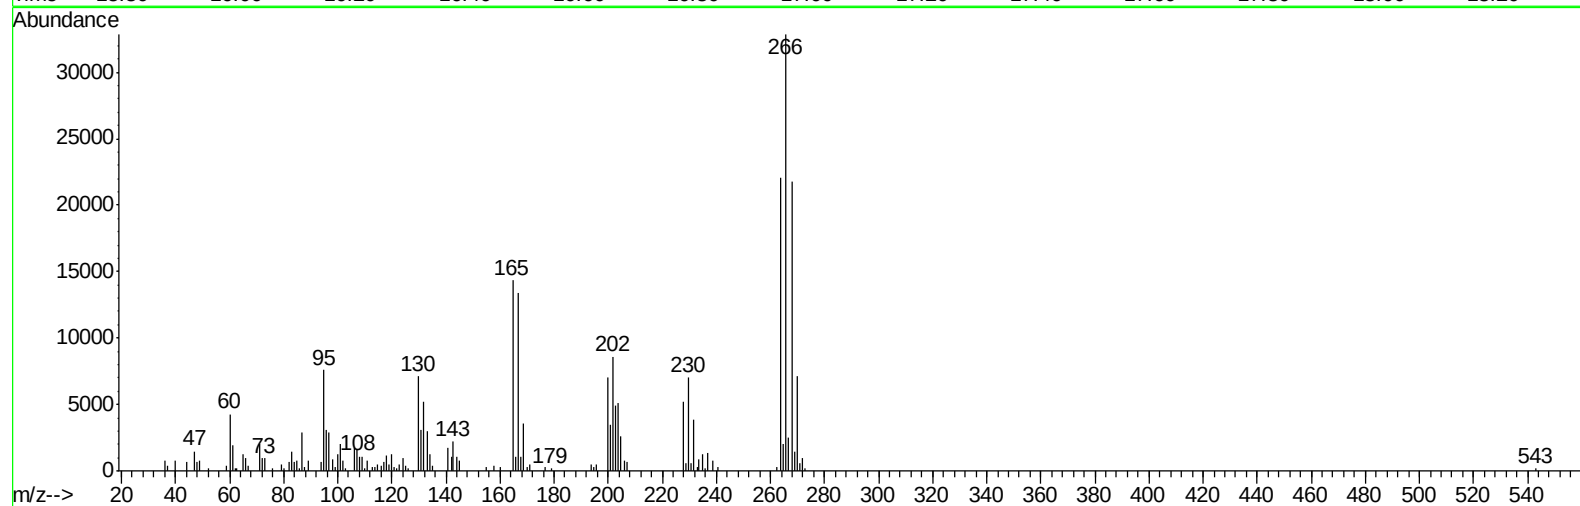


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070219\
Data File : BG041575.D
Acq On : 2 Jul 2019 16:33
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 08:57:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG062619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:25:55 2019
Response via : Initial Calibration

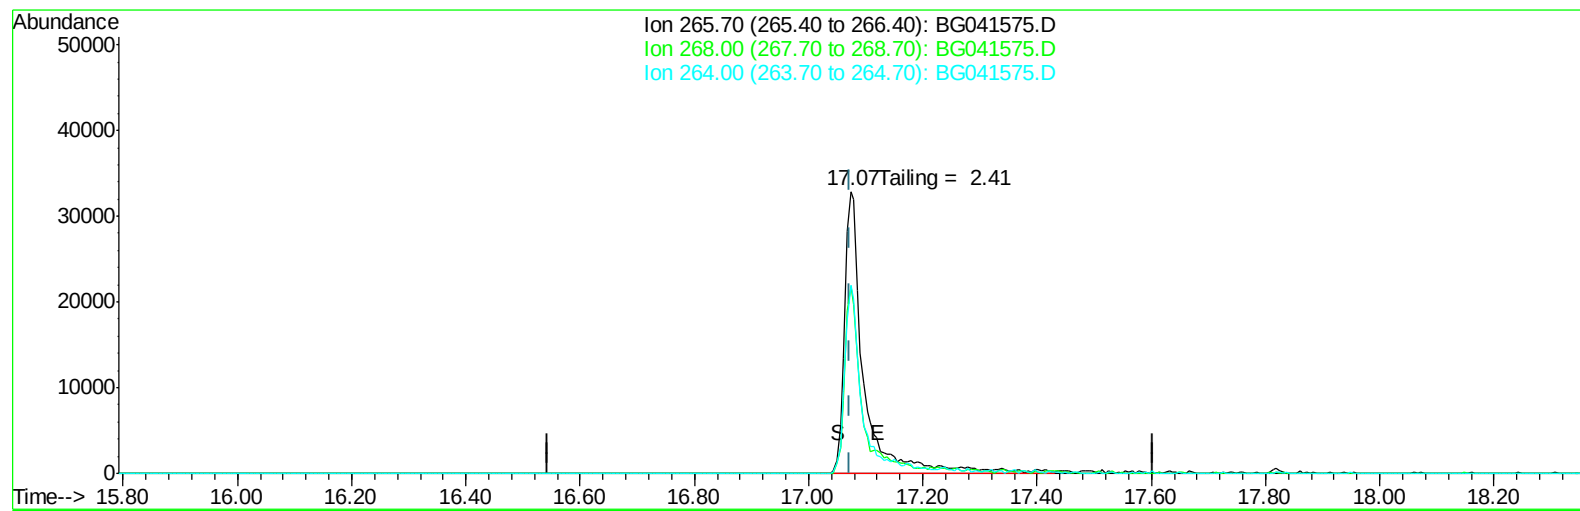

TIC: BG041575.D

(70) Pentachlorophenol (C)



17.073min (-0.001) 14750.65ng

response 73019

Ion	Exp%	Act%
265.70	100	100
268.00	58.70	66.17
264.00	59.20	67.05
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070219\
Data File : BG041575.D
Acq On : 2 Jul 2019 16:33
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 08:57:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG062619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:25:55 2019
Response via : Initial Calibration

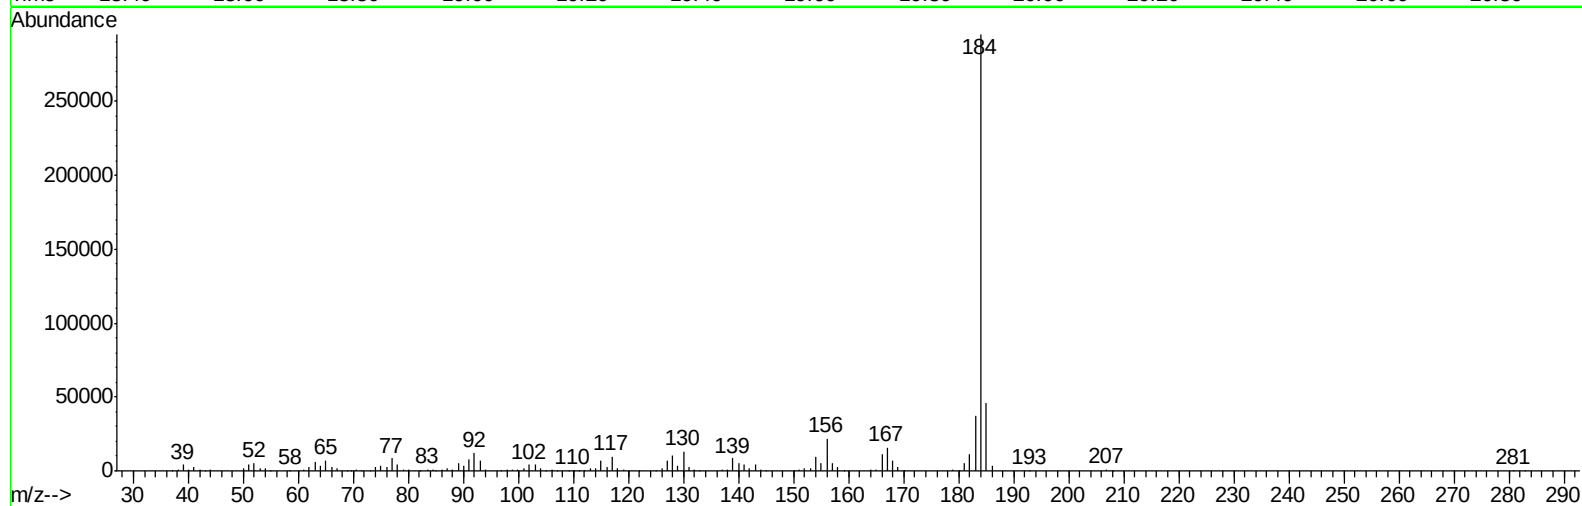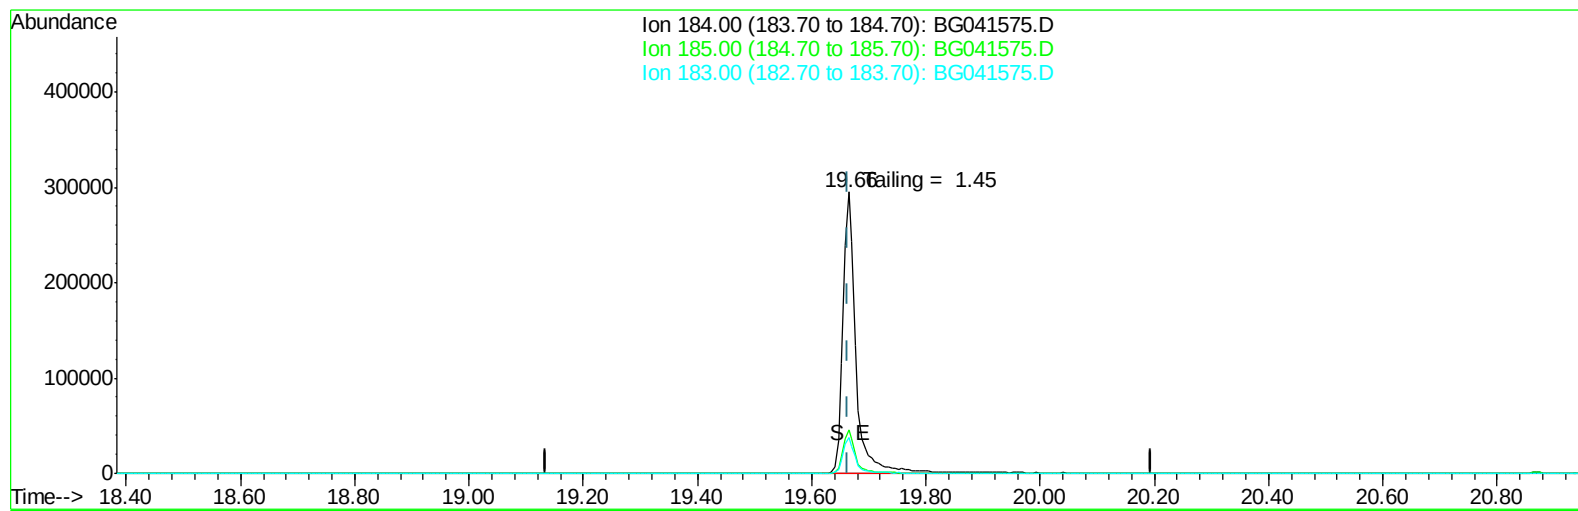

TIC: BG041575.D

(77) Benzidine

19.664min (-0.001) 7374.00ng

response 468590

Ion	Exp%	Act%
184.00	100	100
185.00	15.90	15.55
183.00	11.80	12.54
0.00	0.00	0.00