
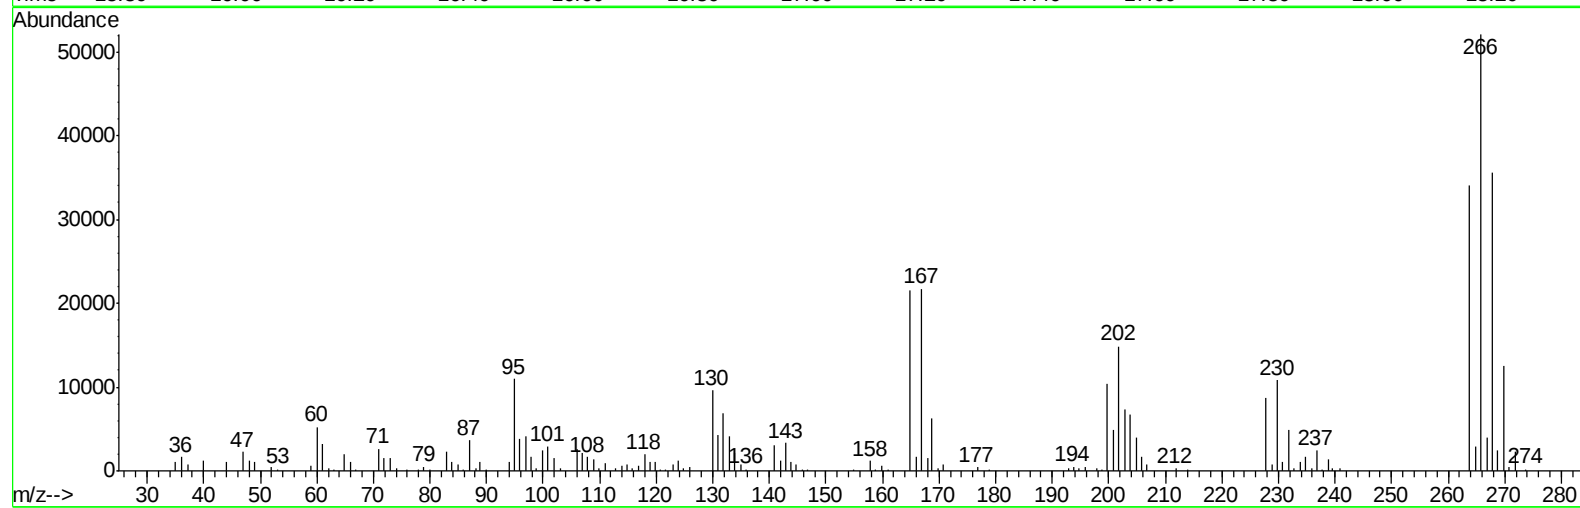


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070219\
Data File : BG041564.D
Acq On : 2 Jul 2019 8:43
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 08:53:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG062619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:25:55 2019
Response via : Initial Calibration

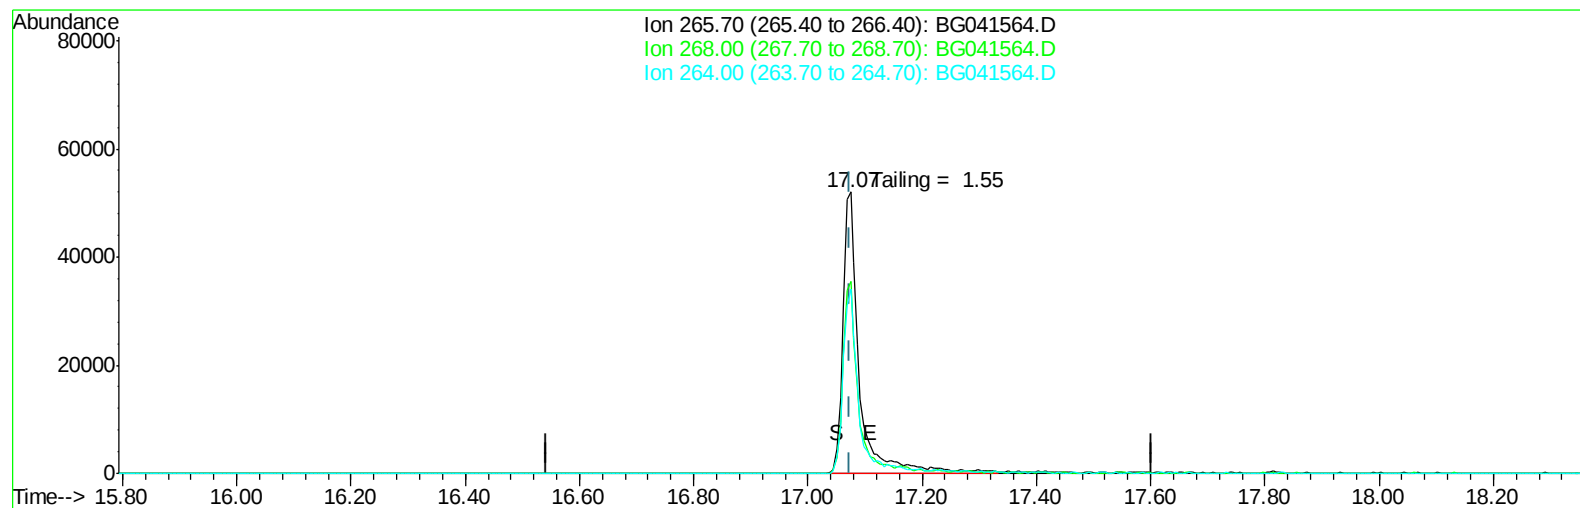

TIC: BG041564.D

(70) Pentachlorophenol (C)



17.074min (+0.001) 12099.85ng

response 99613

Ion	Exp%	Act%
265.70	100	100
268.00	58.70	68.34
264.00	59.20	65.46
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070219\
Data File : BG041564.D
Acq On : 2 Jul 2019 8:43
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 08:53:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG062619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:25:55 2019
Response via : Initial Calibration

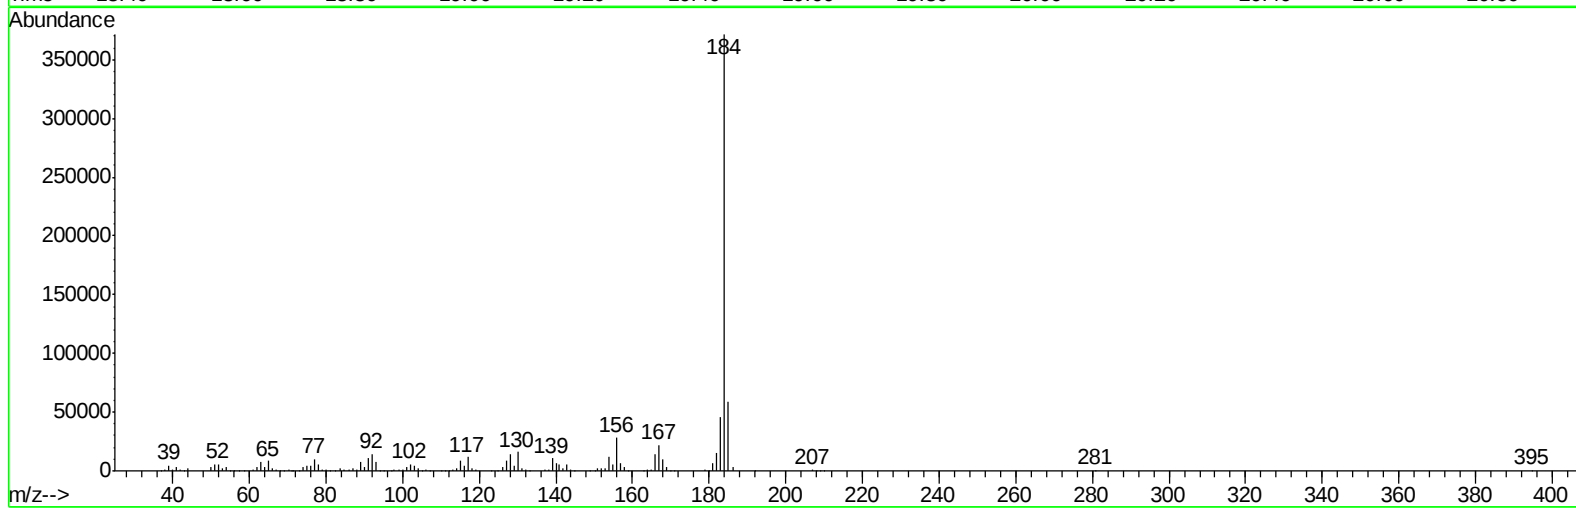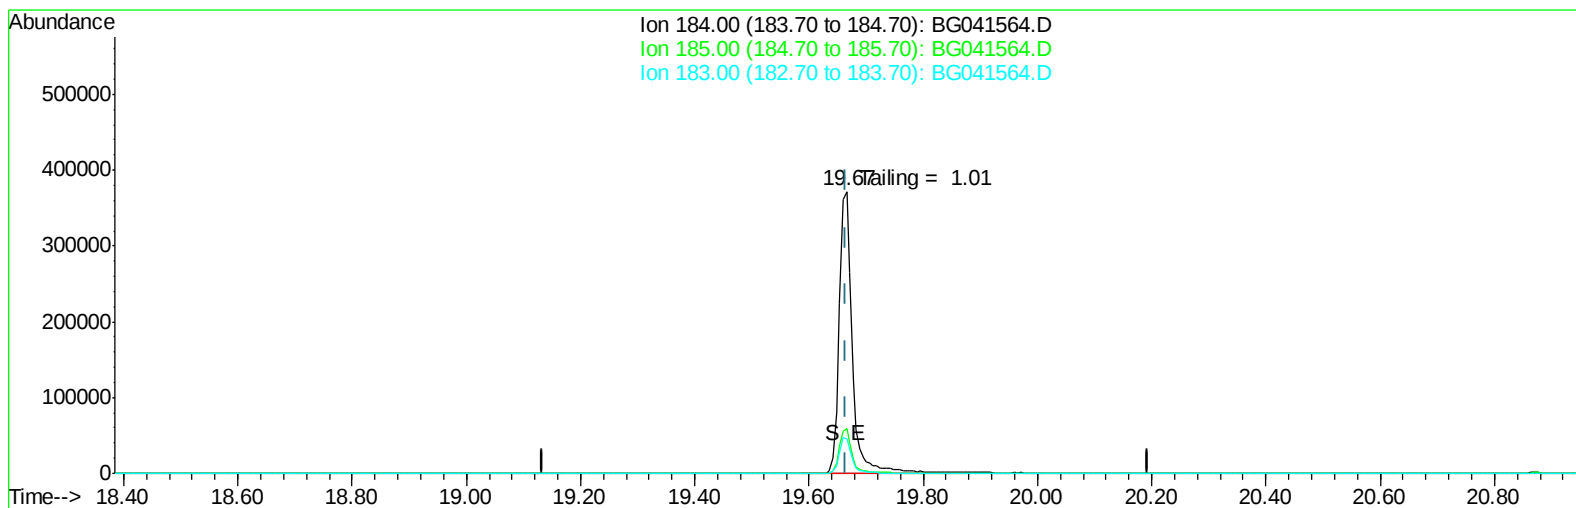

TIC: BG041564.D

(77) Benzidine

19.665min (+0.001) 6846.85ng

response 590503

Ion	Exp%	Act%
184.00	100	100
185.00	15.90	15.81
183.00	11.80	12.37
0.00	0.00	0.00