

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070219\
 Data File : BG041578.D
 Acq On : 3 Jul 2019 1:53
 Operator : HP/JU
 Sample : PB121109BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB121109BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG062619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.568	416	422	438	rBV	514530	854388	29.40%	7.352%
2	7.189	691	698	712	rBV	528568	911514	31.36%	7.843%
3	7.559	753	761	776	rBV	511687	918955	31.62%	7.907%
4	8.029	835	841	849	rBV	106602	187744	6.46%	1.616%
5	8.347	889	895	907	rBV	424474	742575	25.55%	6.390%
6	9.210	1035	1042	1054	rBV	310521	574800	19.78%	4.946%
7	10.856	1316	1322	1331	rBV	99312	198700	6.84%	1.710%
8	13.294	1730	1737	1751	rBV	876253	1381190	47.53%	11.885%
9	14.675	1965	1972	1985	rBV2	174500	306846	10.56%	2.640%
10	16.167	2220	2226	2247	rBV	588870	1048519	36.08%	9.022%
11	17.424	2433	2440	2454	rBV2	266301	439799	15.13%	3.784%
12	20.027	2876	2883	2896	rBV	2191414	2906152	100.00%	25.007%
13	21.696	3161	3167	3179	rBV	346661	610680	21.01%	5.255%
14	24.992	3717	3728	3740	rBV2	171168	539465	18.56%	4.642%


Sum of corrected areas: 11621327

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070219\
Data File : BG041578.D
Acq On : 3 Jul 2019 1:53
Operator : HP/JU
Sample : PB121109BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB121109BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG062619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

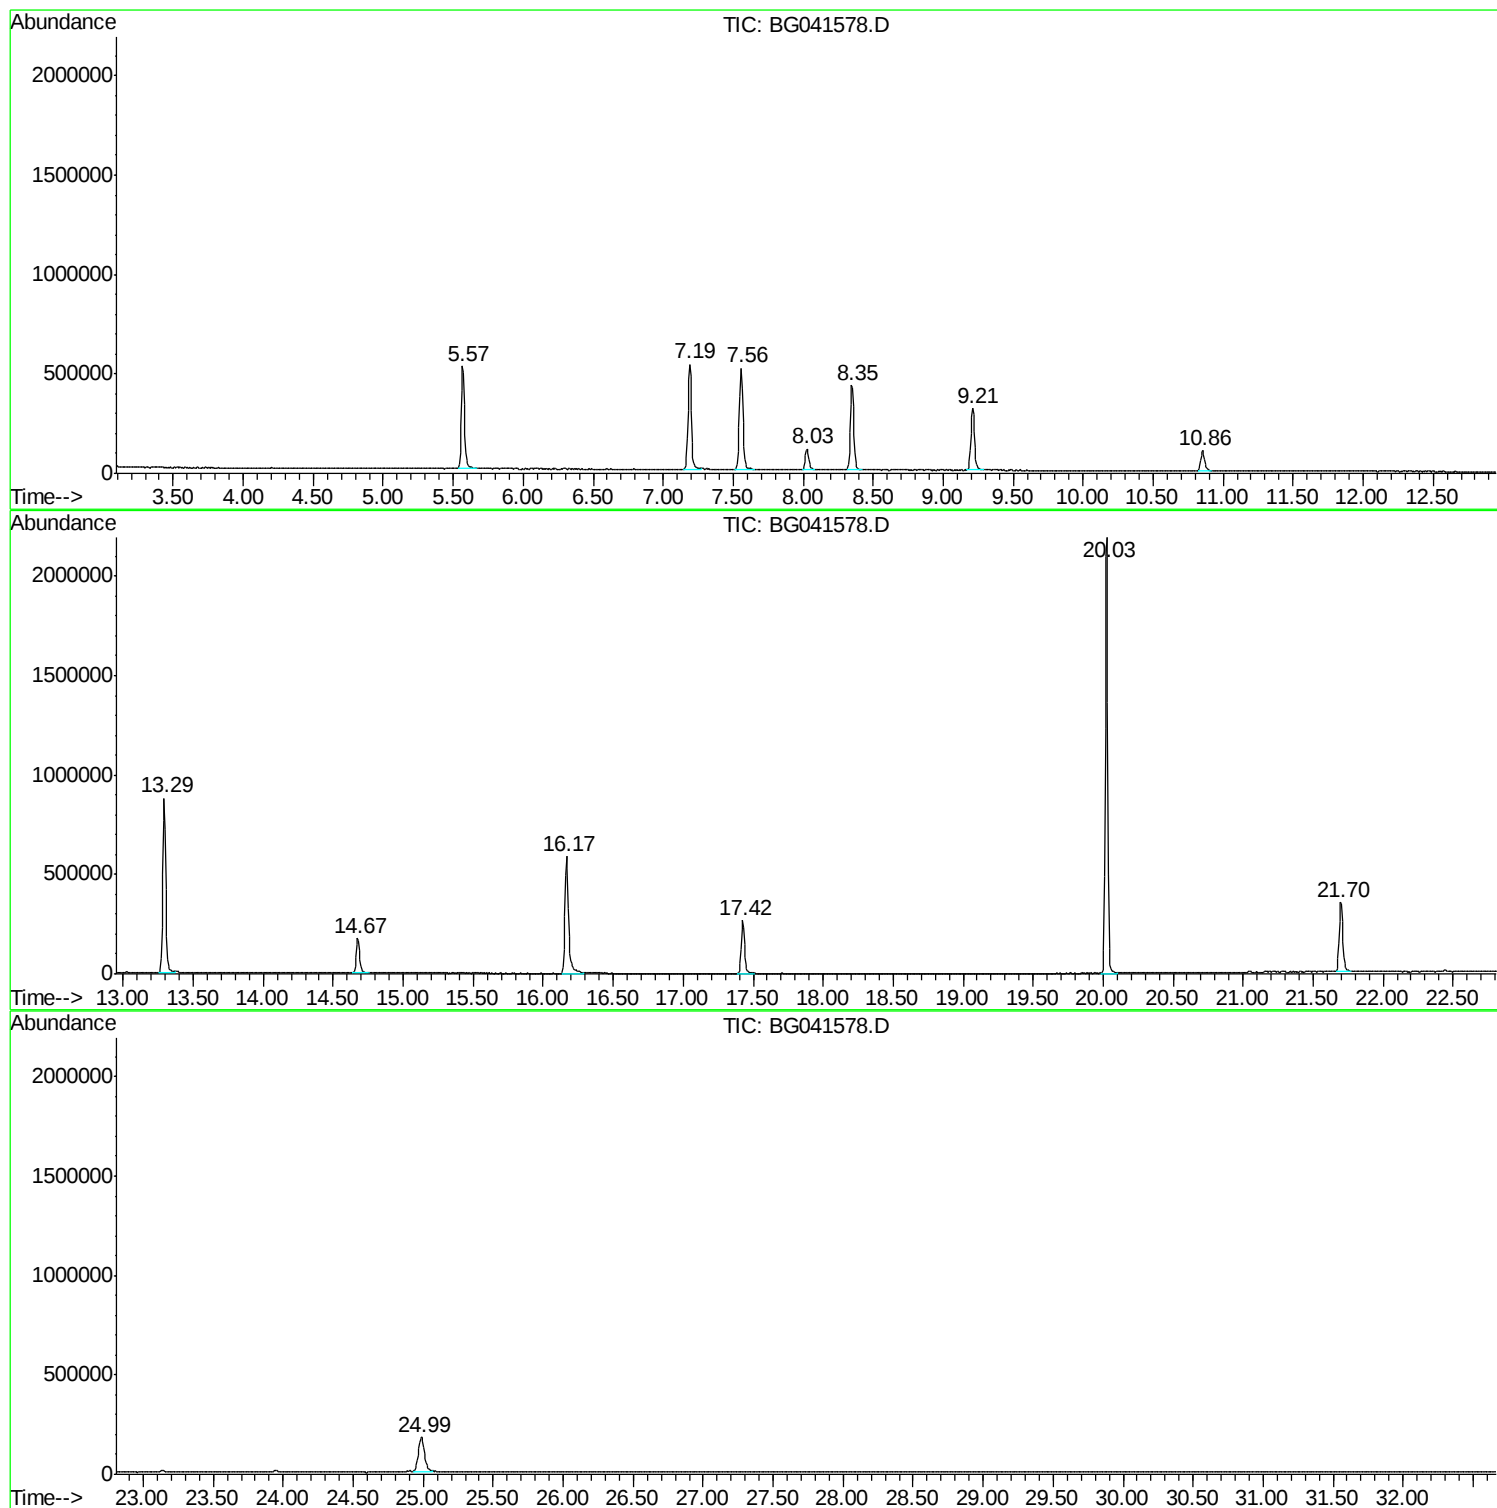

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG070219\
Data_File : BG041578.D
Acq_On : 3_Jul_2019 1:533
Operator : HP/JUU
Sample : PB121109BLL
Misc :
ALS_Vial : 4 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
PB121109BL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG062619.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
