


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070219\
 Data File : BG041564.D
 Acq On : 2 Jul 2019 8:43
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG062619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 27 13:25:55 2019

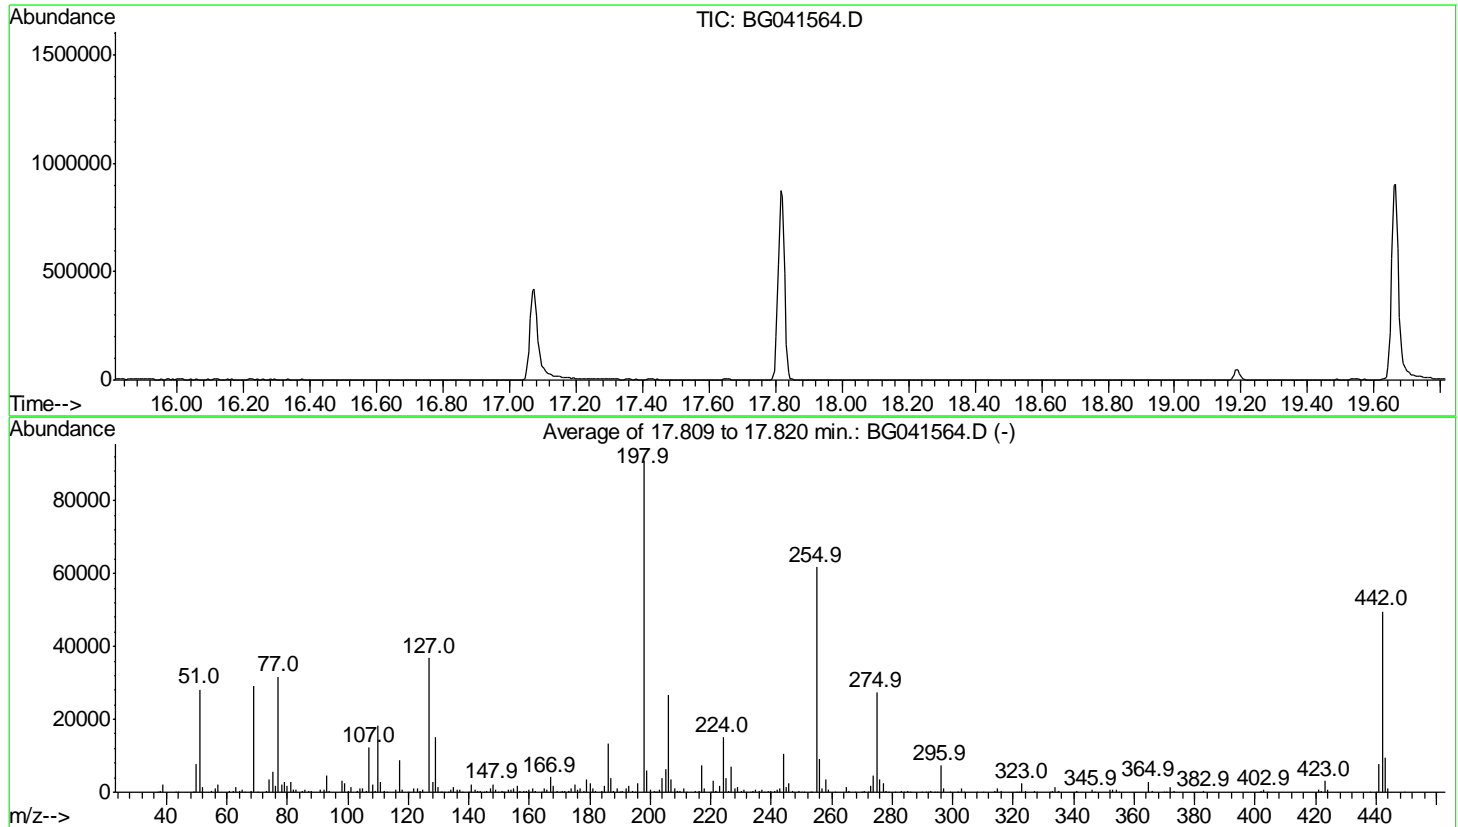

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.0	28229	PASS
68	69	0.00	2	1.5	428	PASS
69	198	0.00	100	32.0	29072	PASS
70	69	0.00	2	0.6	160	PASS
127	198	10	80	40.4	36797	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	90986	PASS
199	198	5	9	6.5	5952	PASS
275	198	10	60	29.9	27248	PASS
365	198	1	100	3.2	2949	PASS
441	198	0.01	100	8.3	7587	PASS
442	198	50	100	54.5	49568	PASS
443	442	15	24	18.9	9385	PASS