


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070219\
 Data File : BG041575.D
 Acq On : 2 Jul 2019 16:33
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG062619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 27 13:25:55 2019

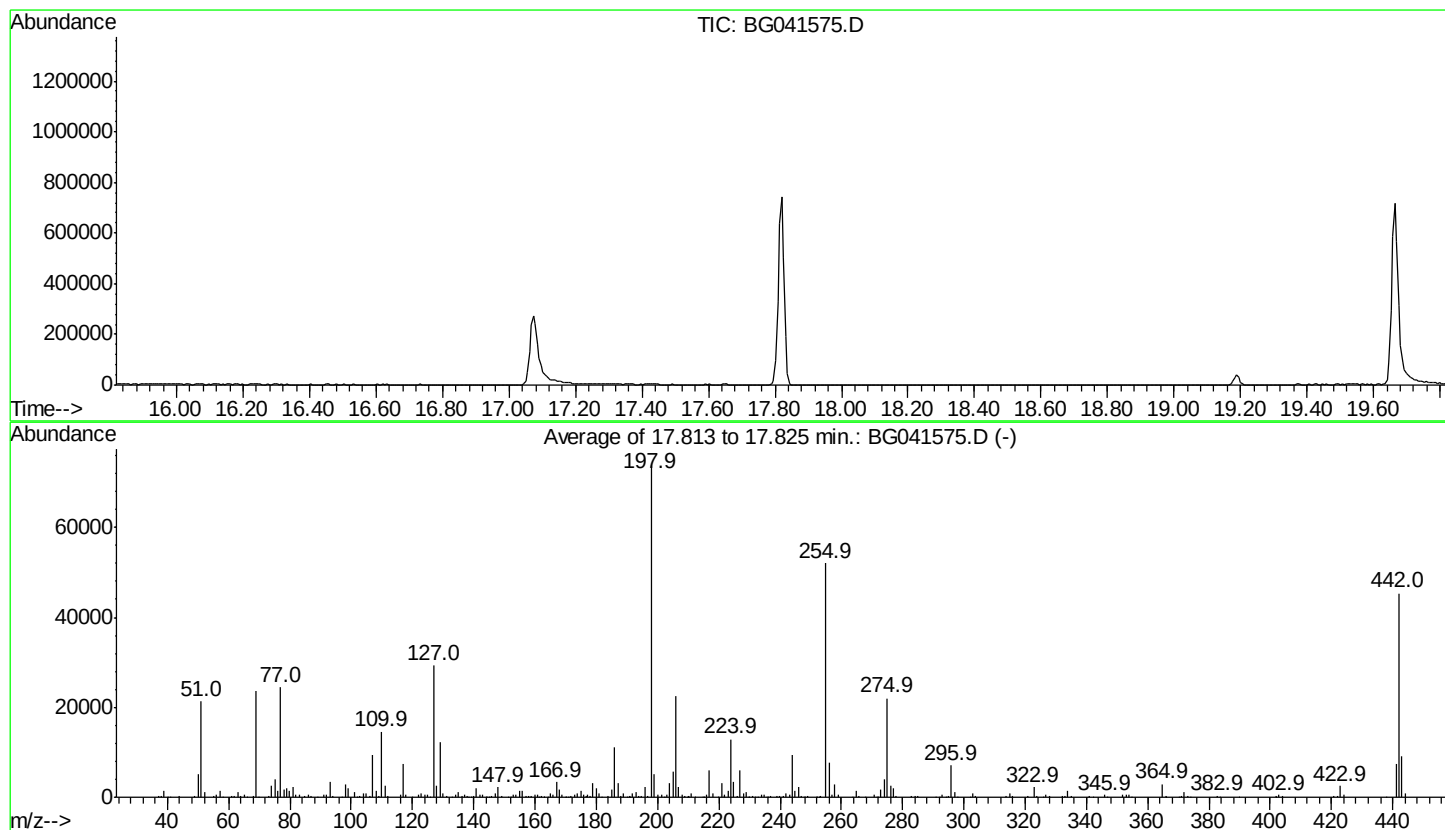

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	21346	PASS
68	69	0.00	2	1.0	230	PASS
69	198	0.00	100	32.0	23582	PASS
70	69	0.00	2	0.2	57	PASS
127	198	10	80	39.7	29296	PASS
197	198	0.00	2	0.2	171	PASS
198	198	100	100	100.0	73752	PASS
199	198	5	9	7.0	5158	PASS
275	198	10	60	29.9	22040	PASS
365	198	1	100	3.9	2866	PASS
441	198	0.01	100	10.0	7342	PASS
442	198	50	100	61.4	45296	PASS
443	442	15	24	20.3	9174	PASS