
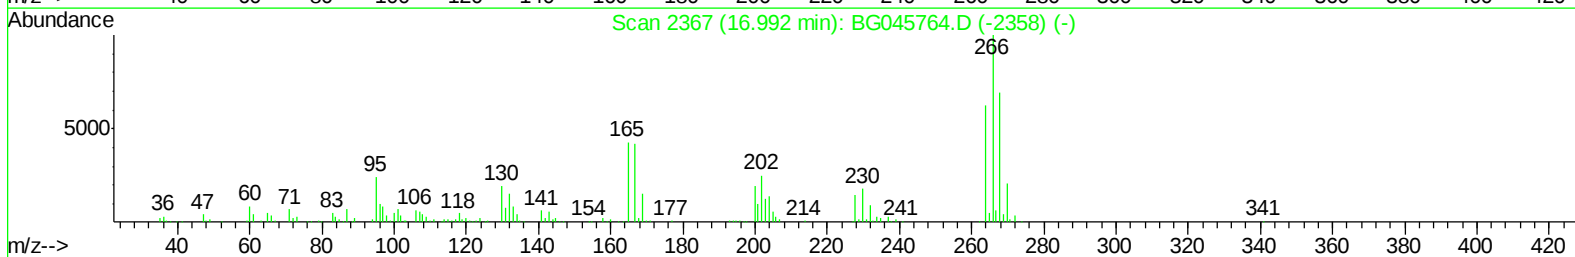
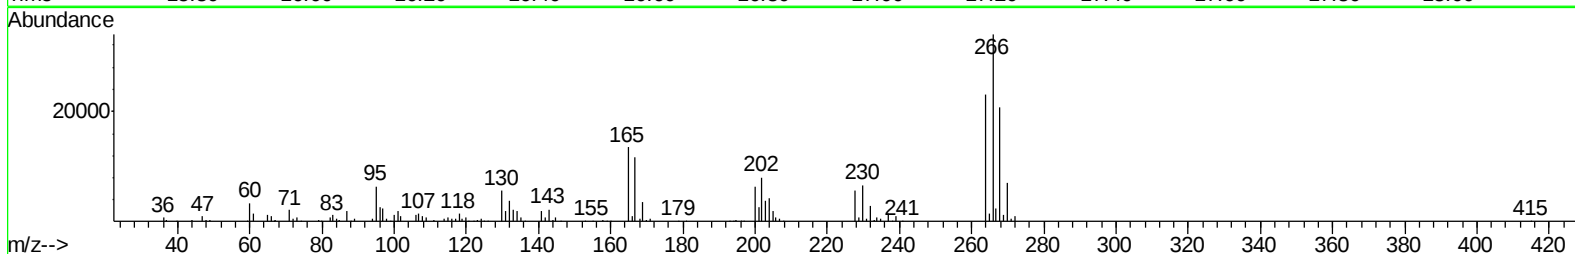


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070220\
Data File : BG045910.D
Acq On : 2 Jul 2020 11:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 06:38:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 02 14:02:29 2020
Response via : Initial Calibration

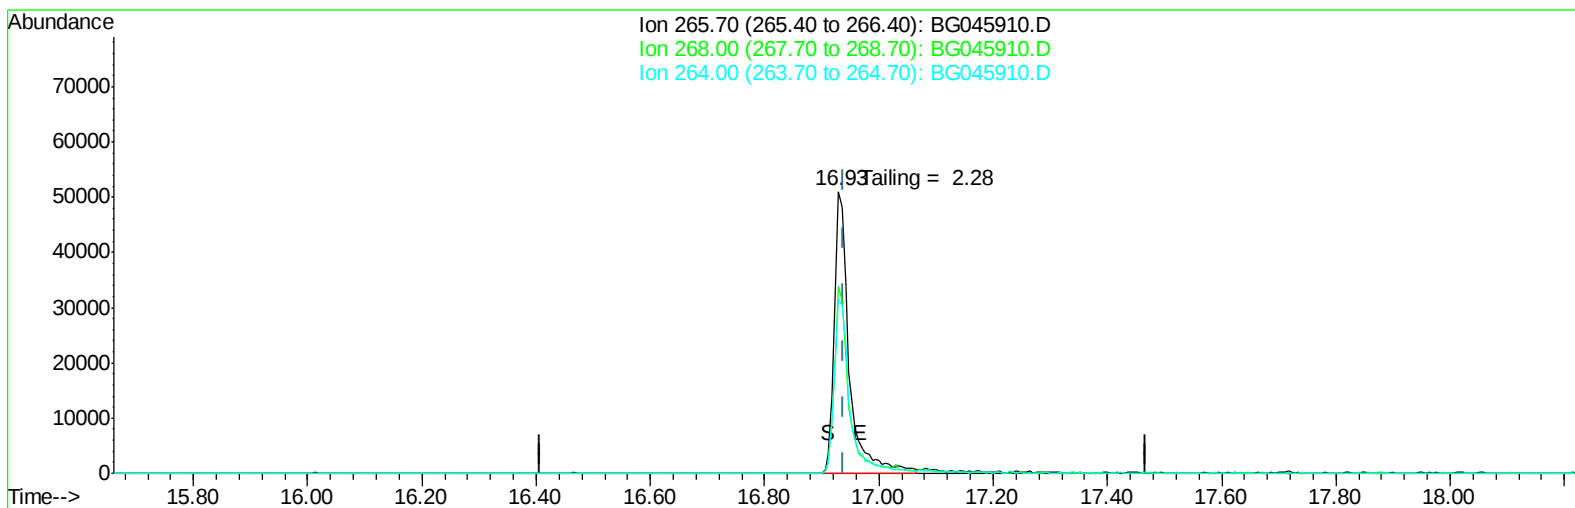

TIC: BG045910.D

(70) Pentachlorophenol (C)




16.929min (-0.009) 178939.60ng

response 93322

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	66.16
264.00	58.80	61.98
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070220\
 Data File : BG045910.D
 Acq On : 2 Jul 2020 11:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 06:38:36 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 02 14:02:29 2020
 Response via : Initial Calibration

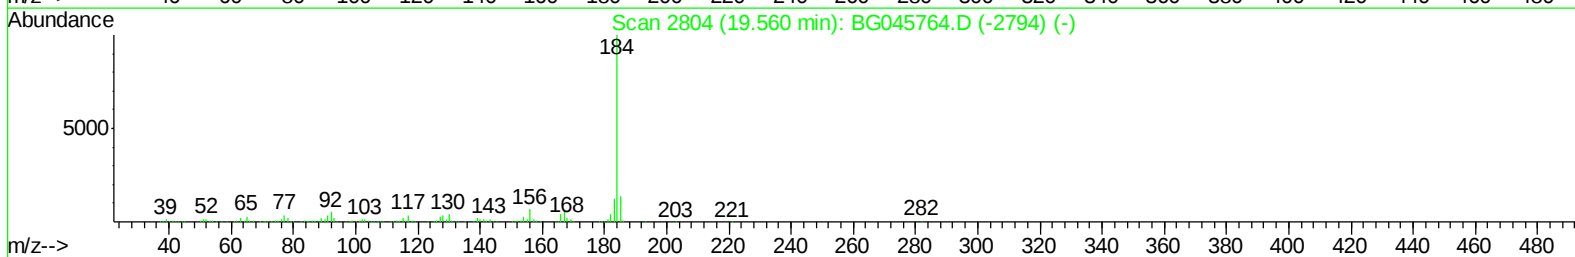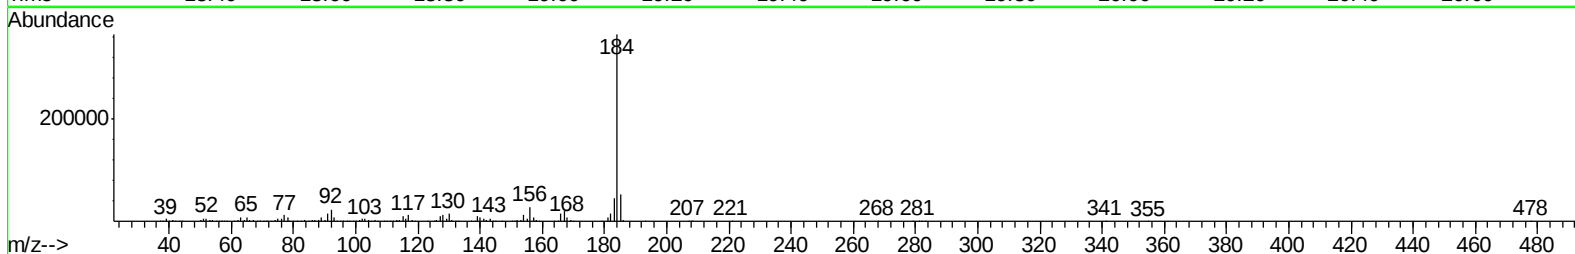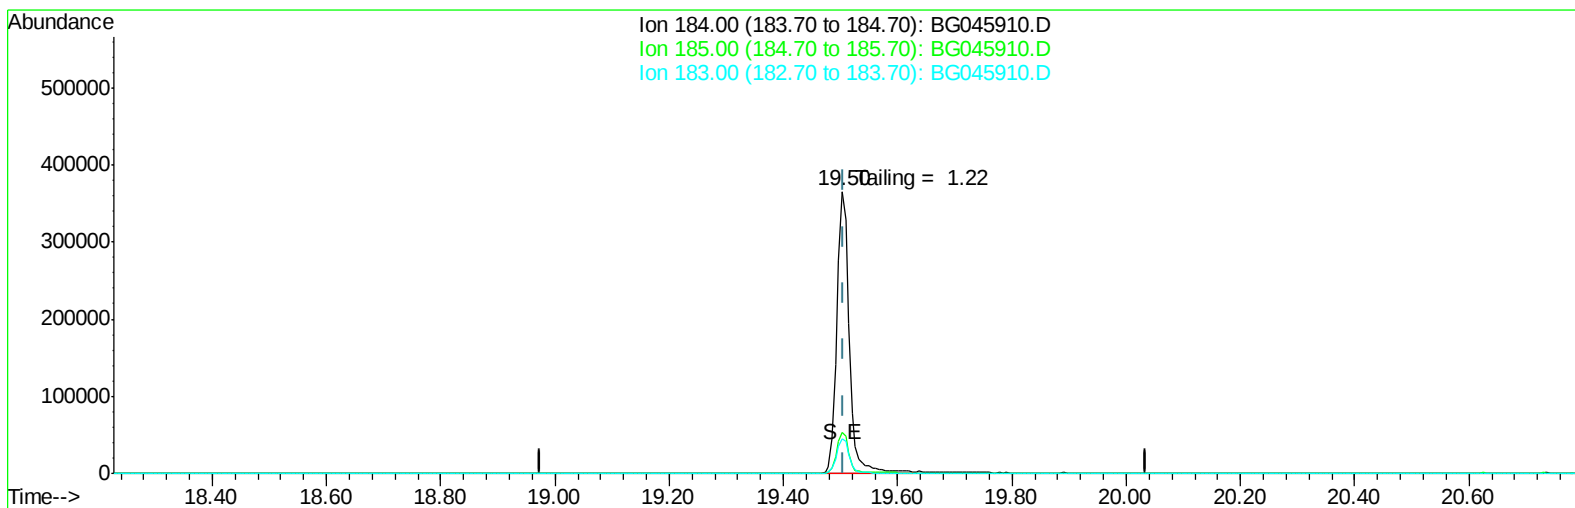

TIC: BG045910.D

(77) Benzidine

19.502min (-0.004) 35428.36ng

response 557224

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.45
183.00	13.20	12.48
0.00	0.00	0.00