
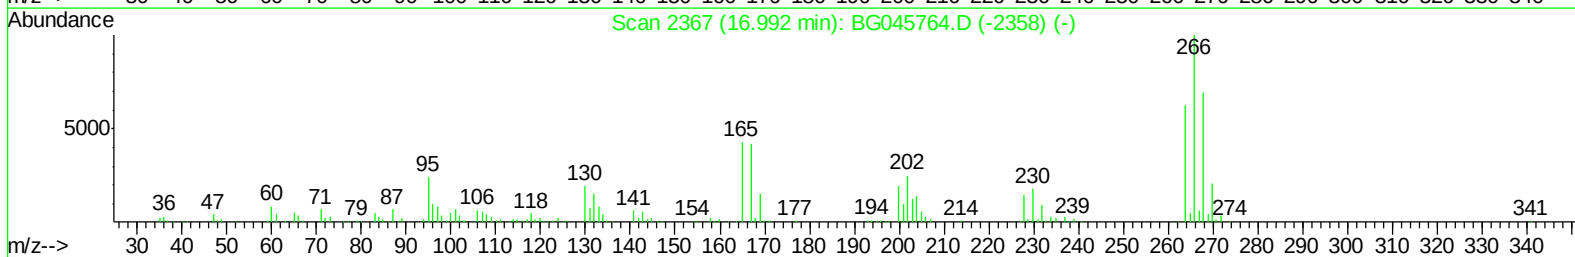
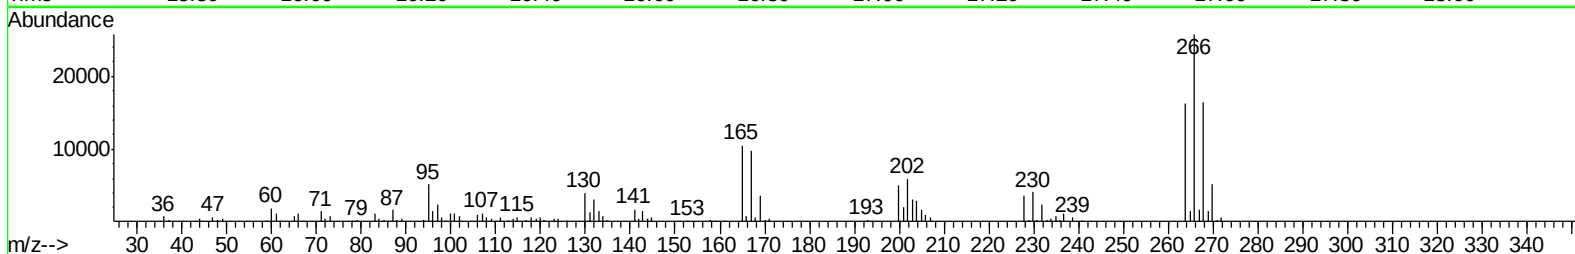


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070220\
 Data File : BG045928.D
 Acq On : 3 Jul 2020 00:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 01:27:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 02 14:02:29 2020
 Response via : Initial Calibration

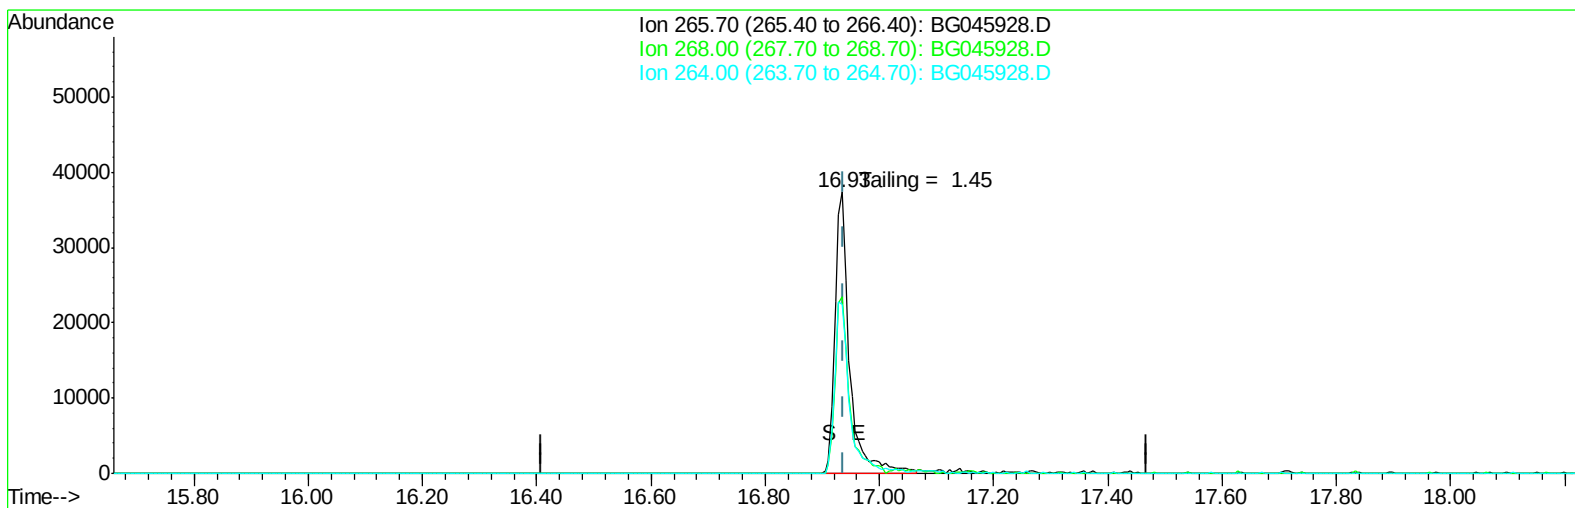

TIC: BG045928.D

(70) Pentachlorophenol (C)




16.934min (-0.005) 24279.19ng

response 65612

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	62.58
264.00	58.80	60.14
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070220\
 Data File : BG045928.D
 Acq On : 3 Jul 2020 00:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 01:27:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 02 14:02:29 2020
 Response via : Initial Calibration

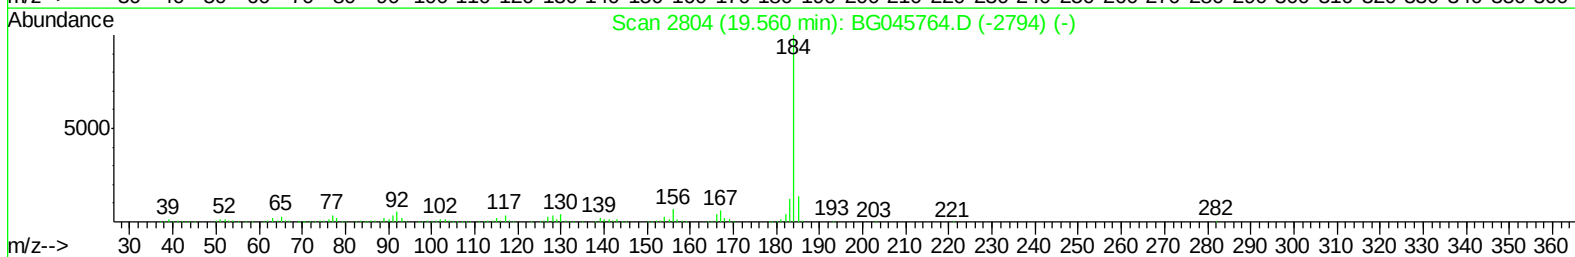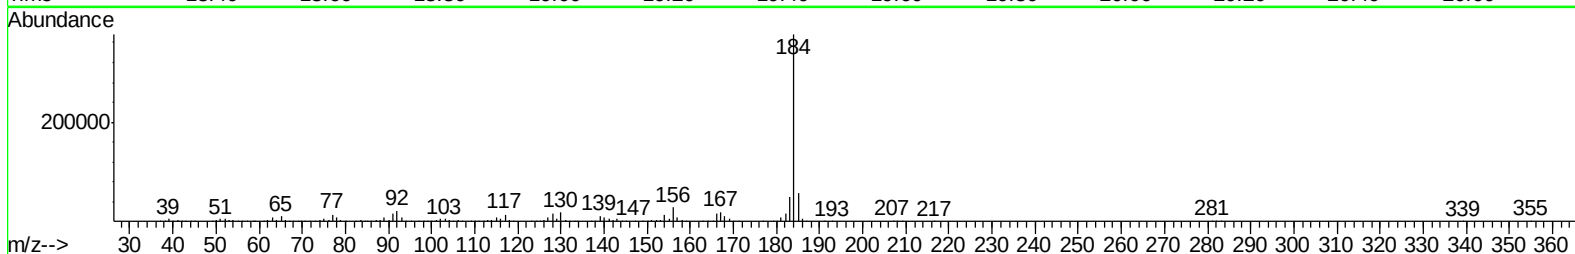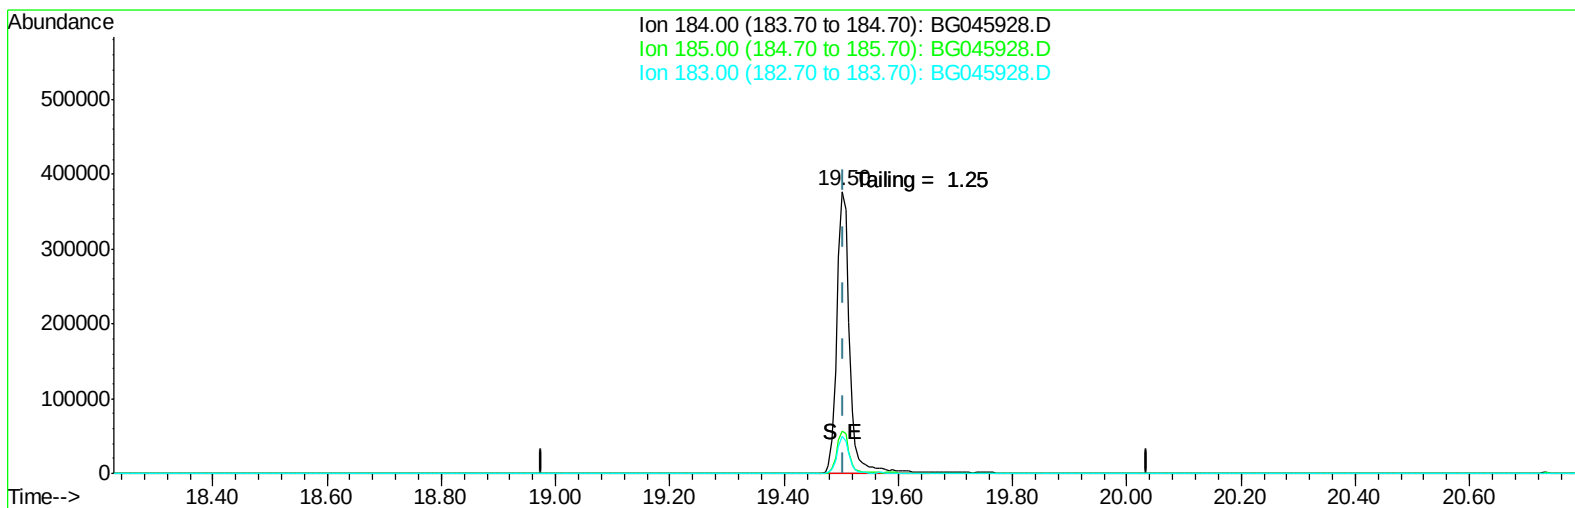

TIC: BG045928.D

(77) Benzidine

19.501min (-0.005) 350731.41ng

response 583550

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.01
183.00	13.20	13.38
0.00	0.00	0.00