


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070220\
 Data File : BG045910.D
 Acq On : 2 Jul 2020 11:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 02 14:02:29 2020

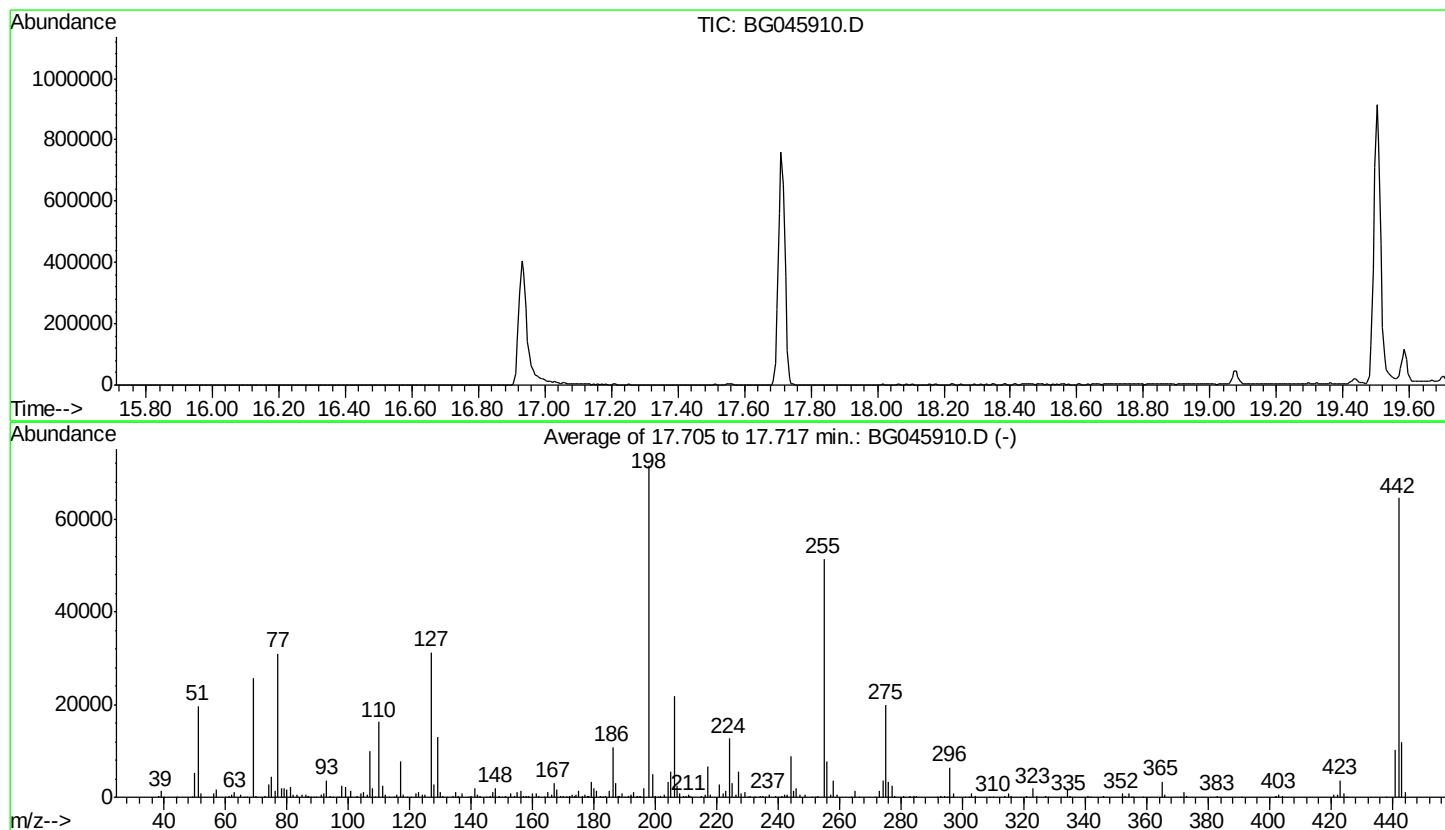

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.5	19690	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.0	25752	PASS
70	69	0.00	2	0.7	184	PASS
127	198	10	80	43.6	31181	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	71474	PASS
199	198	5	9	7.0	4970	PASS
275	198	10	60	28.0	19997	PASS
365	198	1	100	4.7	3344	PASS
441	198	0.01	100	14.3	10244	PASS
442	198	50	100	90.2	64490	PASS
443	442	15	24	18.5	11934	PASS