


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070220\
 Data File : BG045928.D
 Acq On : 3 Jul 2020 00:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 02 14:02:29 2020

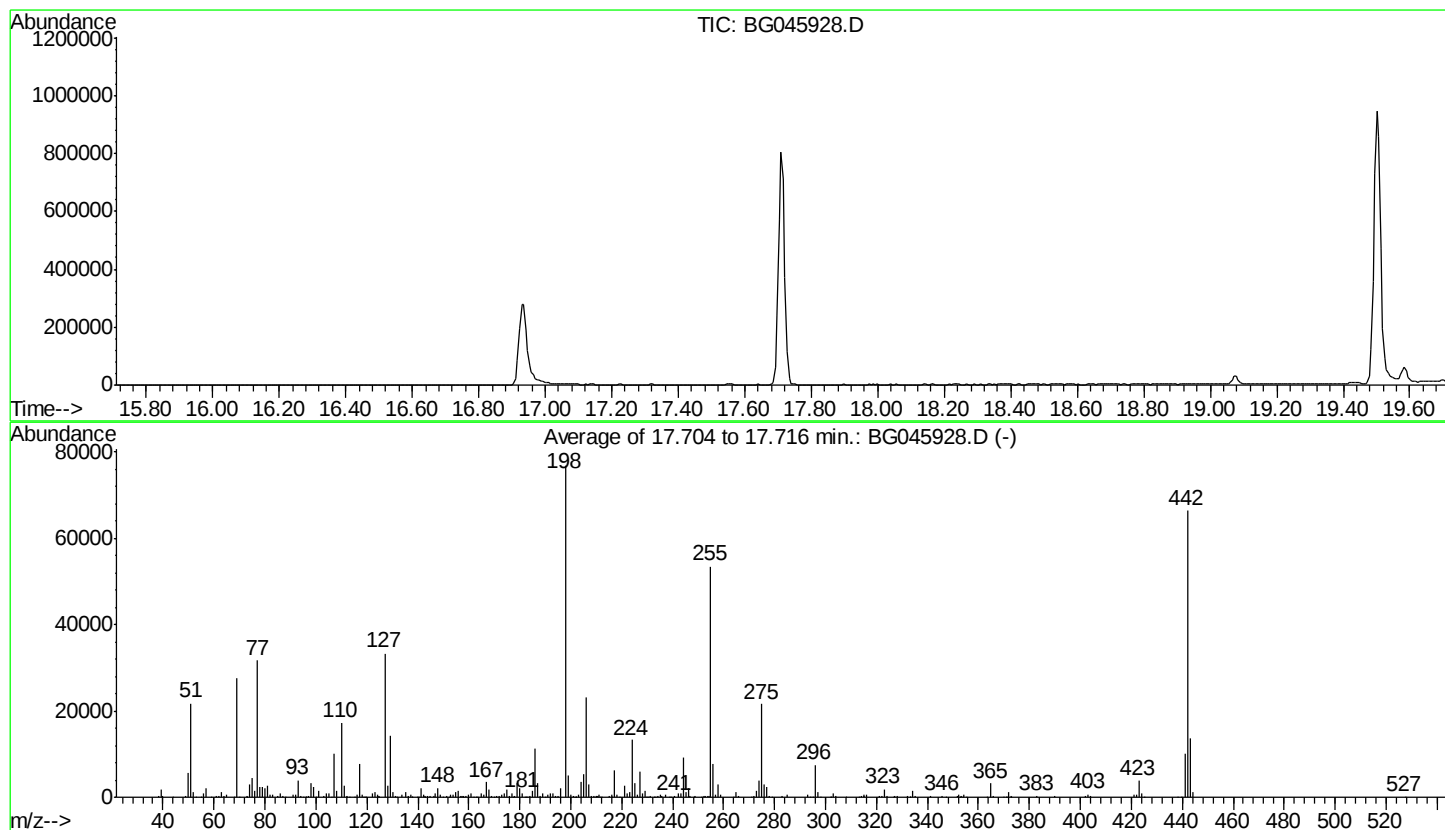

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.3	21722	PASS
68	69	0.00	2	0.4	108	PASS
69	198	0.00	100	36.0	27621	PASS
70	69	0.00	2	0.5	140	PASS
127	198	10	80	43.3	33234	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	76786	PASS
199	198	5	9	6.5	5026	PASS
275	198	10	60	28.0	21530	PASS
365	198	1	100	4.2	3229	PASS
441	198	0.01	100	13.1	10078	PASS
442	198	50	100	86.3	66290	PASS
443	442	15	24	20.4	13508	PASS