
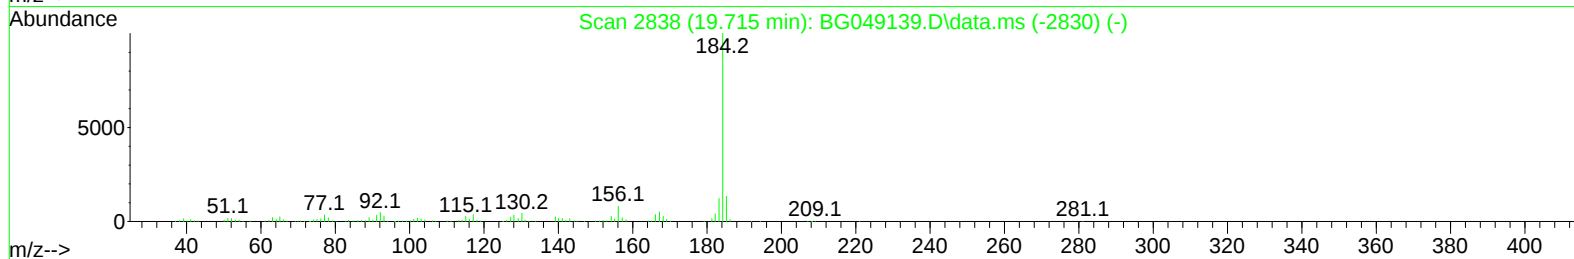
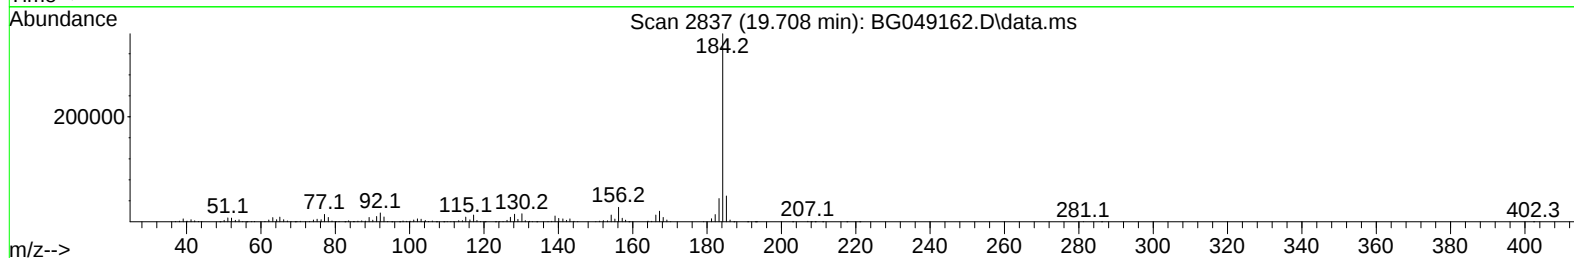


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070221\
Data File : BG049162.D
Acq On : 2 Jul 2021 11:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 13:26:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 30 15:39:12 2021
Response via : Initial Calibration

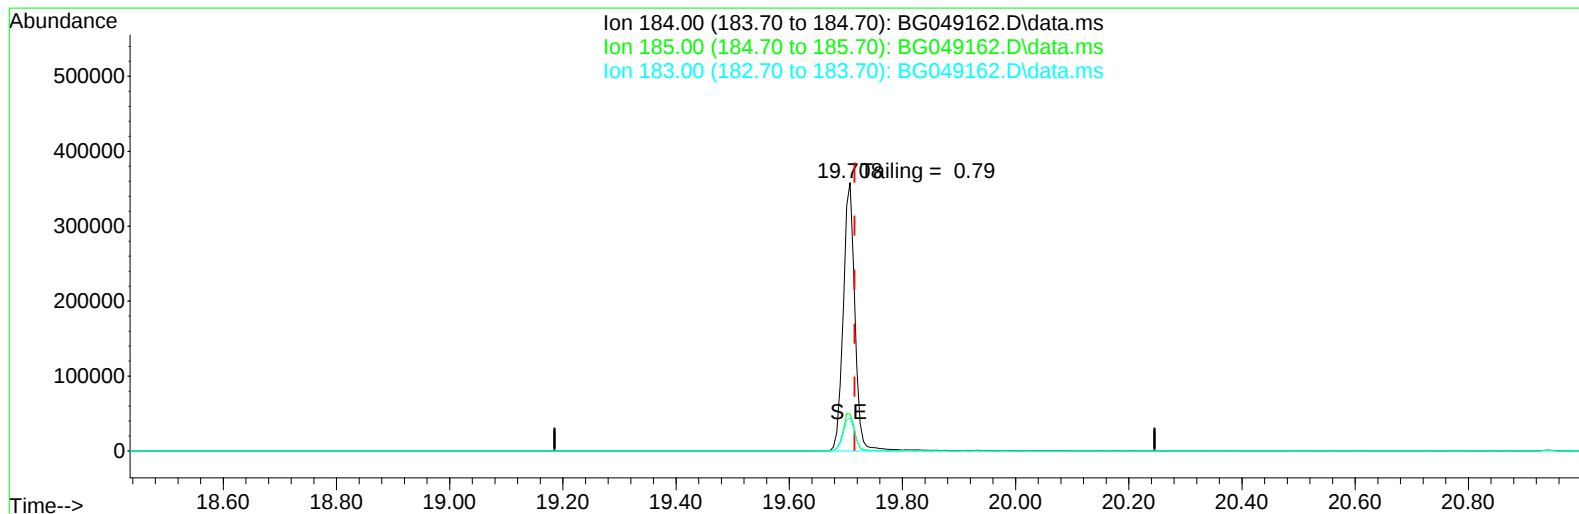




TIC: BG049162.D\data.ms

(77) Benzidine**19.708min (-0.008) 416348.75 ng****response 509754**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.74
183.00	11.70	12.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070221\
Data File : BG049162.D
Acq On : 2 Jul 2021 11:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 13:26:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 30 15:39:12 2021
Response via : Initial Calibration

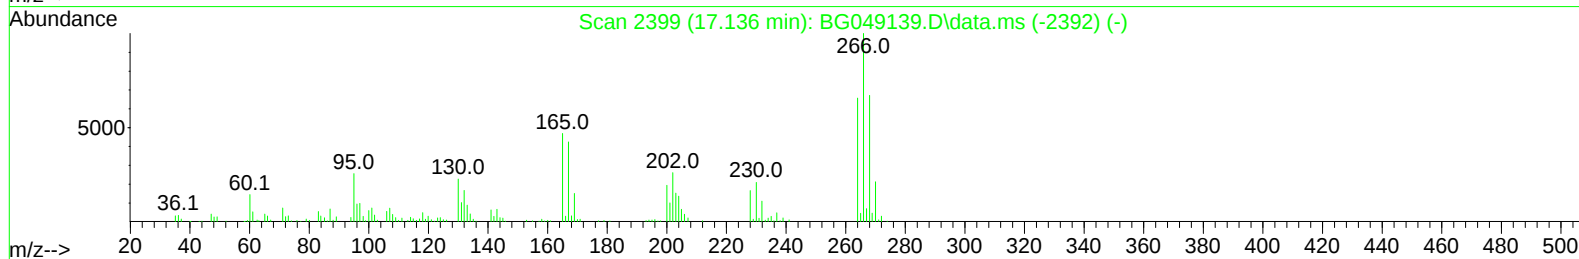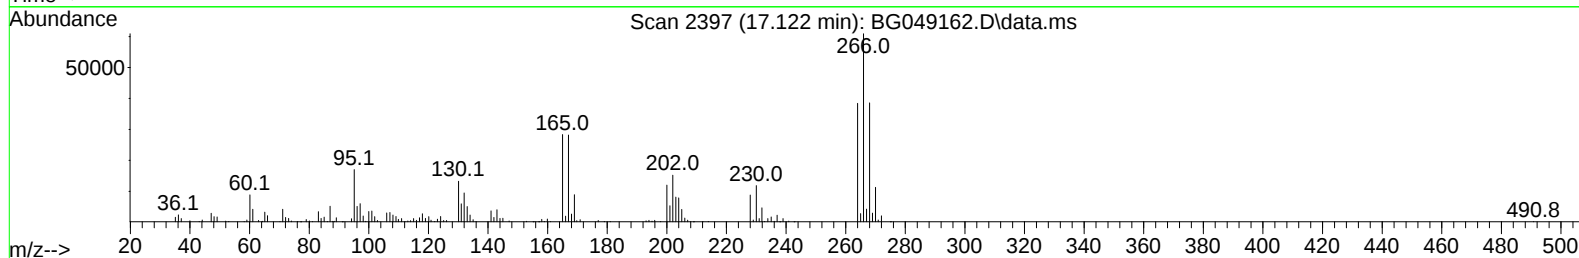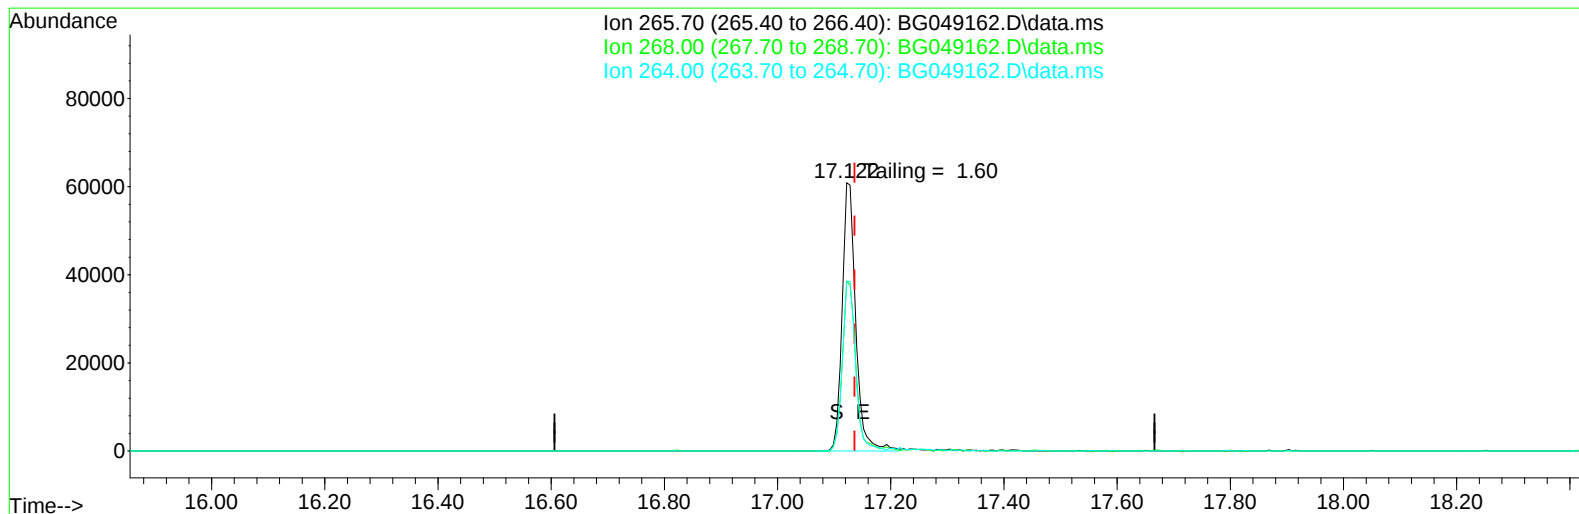

TIC: BG049162.D\data.ms

(70) Pentachlorophenol (C)

17.122min (-0.014) 208884.78 ng

response 99739

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.36
264.00	61.30	63.07
0.00	0.00	0.00