
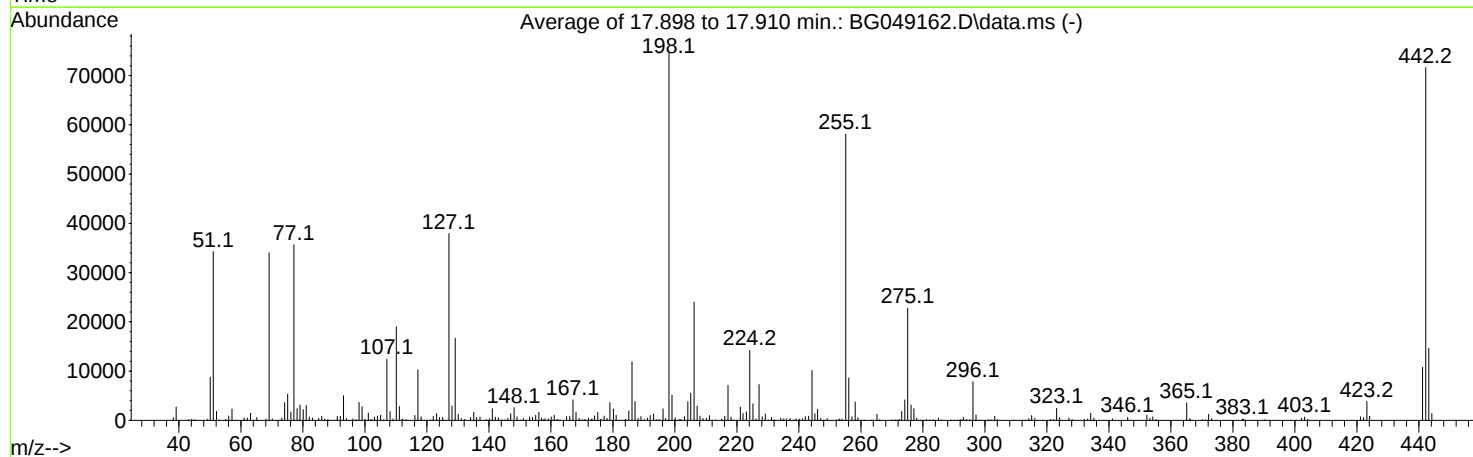


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070221\
 Data File : BG049162.D
 Acq On : 2 Jul 2021 11:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 30 15:39:12 2021

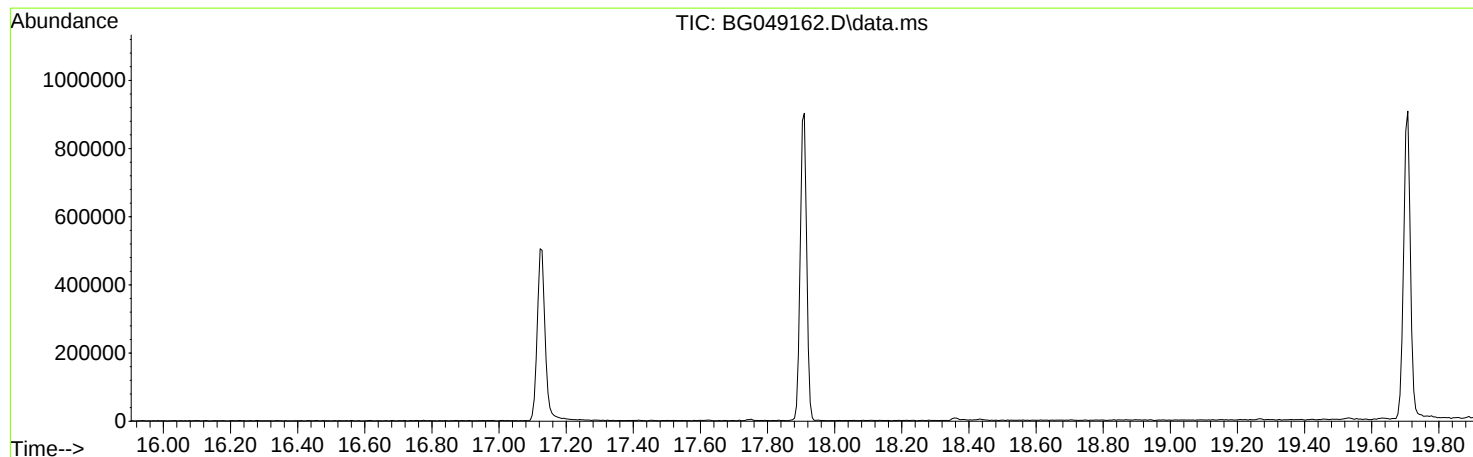

AutoFind: Scans 2529, 2530, 2531; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.9	34272	PASS
68	69	0.00	2	0.9	290	PASS
69	198	0.00	100	45.6	34024	PASS
70	69	0.00	2	0.8	286	PASS
127	198	10	80	50.8	37952	PASS
197	198	0.00	2	0.5	347	PASS
198	198	100	100	100.0	74693	PASS
199	198	5	9	6.9	5121	PASS
275	198	10	60	30.5	22777	PASS
365	198	1	100	4.7	3545	PASS
441	198	0.01	100	14.4	10791	PASS
442	442	100	100	100.0	71629	PASS
443	442	15	24	20.4	14609	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/2/2021	BNA_G	<u>BG049162.D</u>
Compound Name	Response	Retention Time
DDT	271697	20.94
DDD	4080	20.49
DDE	620	19.99
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4700	276397	1.70

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070221\
Data File : BG049162.D
Acq On : 2 Jul 2021 11:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 02 13:26:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 30 15:39:12 2021
Response via : Initial Calibration

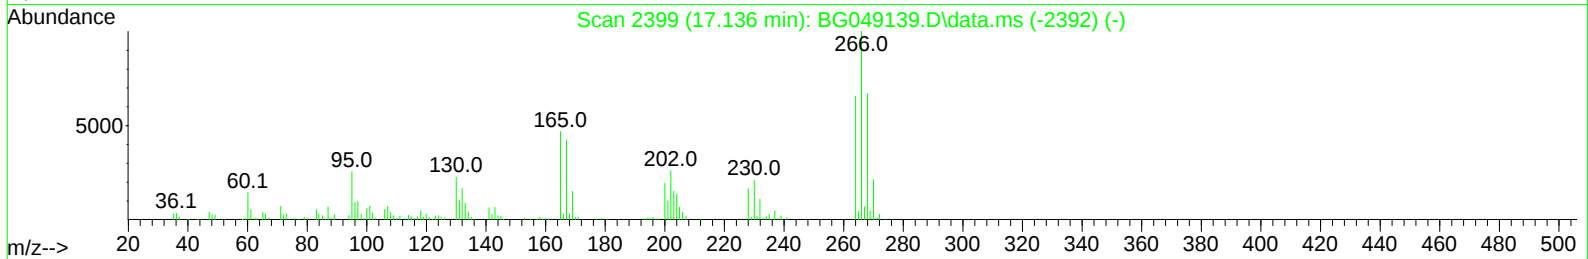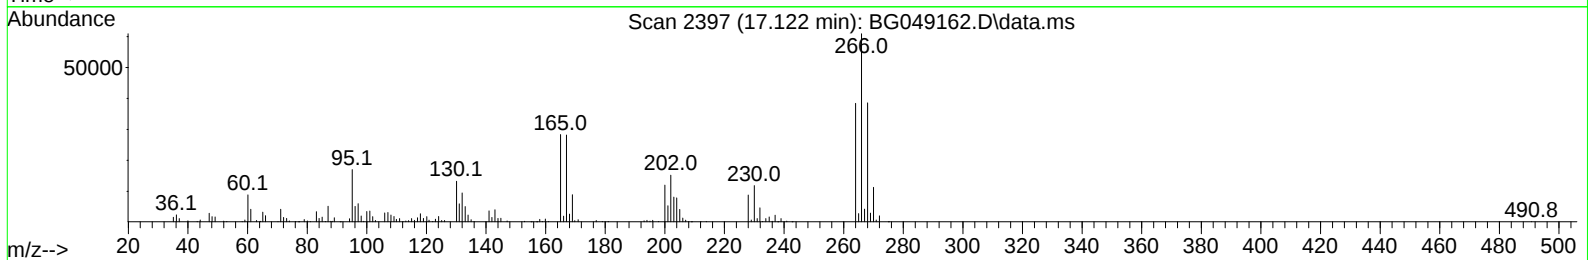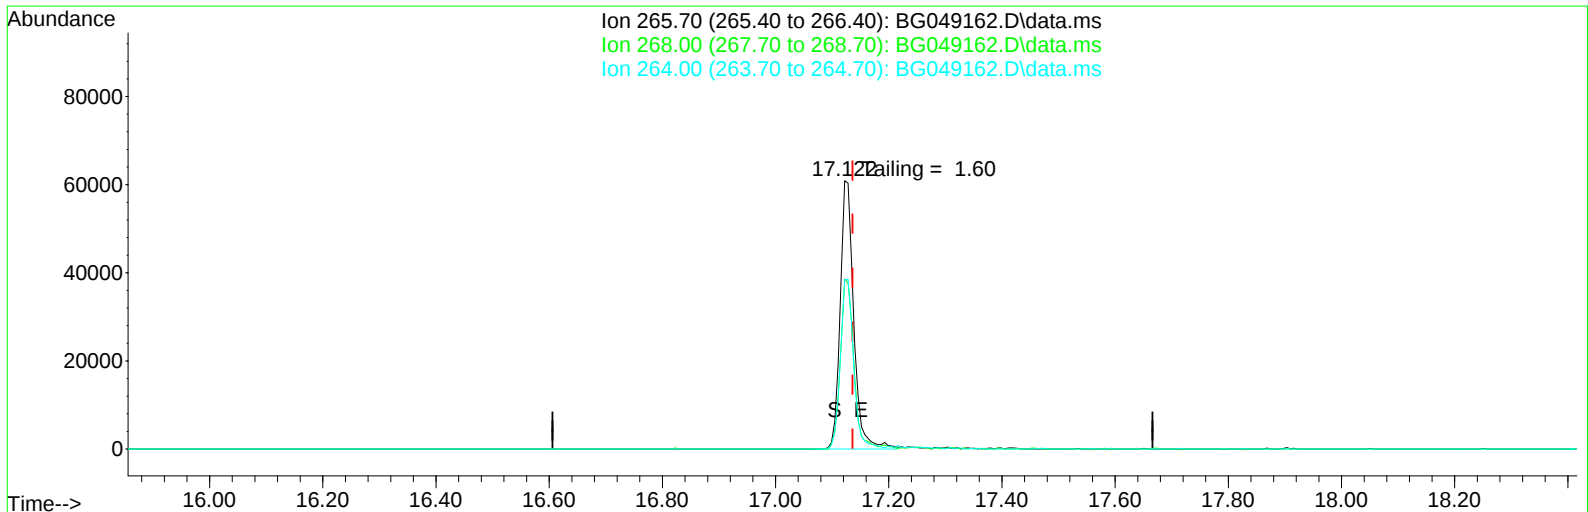

TIC: BG049162.D\data.ms

(70) Pentachlorophenol (C)

17.122min (-0.014) 208884.78 ng




response 99739

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.36
264.00	61.30	63.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070221\
 Data File : BG049162.D
 Acq On : 2 Jul 2021 11:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jul 02 13:26:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 30 15:39:12 2021
 Response via : Initial Calibration

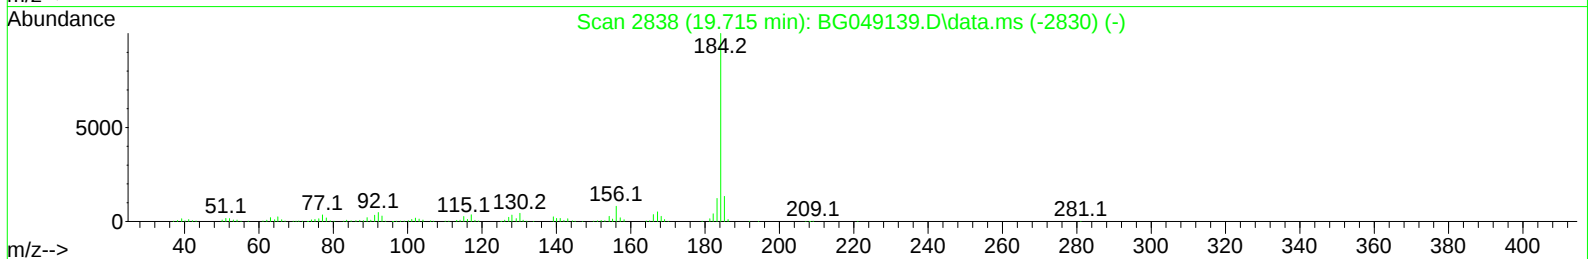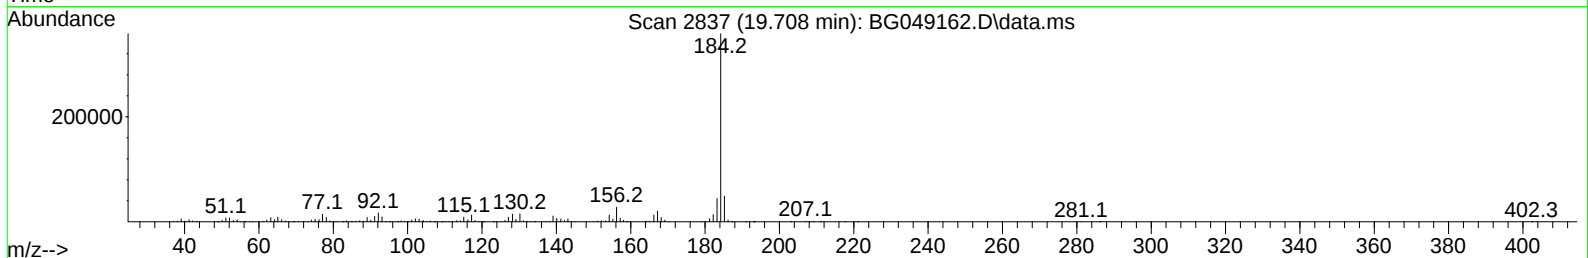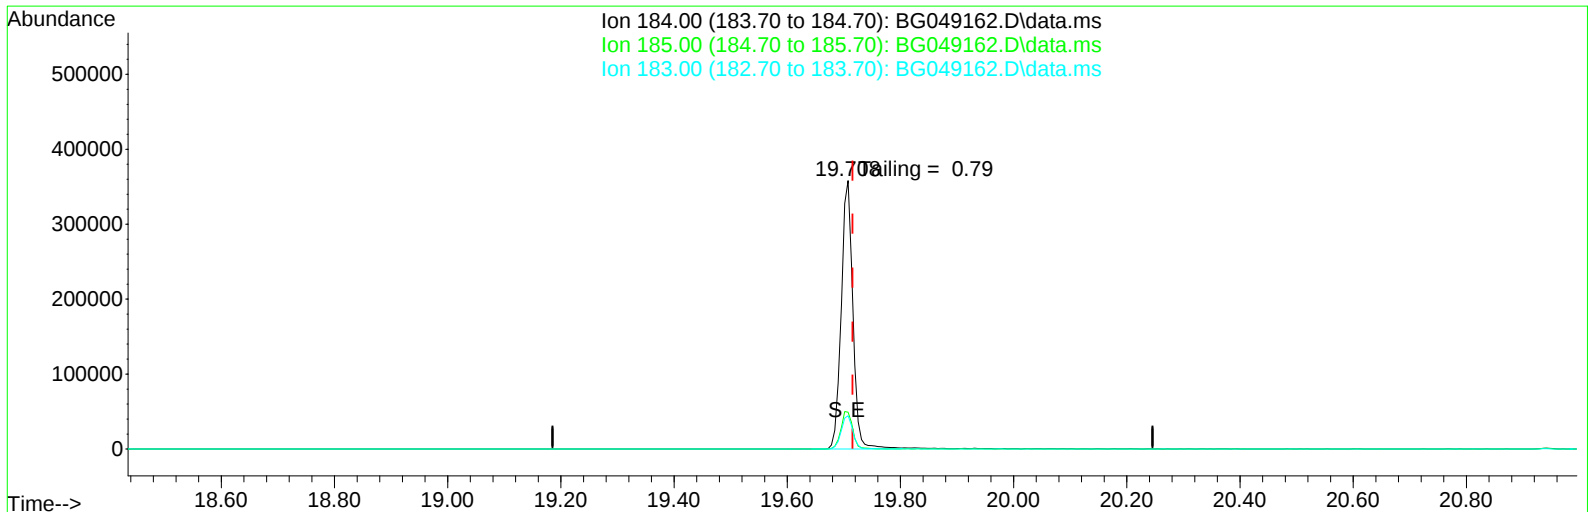

TIC: BG049162.D\data.ms

(77) Benzidine

19.708min (-0.008) 416348.75 ng

response 509754

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.74
183.00	11.70	12.42
0.00	0.00	0.00