

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070316\
 Data File : BG022825.D
 Acq On : 3 Jul 2016 11:53
 Operator : UM/SJ
 Sample : H3844-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jul 04 03:31:09 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 04 03:30:19 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	144554	20.00	ng/ul	0.00
18) Naphthalene-d8	10.98	136	612930	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.79	164	493750	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.55	188	1203612	20.00	ng/ul	0.00
75) Chrysene-d12	21.85	240	1400105	20.00	ng/ul	0.00
83) Perylene-d12	25.22	264	1446445	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.54	96	8194	3.17	ng/uL	0.00
5) Phenol-d5	7.30	99	389791	25.63	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	238199	27.78	ng/ul	0.00
9) 2-Chlorophenol-d4	7.68	132	257776	25.38	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	294287	24.92	ng/ul	0.00
19) Nitrobenzene-d5	9.32	128	134110	27.44	ng/ul	-0.01
22) 2-Nitrophenol-d4	10.06	143	167881	28.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.59	165	311757	25.29	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	394459	37.79	ng/ul	0.00
43) Dimethylphthalate-d6	14.19	166	1151432	28.71	ng/ul	0.00
46) Acenaphthylene-d8	14.49	160	1273578	27.70	ng/ul	-0.01
51) 4-Nitrophenol-d4	14.99	143	182209	28.93	ng/ul	0.00
57) Fluorene-d10	15.79	176	1069131	28.13	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	211046	27.26	ng/ul	-0.01
70) Anthracene-d10	17.65	188	1592949	28.47	ng/ul	0.00
76) Pyrene-d10	19.94	212	1912467	28.59	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.99	264	1950541	28.38	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.24	163	201774	4.93	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070316\
Data File : BG022825.D
Acq On : 3 Jul 2016 11:53
Operator : UM/SJ
Sample : H3844-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jul 04 03:31:09 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 04 03:30:19 2016
Response via : Initial Calibration

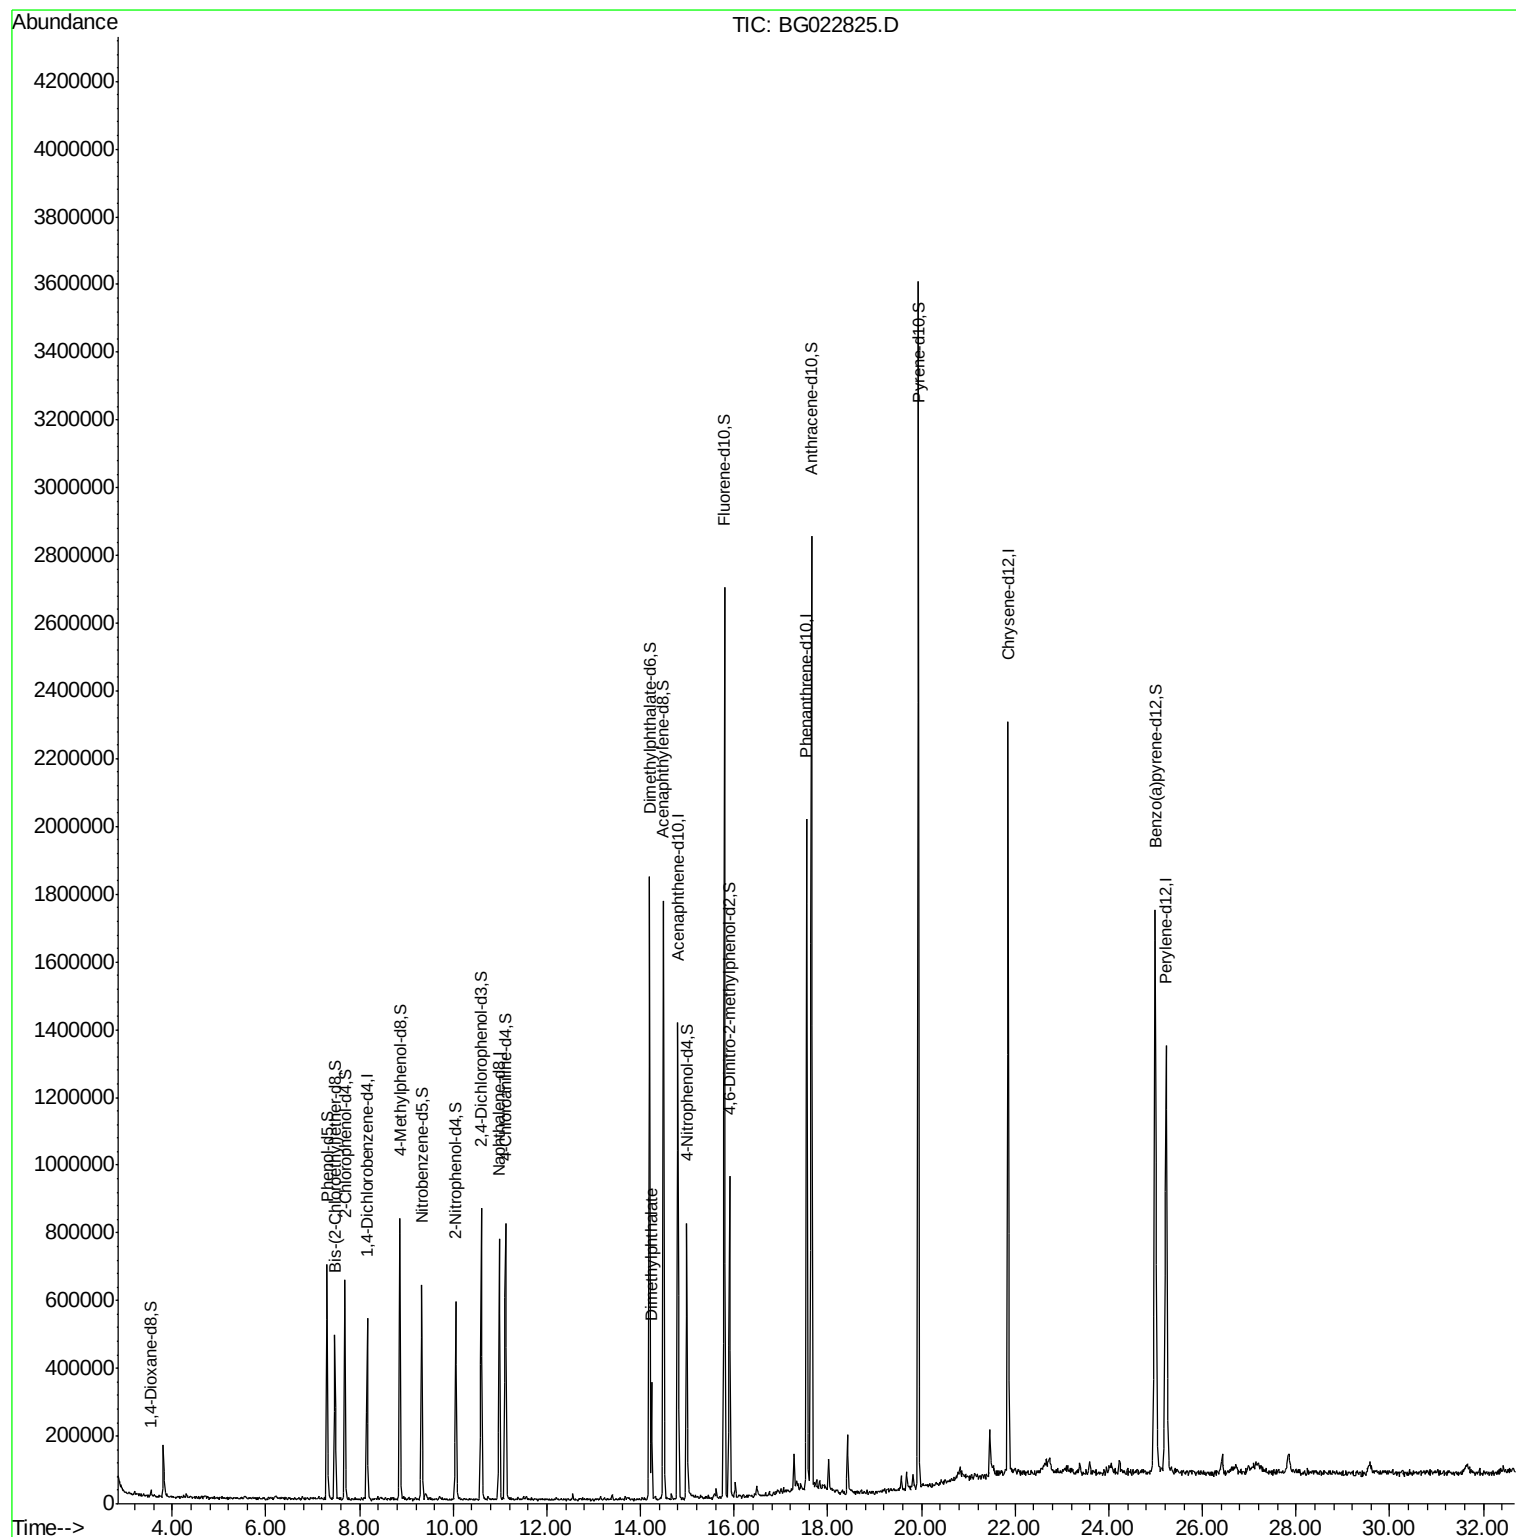

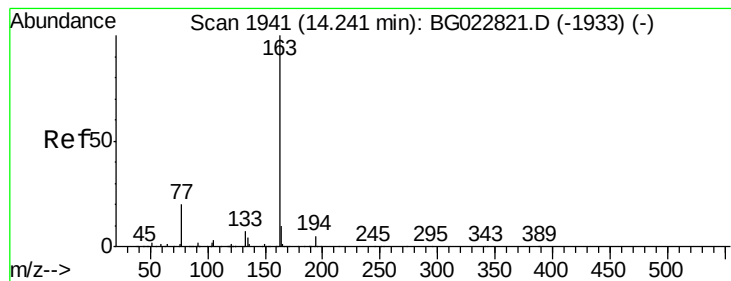

#44

Dimethylphthalate

Concen: 4.93 ng/ul

RT: 14.24 min Scan# 1940

Delta R.T. -0.01 min

Lab File: BG022825.D

Acq: 3 Jul 2016 11:53

Instrument :

BNA_G

ClientSampleId :


Tot Ion:163 Resp: 201774

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.2

164 10.2 8.8 13.2

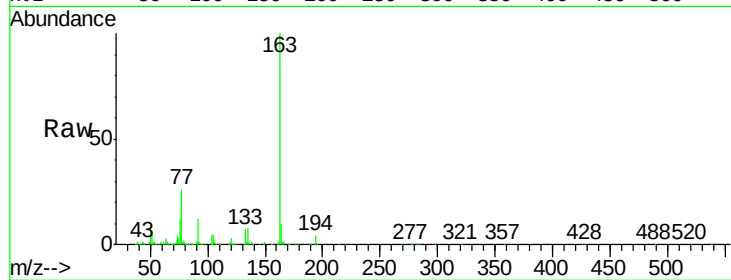

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

