

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070316\
 Data File : BG022836.D
 Acq On : 3 Jul 2016 19:52
 Operator : UM/SJ
 Sample : H3844-17
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jul 04 04:19:30 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 04 04:18:08 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	136934	20.00	ng/ul	0.00
18) Naphthalene-d8	10.99	136	632919	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.79	164	516025	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.55	188	1290079	20.00	ng/ul	0.00
75) Chrysene-d12	21.85	240	1495862	20.00	ng/ul	0.00
83) Perylene-d12	25.22	264	1531137	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.54	96	7745	3.16	ng/uL	0.00
5) Phenol-d5	7.30	99	395392	27.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	247880	30.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.68	132	253177	26.31	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	306077	27.36	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	137220	27.19	ng/ul	0.00
22) 2-Nitrophenol-d4	10.05	143	171545	28.18	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	331937	26.08	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	416524	38.64	ng/ul	0.00
43) Dimethylphthalate-d6	14.19	166	1212497	28.92	ng/ul	0.00
46) Acenaphthylene-d8	14.49	160	1360514	28.32	ng/ul	0.00
51) 4-Nitrophenol-d4	14.99	143	194281	29.52	ng/ul	0.00
57) Fluorene-d10	15.79	176	1157446	29.14	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	223634	26.95	ng/ul	0.00
70) Anthracene-d10	17.65	188	1713665	28.58	ng/ul	0.00
76) Pyrene-d10	19.93	212	2053946	28.74	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.99	264	2086931	28.69	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.24	163	262306	6.13	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070316\
Data File : BG022836.D
Acq On : 3 Jul 2016 19:52
Operator : UM/SJ
Sample : H3844-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jul 04 04:19:30 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 04 04:18:08 2016
Response via : Initial Calibration

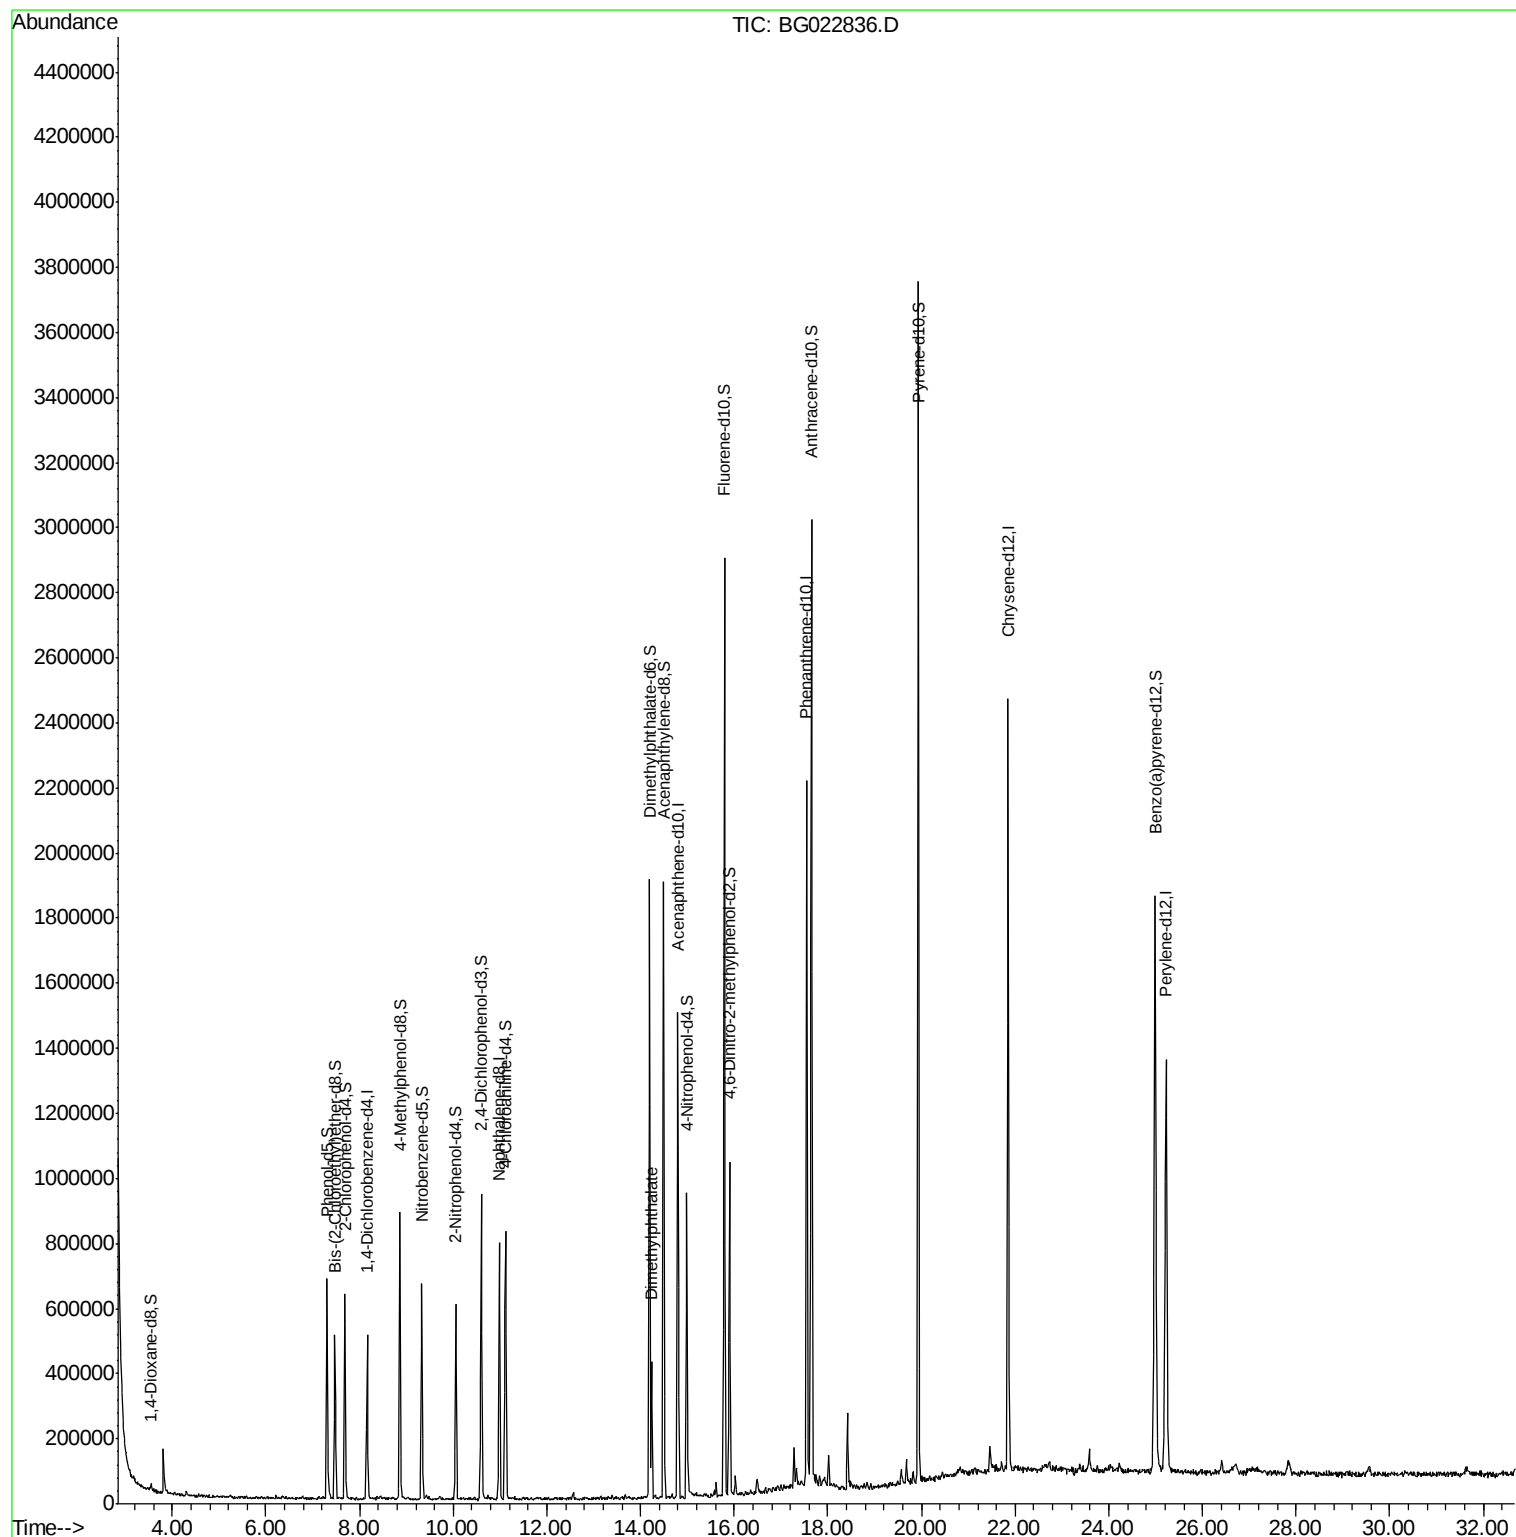

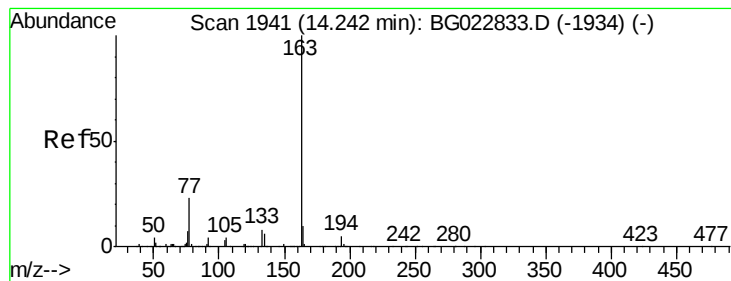

#44

Dimethylphthalate

Concen: 6.13 ng/ul

RT: 14.24 min Scan# 1941

Delta R.T. -0.00 min

Lab File: BG022836.D

Acq: 3 Jul 2016 19:52

Instrument :

BNA_G

ClientSampleId :


Tot Ion:163 Resp: 262306

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.2

164 10.0 8.8 13.2

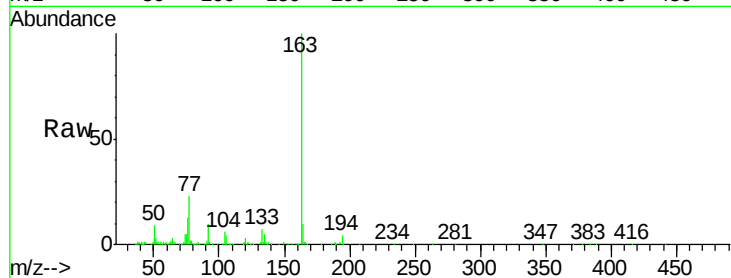

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

