

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070316\
 Data File : BG022832.D
 Acq On : 3 Jul 2016 16:32
 Operator : UM/SJ
 Sample : H3844-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHZ3

Quant Time: Jul 04 03:32:17 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 04 03:30:19 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	163568	20.00	ng/ul	0.00
18) Naphthalene-d8	10.98	136	726517	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.79	164	554031	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.55	188	1285212	20.00	ng/ul	0.00
75) Chrysene-d12	21.85	240	1428530	20.00	ng/ul	0.00
83) Perylene-d12	25.22	264	1474833	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.54	96	7108	2.43	ng/uL	0.00
5) Phenol-d5	7.30	99	433603	25.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	274201	28.26	ng/ul	0.00
9) 2-Chlorophenol-d4	7.68	132	293372	25.53	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	342525	25.63	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	157064	27.11	ng/ul	0.00
22) 2-Nitrophenol-d4	10.05	143	190841	27.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.59	165	364797	24.97	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	449791	36.35	ng/ul	0.00
43) Dimethylphthalate-d6	14.19	166	1278283	28.40	ng/ul	0.00
46) Acenaphthylene-d8	14.49	160	1442384	27.96	ng/ul	0.00
51) 4-Nitrophenol-d4	14.99	143	203156	28.75	ng/ul	0.00
57) Fluorene-d10	15.79	176	1201891	28.18	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	230903	27.93	ng/ul	-0.01
70) Anthracene-d10	17.65	188	1730753	28.97	ng/ul	0.00
76) Pyrene-d10	19.93	212	2003574	29.36	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.99	264	2062756	29.44	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.24	163	183264	3.99	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070316\
Data File : BG022832.D
Acq On : 3 Jul 2016 16:32
Operator : UM/SJ
Sample : H3844-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDHZ3

Quant Time: Jul 04 03:32:17 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 04 03:30:19 2016
Response via : Initial Calibration

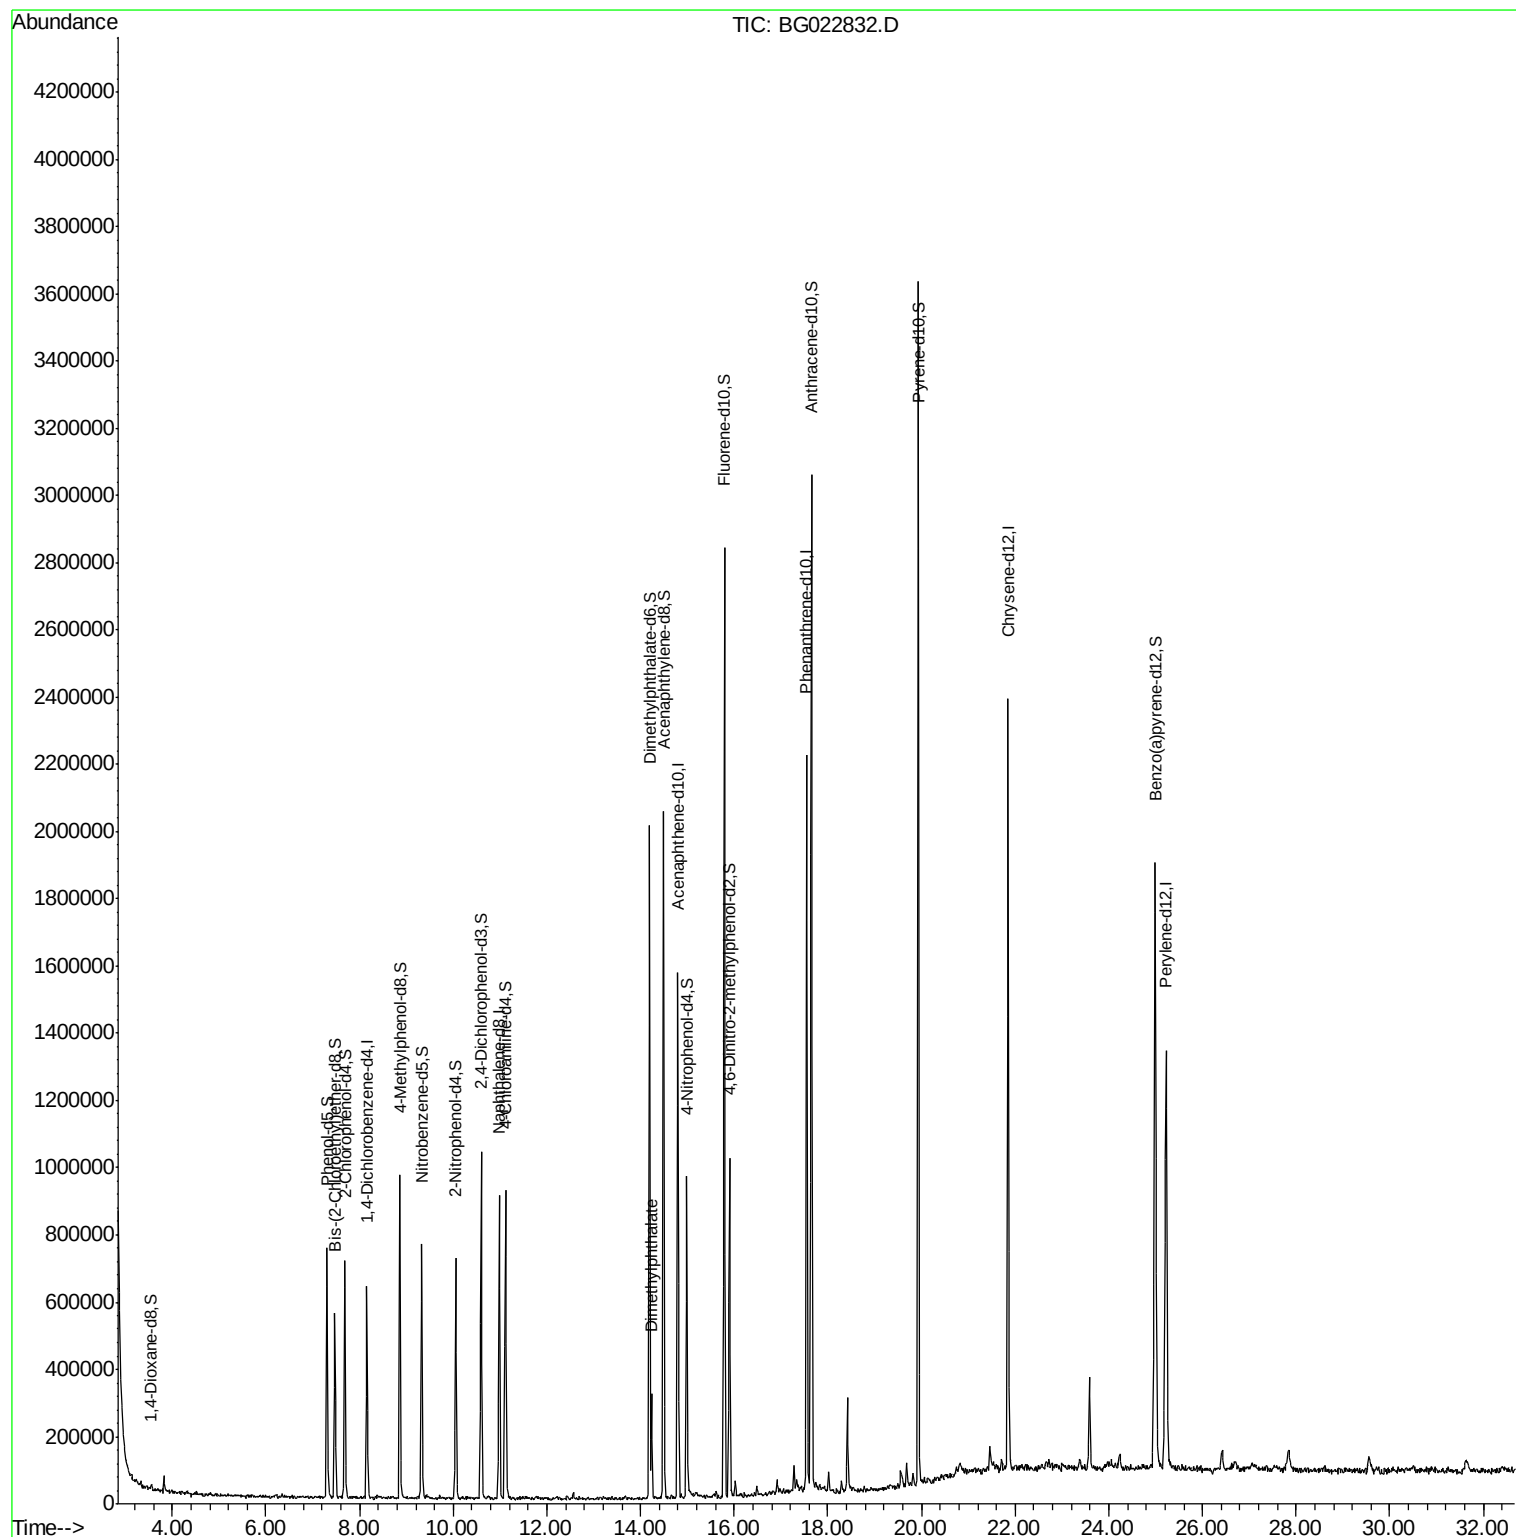

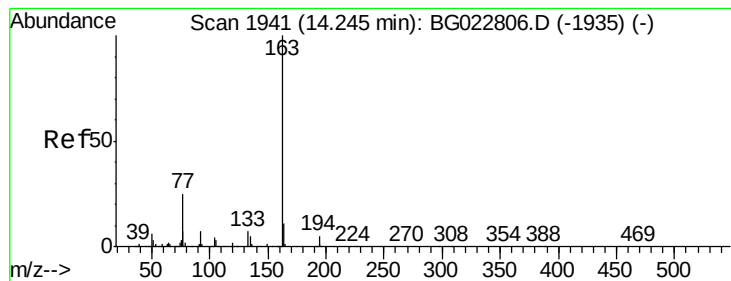

#44

Dimethylphthalate

Concen: 3.99 ng/ul

RT: 14.24 min Scan# 1940

Delta R.T. -0.01 min

Lab File: BG022832.D

Acq: 3 Jul 2016 16:32

Instrument :

BNA_G

ClientSampleId :

BDHZ3


Tot Ion:163 Resp: 183264

Ion Ratio Lower Upper

163 100

194 3.6 3.4 5.2

164 11.1 8.8 13.2

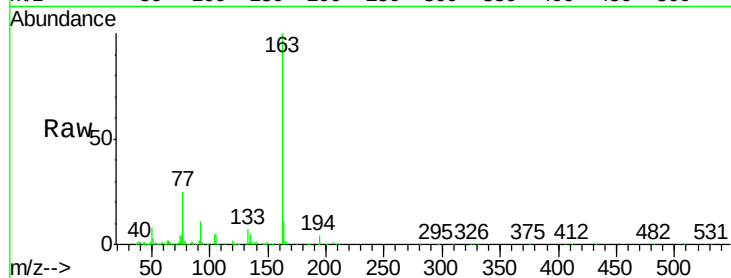

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

