

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070316\
 Data File : BG022834.D
 Acq On : 3 Jul 2016 18:32
 Operator : UM/SJ
 Sample : H3844-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHZ4

Manual Integrations

umangi
 7/5/2016 7:55:12 PM

Quant Time: Jul 04 04:22:37 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 04 04:18:08 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	140011	20.00	ng/ul	0.00
18) Naphthalene-d8	10.98	136	646123	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.80	164	516111	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.55	188	1229556m	20.00	ng/ul	0.00
75) Chrysene-d12	21.85	240	1389727	20.00	ng/ul	0.00
83) Perylene-d12	25.23	264	1419606	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.54	96	6926	2.76	ng/uL	0.00
5) Phenol-d5	7.31	99	469554	31.88	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.48	67	295108	35.53	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	306209	31.13	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	369262	32.28	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	171251	33.24	ng/ul	0.00
22) 2-Nitrophenol-d4	10.06	143	202950	32.65	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	395966	30.47	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	493662	44.86	ng/ul	0.00
43) Dimethylphthalate-d6	14.20	166	1349574	32.19	ng/ul	0.00
46) Acenaphthylene-d8	14.50	160	1555498	32.37	ng/ul	0.00
51) 4-Nitrophenol-d4	14.99	143	218851	33.24	ng/ul	0.00
57) Fluorene-d10	15.79	176	1298089	32.68	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	249707m	31.58	ng/ul	0.00
70) Anthracene-d10	17.65	188	1820306	31.85	ng/ul	0.00
76) Pyrene-d10	19.93	212	2141503	32.26	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.99	264	2223479	32.97	ng/ul	0.00

Target Compounds					Ovalue
44) Dimethylphthalate	14.25	163	191003	4.46 ng/ul#	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG070316\
Data File : BG022834.D
Acq On : 3 Jul 2016 18:32
Operator : UM/SJ
Sample : H3844-15
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BDHZ4

Manual Integrations

Quant Time: Jul 04 04:22:37 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 04 04:18:08 2016
Response via : Initial Calibration

umangi
7/5/2016 7:55:12 PM

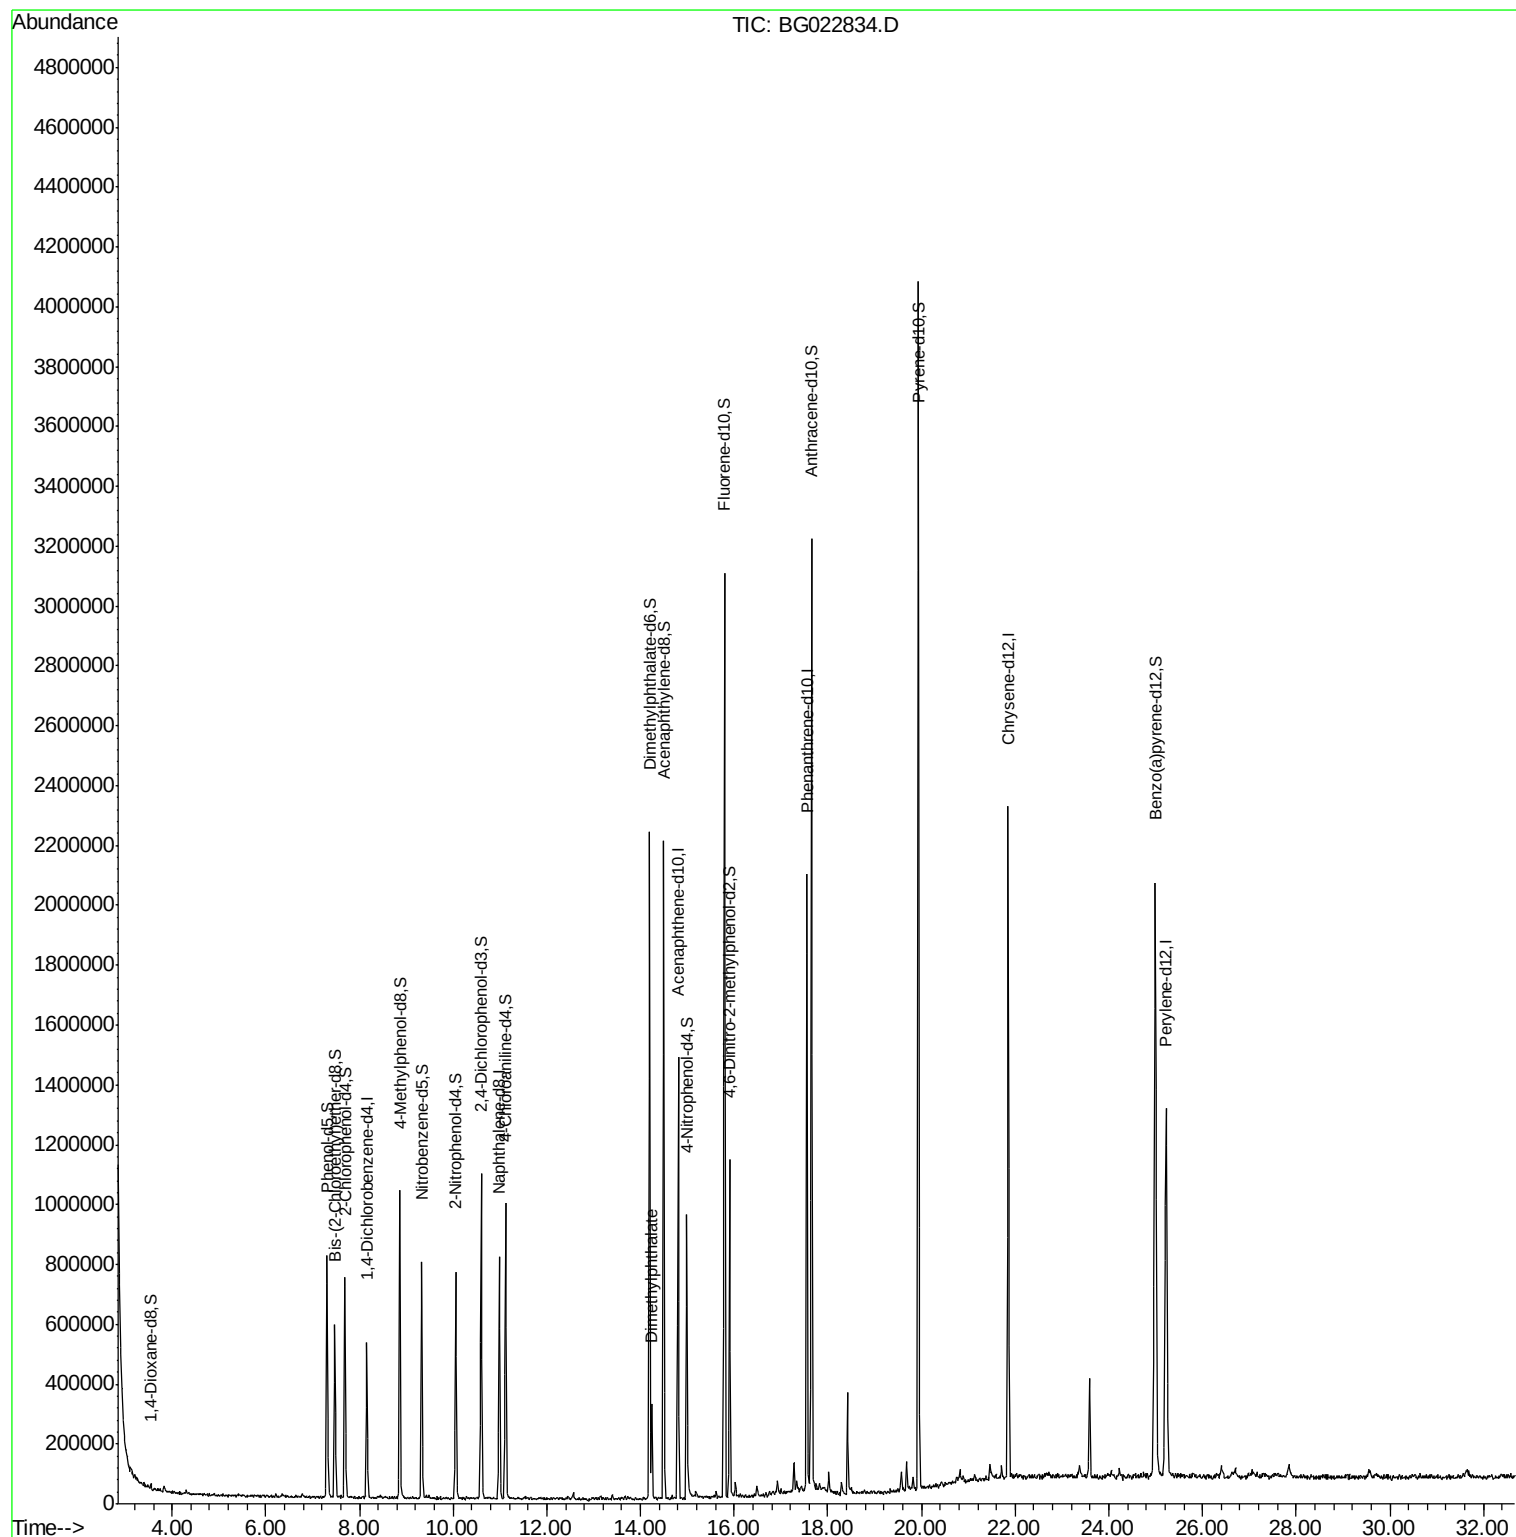

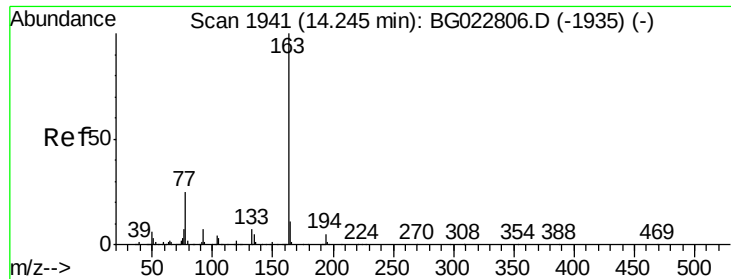

#44
 Dimethylphthalate
 Concen: 4.46 ng/ul
 RT: 14.25 min Scan# 1941
 Delta R.T. 0.00 min
 Lab File: BG022834.D
 Acq: 3 Jul 2016 18:32

Instrument :
 BNA_G
 ClientSampleId :
 BDHZ4

Tot Ion	Ratio	Resp	Lower	Upper
163	100	191003		
194	4.4		3.4	5.2
164	8.7		8.8	13.2#

Manual Integrations

umangi
 7/5/2016 7:55:12 PM

