

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070316\
 Data File : BG022837.D
 Acq On : 3 Jul 2016 20:32
 Operator : UM/SJ
 Sample : H3844-18
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHZ7

Manual Integrations

umangi
 7/5/2016 7:55:05 PM

Quant Time: Jul 04 04:27:09 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 04 04:18:08 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	161025	20.00	ng/ul	0.00
18) Naphthalene-d8	10.98	136	683974	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.80	164	561257	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.55	188	1368600m	20.00	ng/ul	0.00
75) Chrysene-d12	21.85	240	1560691m	20.00	ng/ul	0.00
83) Perylene-d12	25.23	264	1590382	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.54	96	8500	2.95	ng/uL	0.00
5) Phenol-d5	7.31	99	458127	27.05	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.48	67	286305	29.98	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	302572	26.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	353423	26.86	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	157207	28.82	ng/ul	0.00
22) 2-Nitrophenol-d4	10.05	143	192456	29.25	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	381003	27.70	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	480548	41.25	ng/ul	0.00
43) Dimethylphthalate-d6	14.20	166	1348078	29.57	ng/ul	0.00
46) Acenaphthylene-d8	14.50	160	1517123	29.03	ng/ul	0.00
51) 4-Nitrophenol-d4	14.99	143	225680	31.52	ng/ul	0.00
57) Fluorene-d10	15.80	176	1292462	29.92	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.91	200	264244m	30.02	ng/ul	0.00
70) Anthracene-d10	17.65	188	1895608	29.80	ng/ul	0.00
76) Pyrene-d10	19.93	212	2218130	29.75	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.00	264	2333139	30.88	ng/ul	0.00

Target Compounds					Ovalue
44) Dimethylphthalate	14.24	163	195612	4.20 ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG070316\
Data File : BG022837.D
Acq On : 3 Jul 2016 20:32
Operator : UM/SJ
Sample : H3844-18
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BDHZ7

Manual Integrations

umangi
7/5/2016 7:55:05 PM

Quant Time: Jul 04 04:27:09 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 04 04:18:08 2016
Response via : Initial Calibration

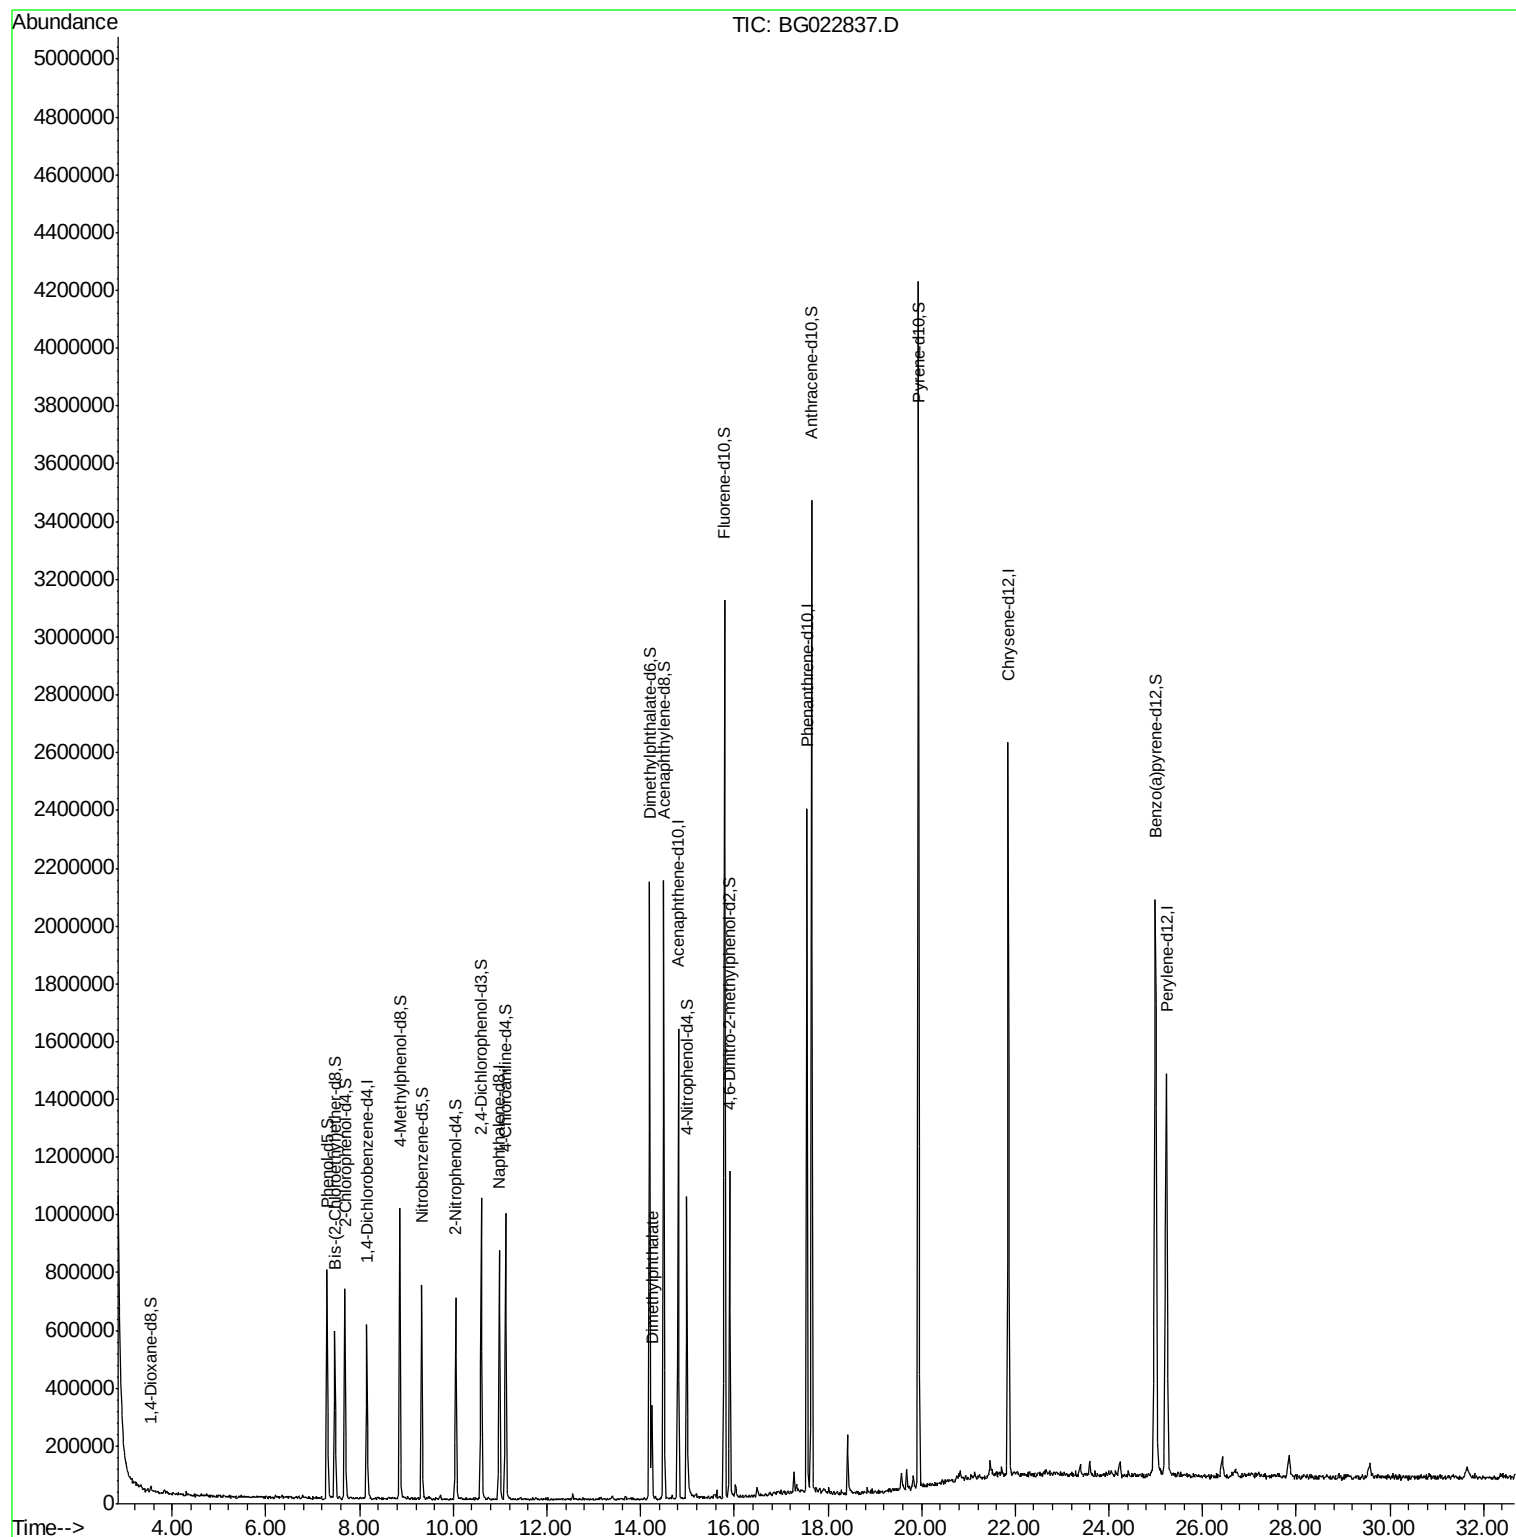

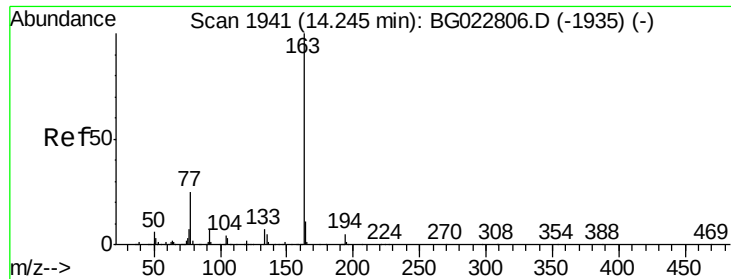

#44
 Dimethylphthalate
 Concen: 4.20 ng/ul
 RT: 14.24 min Scan# 1941
 Delta R.T. 0.00 min
 Lab File: BG022837.D
 Acq: 3 Jul 2016 20:32

Instrument :
 BNA_G
 ClientSampleId :
 BDHZ7

Tot Ion:	163	Resp:	195612
Ion Ratio	Lower	Upper	
163	100		
194	4.6	3.4	5.2
164	12.3	8.8	13.2

Manual Integrations

umangi
 7/5/2016 7:55:05 PM

