

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070316\
 Data File : BG022836.D
 Acq On : 3 Jul 2016 19:52
 Operator : UM/SJ
 Sample : H3844-17
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHZ6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.542	118	120	121	rBV2	14132	7557	0.13%	0.013%
2	3.672	140	142	145	rBV4	10837	9910	0.18%	0.017%
3	3.813	162	166	177	rBV	130968	196668	3.49%	0.337%
4	4.294	244	248	249	rBV3	14622	13708	0.24%	0.023%
5	4.559	291	293	297	rBV3	8299	8471	0.15%	0.015%
6	5.323	421	423	426	rVB4	7015	7559	0.13%	0.013%
7	5.910	521	523	526	rVB4	8164	7487	0.13%	0.013%
8	5.957	526	531	533	rBV3	6577	9187	0.16%	0.016%
9	6.216	571	575	578	rVB3	12315	17027	0.30%	0.029%
10	6.292	586	588	594	rVB4	4323	7490	0.13%	0.013%
11	6.345	594	597	599	rBV3	10469	11733	0.21%	0.020%
12	6.721	657	661	663	rBV5	7010	7332	0.13%	0.013%
13	7.303	753	760	770	rBV	677155	1249760	22.20%	2.141%
14	7.473	783	789	798	rBV	505892	825839	14.67%	1.415%
15	7.685	819	825	833	rBV	629832	1123857	19.96%	1.926%
16	8.161	893	906	914	rBV	506257	941852	16.73%	1.614%
17	8.443	949	954	955	rBV3	7194	9972	0.18%	0.017%
18	8.689	993	996	1000	rBV6	7229	10187	0.18%	0.017%
19	8.860	1016	1025	1033	rBV2	880535	1528253	27.14%	2.619%
20	9.330	1098	1105	1112	rBV	661705	1204667	21.40%	2.064%
21	9.430	1118	1122	1125	rVB6	12257	17729	0.31%	0.030%
22	9.477	1129	1130	1136	rVB4	11847	12993	0.23%	0.022%
23	9.559	1141	1144	1147	rBV4	7127	8581	0.15%	0.015%
24	9.717	1166	1171	1176	rVB6	12151	24573	0.44%	0.042%
25	9.958	1208	1212	1214	rBV3	5709	8325	0.15%	0.014%
26	10.052	1221	1228	1236	rVB	597820	1102060	19.57%	1.888%
27	10.364	1278	1281	1284	rBV5	6726	10410	0.18%	0.018%
28	10.599	1312	1321	1330	rBV	938974	1685832	29.94%	2.889%
29	10.734	1340	1344	1349	rBV5	11984	20518	0.36%	0.035%
30	10.928	1375	1377	1380	rBV4	6563	8134	0.14%	0.014%
31	10.987	1380	1387	1395	rVB	789086	1438707	25.55%	2.465%
32	11.116	1401	1409	1420	rBV	826260	1610041	28.59%	2.759%
33	11.480	1468	1471	1472	rBV3	6575	7202	0.13%	0.012%
34	11.498	1472	1474	1479	rVB5	6268	8670	0.15%	0.015%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070316\
 Data File : BG022836.D
 Acq On : 3 Jul 2016 19:52
 Operator : UM/SJ
 Sample : H3844-17
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHZ6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
 Title : SVOA CALIBRATION

35	11.974	1553	1555	1559	rBV4	7453	10824	0.19%	0.019%
36	12.326	1611	1615	1616	rBV3	5837	7438	0.13%	0.013%
37	12.438	1630	1634	1637	rBV3	8182	9747	0.17%	0.017%
38	12.561	1649	1655	1661	rBV4	22974	46655	0.83%	0.080%
39	13.143	1750	1754	1759	rBV5	11199	19190	0.34%	0.033%
40	13.302	1778	1781	1782	rBV2	9691	9716	0.17%	0.017%
41	13.390	1793	1796	1800	rVB5	11658	15061	0.27%	0.026%
42	13.443	1802	1805	1806	rBV3	7195	7903	0.14%	0.014%
43	13.660	1840	1842	1843	rBV	14318	11747	0.21%	0.020%
44	13.930	1886	1888	1891	rBV3	6064	7472	0.13%	0.013%
45	14.195	1926	1933	1937	rBV	1897167	2874240	51.05%	4.925%
46	14.242	1937	1941	1948	rVB	420971	641624	11.40%	1.099%
47	14.312	1948	1953	1956	rBV7	13857	24331	0.43%	0.042%
48	14.424	1969	1972	1976	rBV6	5881	9892	0.18%	0.017%
49	14.494	1976	1984	1992	rVV	1893164	3113677	55.30%	5.335%
50	14.612	2002	2004	2007	rVB3	6797	8663	0.15%	0.015%
51	14.671	2011	2014	2020	rVB7	14874	22282	0.40%	0.038%
52	14.800	2028	2036	2043	rVB2	1493800	2500610	44.41%	4.285%
53	14.988	2060	2068	2077	rBV	939088	1614237	28.67%	2.766%
54	15.575	2164	2168	2171	rBV5	18487	25912	0.46%	0.044%
55	15.616	2171	2175	2180	rVB3	45044	53665	0.95%	0.092%
56	15.787	2197	2204	2215	rBV	2882622	4410053	78.32%	7.556%
57	15.898	2217	2223	2232	rBV	1025230	1503961	26.71%	2.577%
58	16.028	2240	2245	2251	rVB4	58788	97517	1.73%	0.167%
59	16.227	2276	2279	2280	rBV2	6551	7552	0.13%	0.013%
60	16.480	2319	2322	2325	rBV3	40750	54908	0.98%	0.094%
61	16.815	2376	2379	2380	rBV3	13452	14345	0.25%	0.025%
62	16.886	2389	2391	2393	rVB2	13324	9938	0.18%	0.017%
63	16.927	2393	2398	2405	rBV2	17133	44140	0.78%	0.076%
64	16.997	2406	2410	2414	rVB6	16802	26921	0.48%	0.046%
65	17.279	2452	2458	2461	rBV	126437	175156	3.11%	0.300%
66	17.326	2464	2466	2470	rVB4	51843	66235	1.18%	0.113%
67	17.549	2497	2504	2512	rBV	2161431	3380236	60.03%	5.792%
68	17.649	2514	2521	2529	rVB	2946972	4689878	83.29%	8.036%
69	17.749	2536	2538	2546	rVB9	34170	54808	0.97%	0.094%
70	18.020	2580	2584	2590	rVB3	95286	131658	2.34%	0.226%
71	18.419	2647	2652	2658	rBV	227499	326980	5.81%	0.560%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070316\
Data File : BG022836.D
Acq On : 3 Jul 2016 19:52
Operator : UM/SJ
Sample : H3844-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDHZ6

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Title : SVOA CALIBRATION

72	18.490	2662	2664	2667	rBV3	16233	13779	0.24%	0.024%
73	19.565	2843	2847	2851	rBV2	46706	80460	1.43%	0.138%
74	19.682	2864	2867	2871	rVB2	67331	73661	1.31%	0.126%
75	19.817	2887	2890	2898	rVB2	38249	73847	1.31%	0.127%
76	19.935	2903	2910	2918	rVV	3682308	5630583	100.00%	9.648%
77	21.457	3165	3169	3178	rBV10	75448	191781	3.41%	0.329%
78	21.850	3229	3236	3243	rBV2	2367967	4094255	72.71%	7.015%
79	24.988	3760	3770	3784	rVB3	1750514	5220951	92.72%	8.946%
80	25.223	3800	3810	3821	rVB2	1253111	3791494	67.34%	6.496%


Sum of corrected areas: 58362274

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070316\
Data File : BG022836.D
Acq On : 3 Jul 2016 19:52
Operator : UM/SJ
Sample : H3844-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDHZ6

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

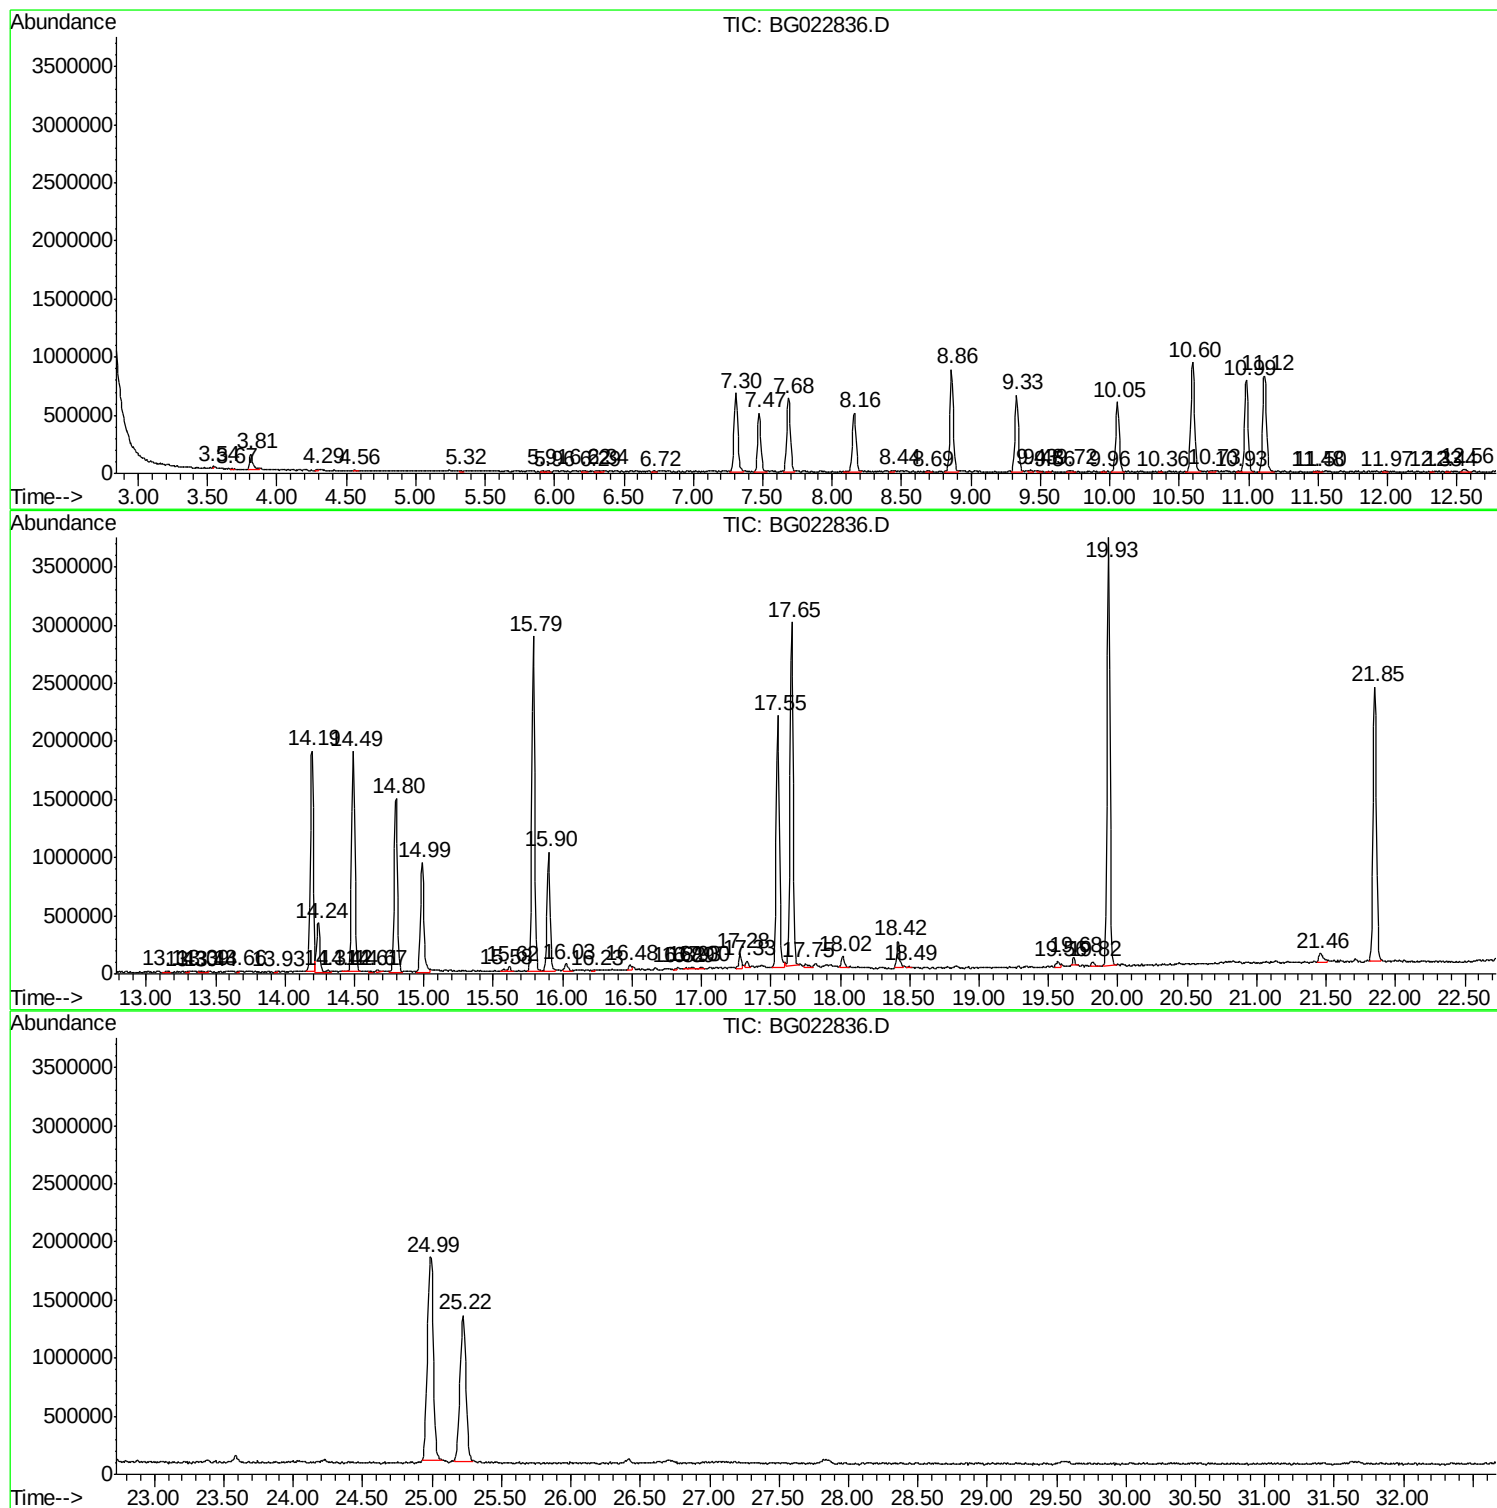

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070316\
Data File : BG022836.D
Acq On : 3 Jul 2016 19:52
Operator : UM/SJ
Sample : H3844-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDHZ6

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070316\
Data File : BG022836.D
Acq On : 3 Jul 2016 19:52
Operator : UM/SJ
Sample : H3844-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDHZ6

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc