


Data Path : Z:\HPCHEM1\BNA_G\Data\BG070317\
 Data File : BG027829.D
 Acq On : 3 Jul 2017 12:57
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 28 19:26:37 2017

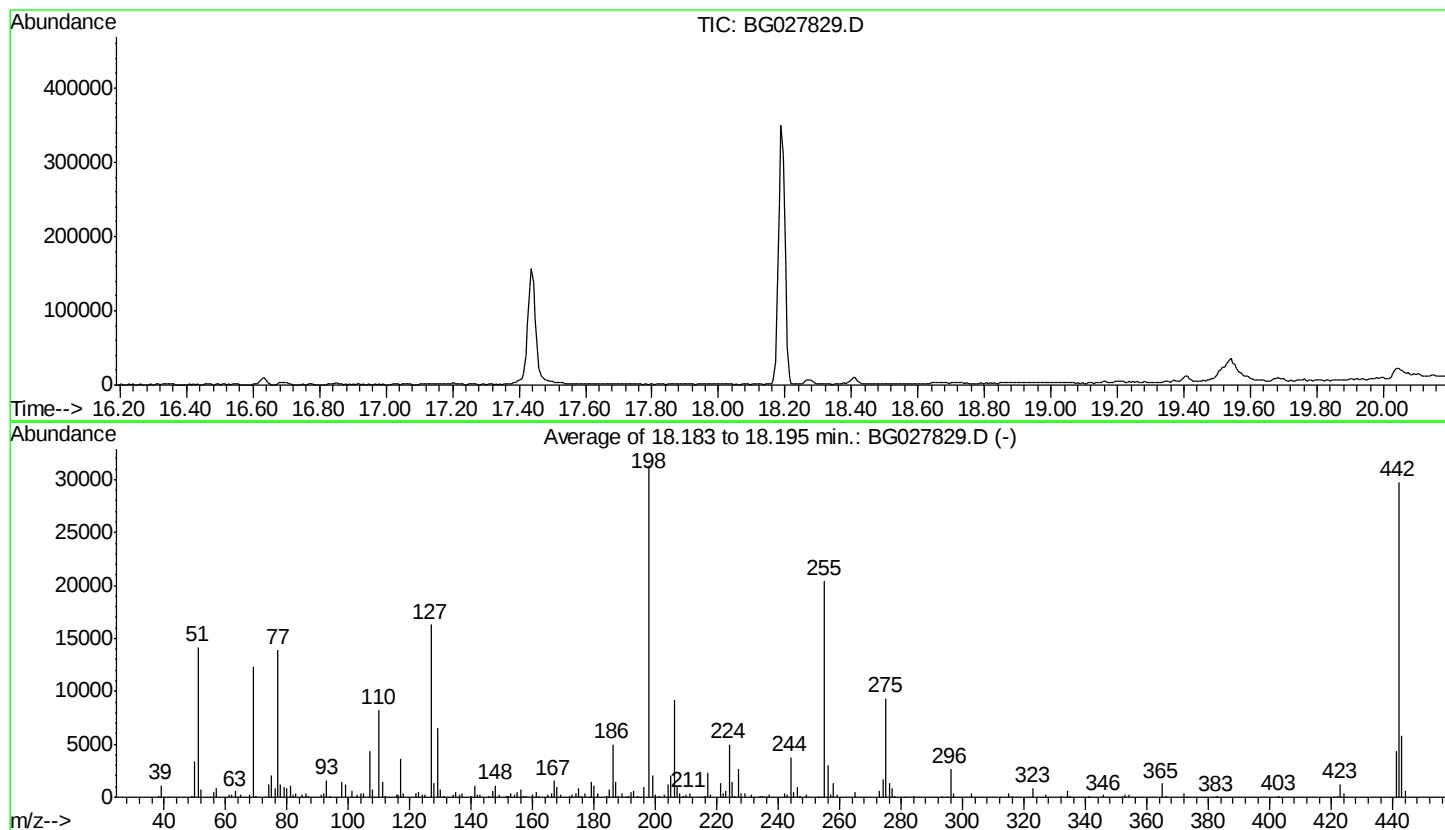

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.3	14173	PASS
68	69	0.00	2	1.6	194	PASS
69	198	0.00	100	39.3	12298	PASS
70	69	0.00	2	0.9	109	PASS
127	198	10	80	52.1	16303	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	31317	PASS
199	198	5	9	6.7	2108	PASS
275	198	10	60	29.8	9336	PASS
365	198	1	100	4.1	1277	PASS
441	442	0.01	24	14.7	4387	PASS
442	198	50	100	95.0	29757	PASS
443	442	15	24	19.5	5813	PASS