
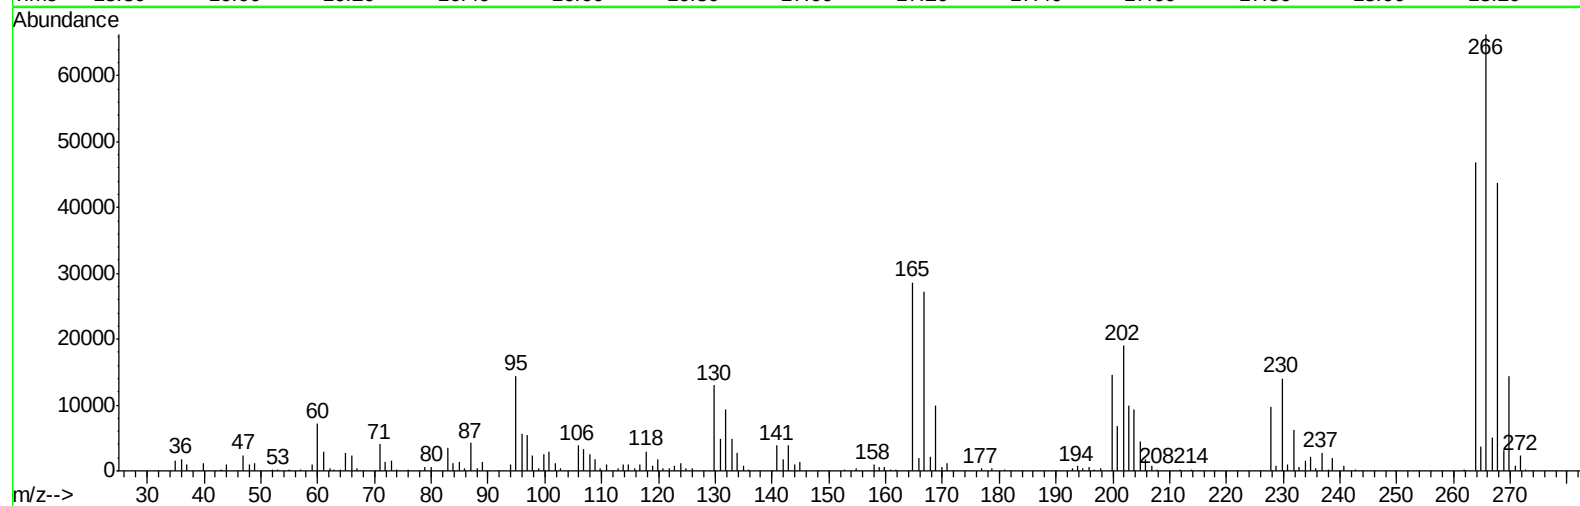


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070319\
Data File : BG041590.D
Acq On : 3 Jul 2019 14:38
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 04 06:39:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG062619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:25:55 2019
Response via : Initial Calibration

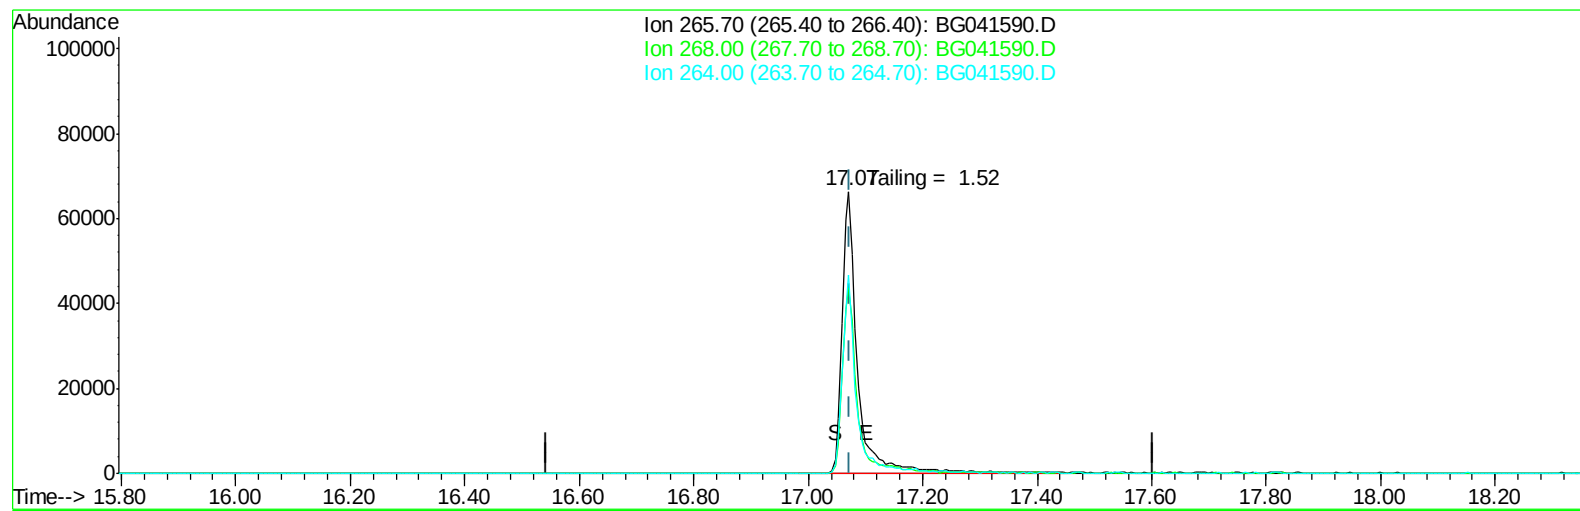

TIC: BG041590.D

(70) Pentachlorophenol (C)



17.071min (-0.003) 16680.55ng

response 121633

Ion	Exp%	Act%
265.70	100	100
268.00	58.70	66.01
264.00	59.20	70.54
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070319\
Data File : BG041590.D
Acq On : 3 Jul 2019 14:38
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 04 06:39:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG062619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:25:55 2019
Response via : Initial Calibration

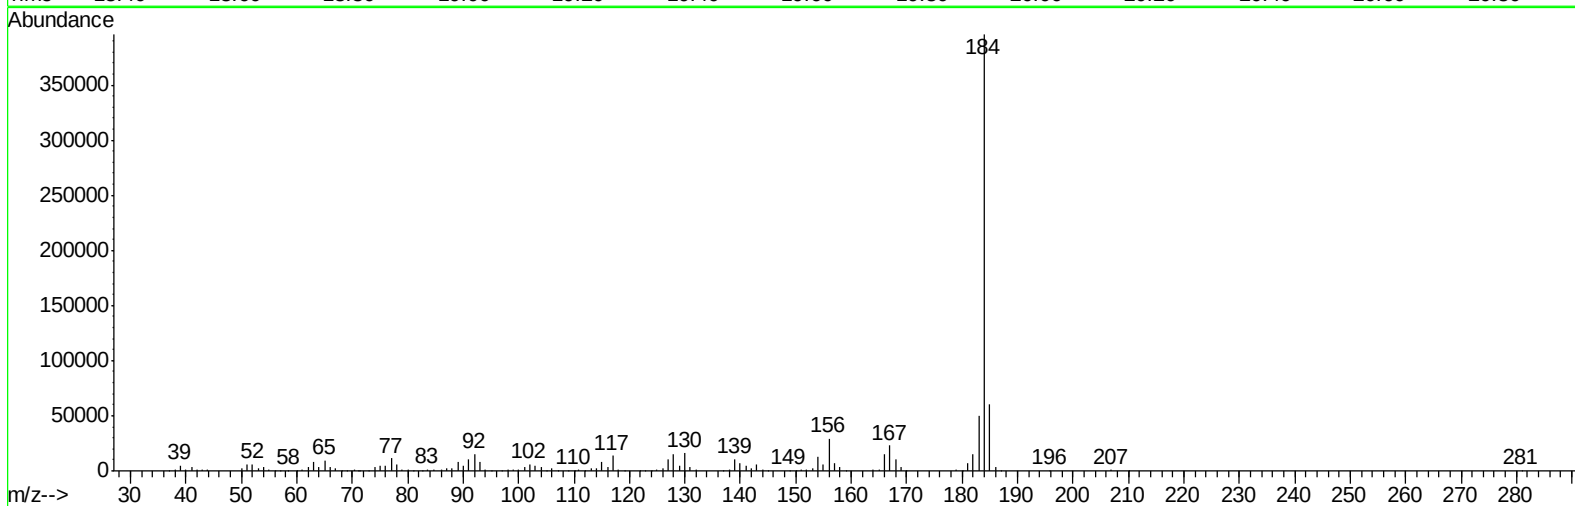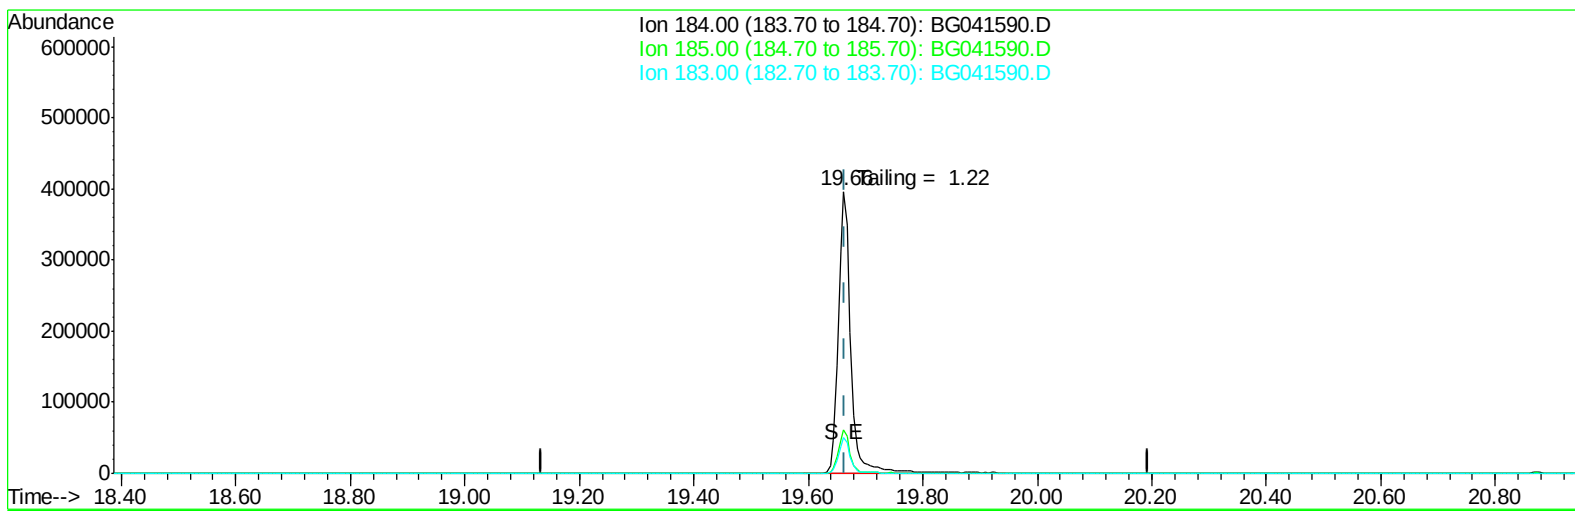

TIC: BG041590.D

(77) Benzidine

19.662min (-0.003) 10008.51ng

response 604247

Ion	Exp%	Act%
184.00	100	100
185.00	15.90	15.27
183.00	11.80	12.52
0.00	0.00	0.00