


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070319\
 Data File : BG041583.D
 Acq On : 3 Jul 2019 10:07
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG062619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 27 13:25:55 2019

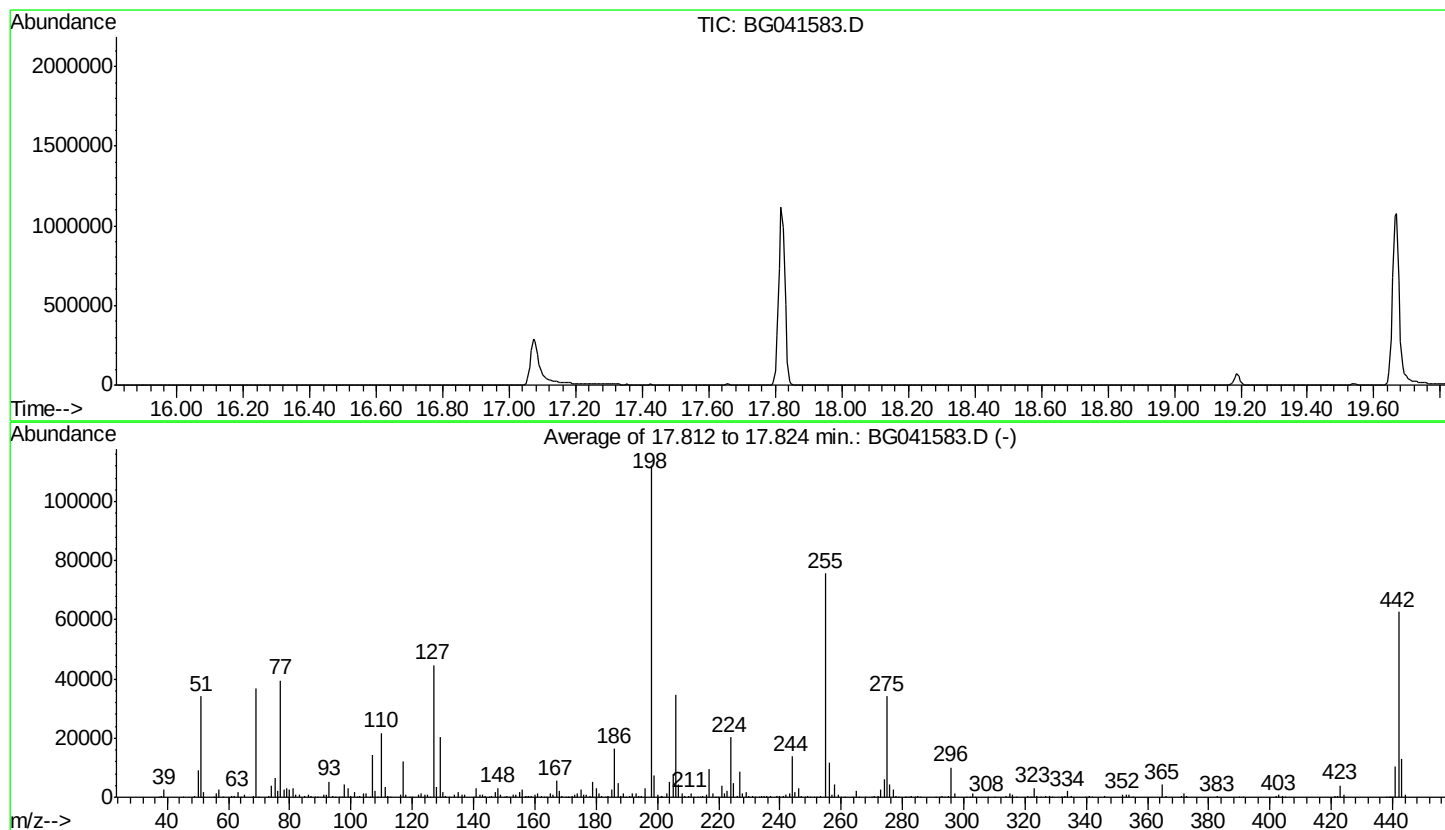

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.3	34021	PASS
68	69	0.00	2	0.7	253	PASS
69	198	0.00	100	33.0	36968	PASS
70	69	0.00	2	0.2	71	PASS
127	198	10	80	39.9	44712	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	112138	PASS
199	198	5	9	6.7	7471	PASS
275	198	10	60	30.5	34165	PASS
365	198	1	100	3.7	4187	PASS
441	198	0.01	100	9.2	10329	PASS
442	198	50	100	55.9	62658	PASS
443	442	15	24	20.9	13116	PASS