

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070516\
 Data File : BG022858.D
 Acq On : 5 Jul 2016 20:06
 Operator : UM/SJ
 Sample : H3811-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4TV9

Manual Integrations

sohil
 7/6/2016 7:17:24 PM

Quant Time: Jul 06 04:31:33 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 06 03:22:12 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	147842	20.00	ng/ul	0.00
18) Naphthalene-d8	10.98	136	682899	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.80	164	500600	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.55	188	1082691m	20.00	ng/ul	0.00
75) Chrysene-d12	21.85	240	1172241m	20.00	ng/ul	0.00
83) Perylene-d12	25.23	264	1214144	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.55	96	5756	2.18	ng/uL	0.00
5) Phenol-d5	7.31	99	381060	24.50	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.48	67	225219	25.68	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	242359	23.33	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	282920	23.42	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	134835	24.76	ng/ul	0.00
22) 2-Nitrophenol-d4	10.06	143	162245	24.70	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	323160	23.53	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	99718	8.57	ng/ul	0.00
43) Dimethylphthalate-d6	14.19	166	1050531	25.83	ng/ul	0.00
46) Acenaphthylene-d8	14.49	160	1195297	25.65	ng/ul	0.00
51) 4-Nitrophenol-d4	14.99	143	149743	23.45	ng/ul	0.00
57) Fluorene-d10	15.79	176	968198	25.13	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	167207m	24.01	ng/ul	0.00
70) Anthracene-d10	17.65	188	1261457m	25.07	ng/ul	0.00
76) Pyrene-d10	19.93	212	1513711	27.03	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.99	264	1448868	25.12	ng/ul	0.00

Target Compounds					Ovalue
44) Dimethylphthalate	14.24	163	296945	7.15	ng/ul 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG070516\
Data File : BG022858.D
Acq On : 5 Jul 2016 20:06
Operator : UM/SJ
Sample : H3811-11
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
A4TV9

Manual Integrations

sohil
7/6/2016 7:17:24 PM

Quant Time: Jul 06 04:31:33 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 06 03:22:12 2016
Response via : Initial Calibration

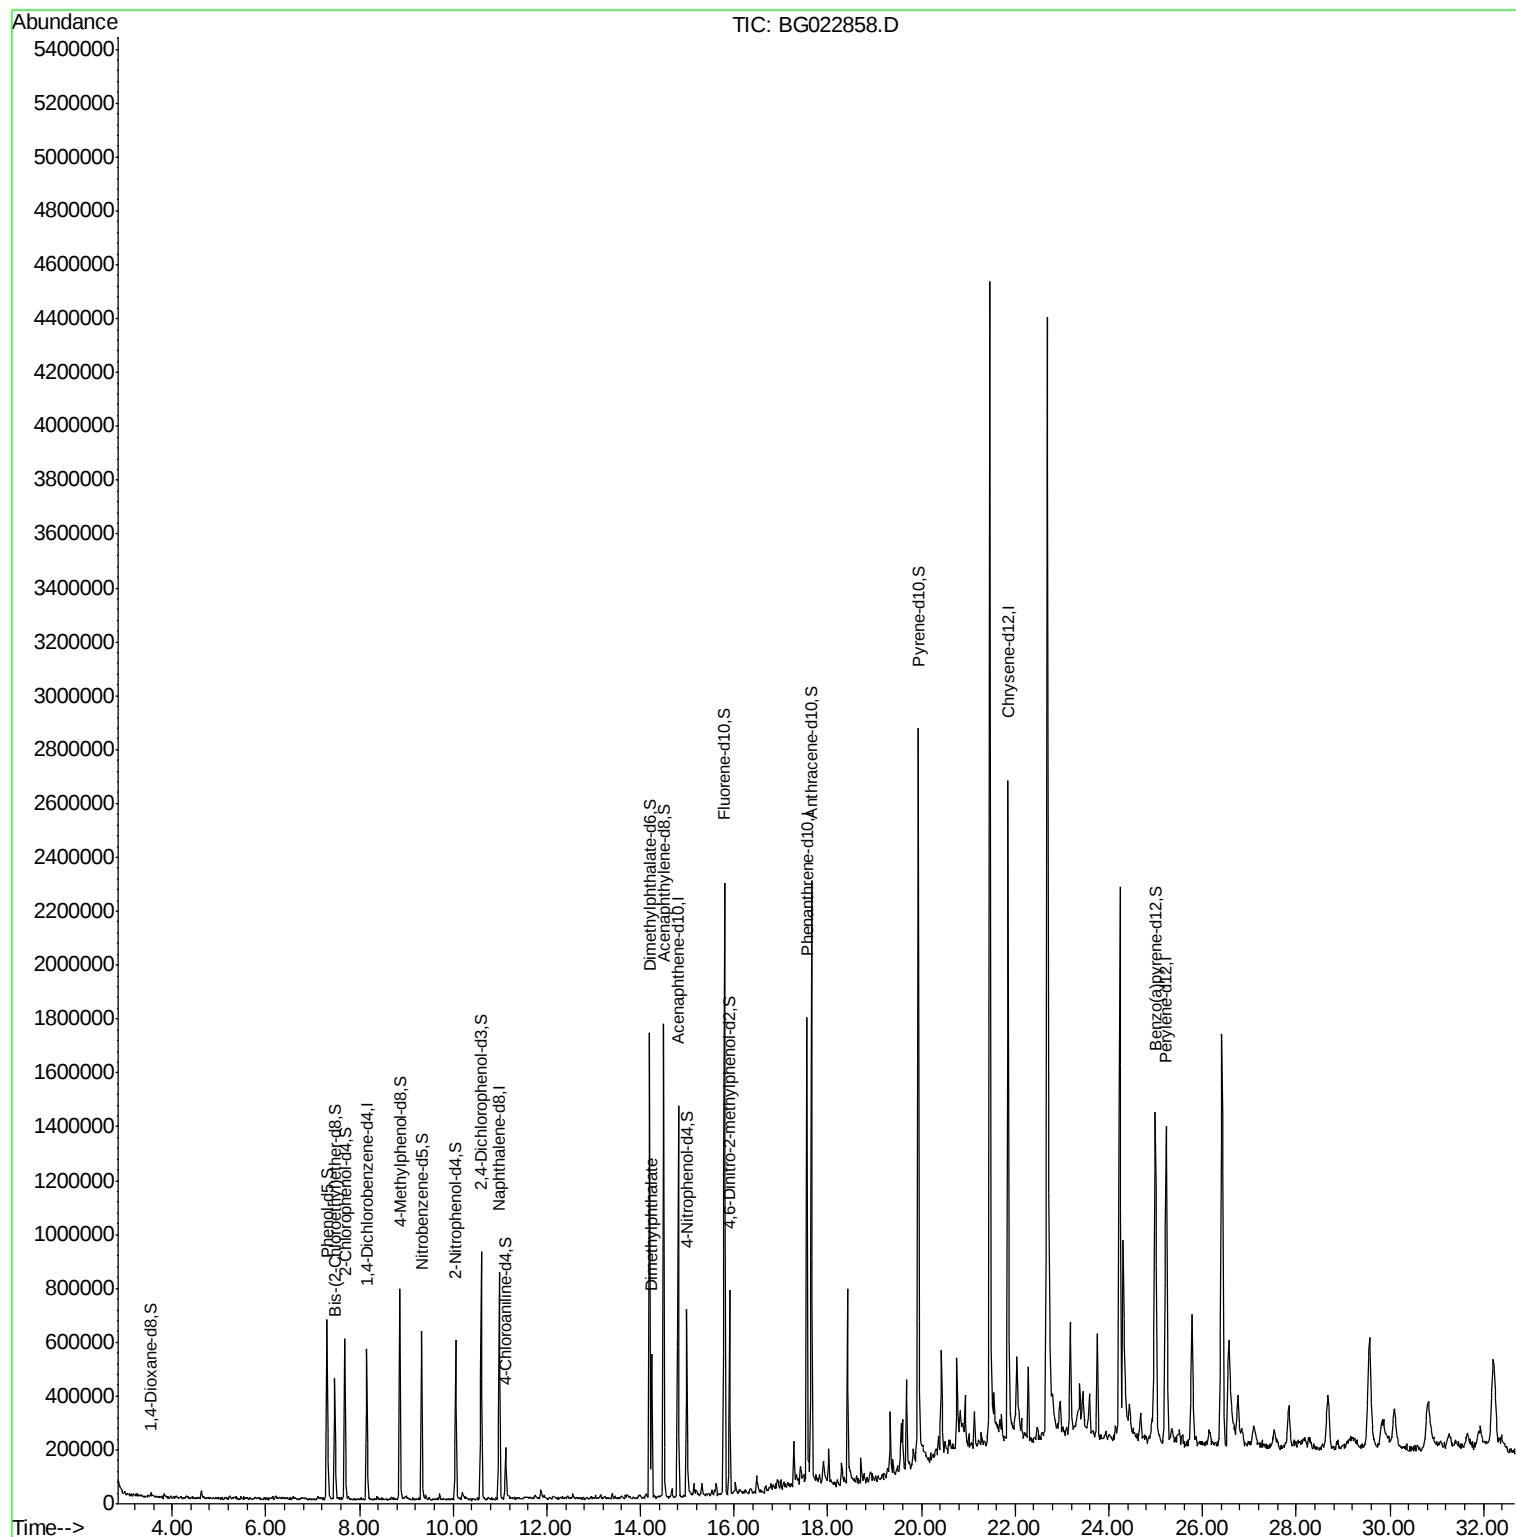

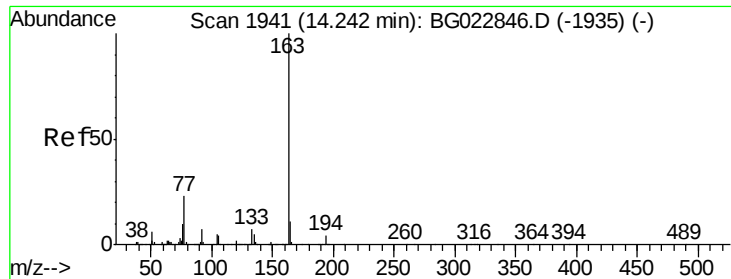

#44
 Dimethylphthalate
 Concen: 7.15 ng/ul
 RT: 14.24 min Scan# 1940
 Delta R.T. -0.00 min
 Lab File: BG022858.D
 Acq: 5 Jul 2016 20:06

Instrument :
 BNA_G
 ClientSampleId :
 A4TV9

Tot Ion	Ratio	Resp	Lower	Upper
163	100	296945		
194	5.0		3.4	5.2
164	10.1		8.8	13.2

Manual Integrations

sohil
 7/6/2016 7:17:24 PM

