

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070516\
 Data File : BG022864.D
 Acq On : 6 Jul 2016 00:07
 Operator : UM/SJ
 Sample : H3811-22
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4TX0

Quant Time: Jul 06 04:58:33 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 06 03:22:12 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	156335	20.00	ng/ul	0.00
18) Naphthalene-d8	10.99	136	695094	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.80	164	524125	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.56	188	1177869	20.00	ng/ul	0.00
75) Chrysene-d12	21.86	240	1229172	20.00	ng/ul	0.01
83) Perylene-d12	25.23	264	1272992	20.00	ng/ul	0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.54	96	5301	1.89	ng/uL	0.00
5) Phenol-d5	7.31	99	348589	21.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.48	67	204218	22.02	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	233591	21.27	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	277678	21.74	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	124030	22.38	ng/ul	0.00
22) 2-Nitrophenol-d4	10.06	143	146645	21.93	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.61	165	304176	21.76	ng/ul	0.00
29) 4-Chloroaniline-d4	11.13	131	16267	1.37	ng/ul	0.01
43) Dimethylphthalate-d6	14.20	166	975798	22.92	ng/ul	0.00
46) Acenaphthylene-d8	14.50	160	1147183	23.51	ng/ul	0.00
51) 4-Nitrophenol-d4	15.00	143	144934	21.68	ng/ul	0.00
57) Fluorene-d10	15.80	176	940873	23.32	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.91	200	172297	22.74	ng/ul	0.00
70) Anthracene-d10	17.65	188	1263550	23.08	ng/ul	0.00
76) Pyrene-d10	19.94	212	1443558	24.58	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.00	264	1406216	23.25	ng/ul	0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.24	163	289954	6.67	ng/ul#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070516\
Data File : BG022864.D
Acq On : 6 Jul 2016 00:07
Operator : UM/SJ
Sample : H3811-22
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4TX0

Quant Time: Jul 06 04:58:33 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 06 03:22:12 2016
Response via : Initial Calibration

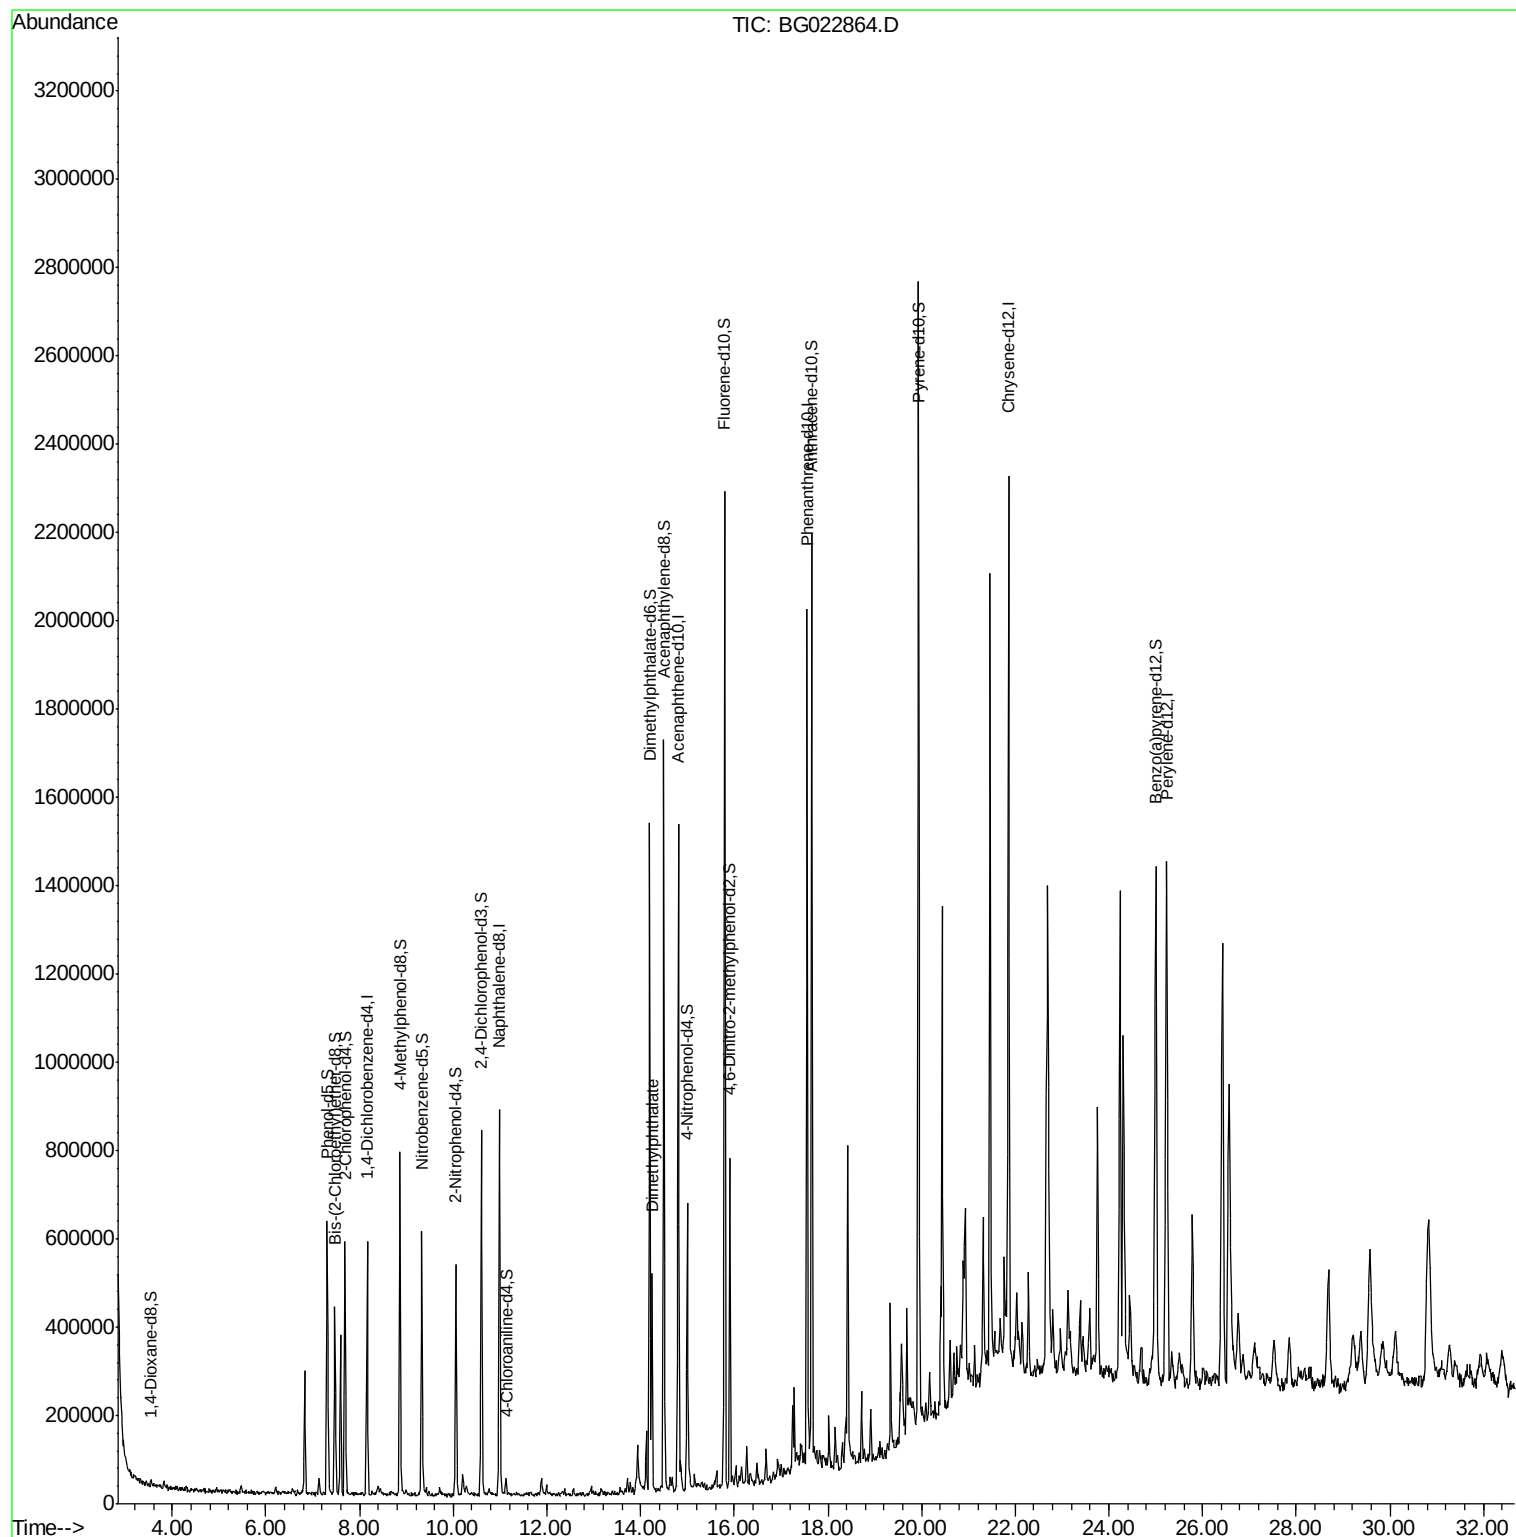

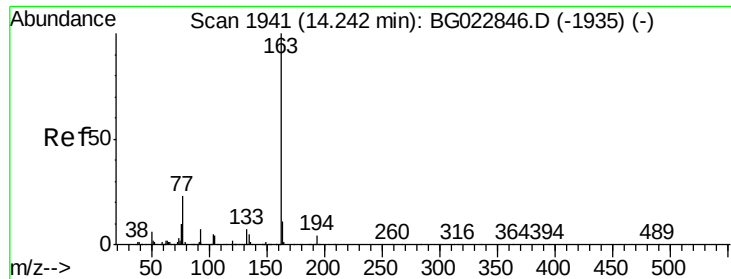

#44
 Dimethylphthalate
 Concen: 6.67 ng/ul
 RT: 14.24 min Scan# 1941
 Delta R.T. 0.00 min
 Lab File: BG022864.D
 Acq: 6 Jul 2016 00:07

Instrument :
 BNA_G
 ClientSampleId :
 A4TX0

Tot Ion	Ratio	Lower	Upper
163	100		
194	3.7	3.4	5.2
164	8.3	8.8	13.2#

