
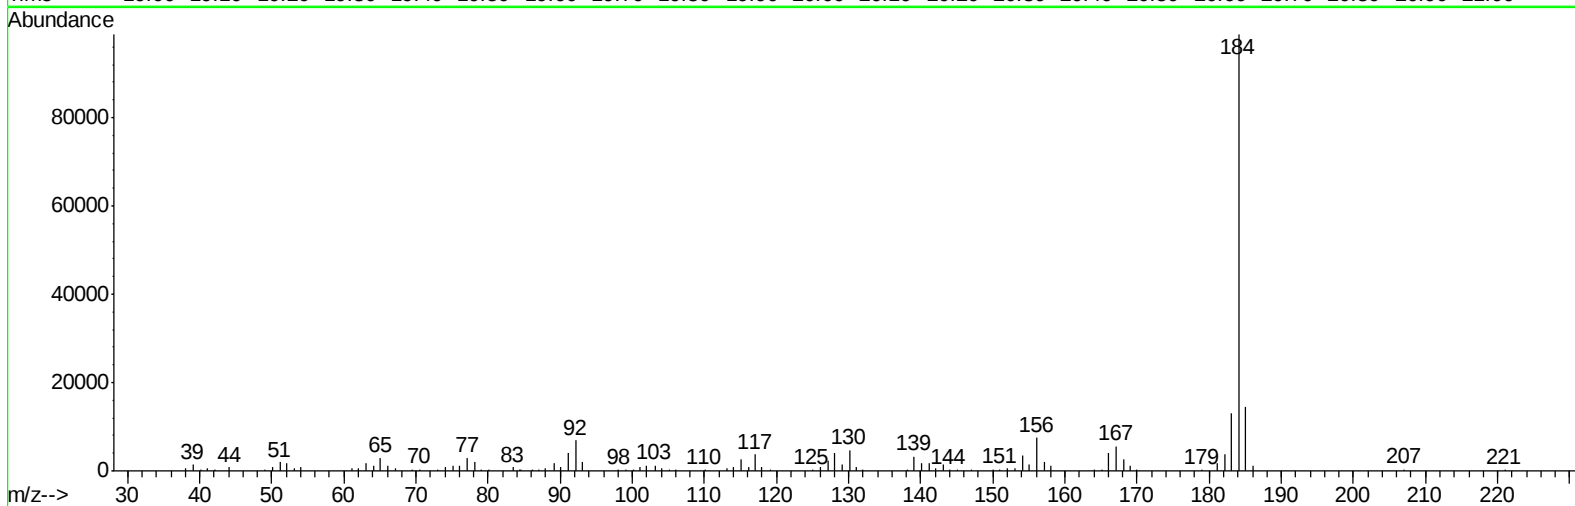


Data Path : Z:\HPCHEM1\BNA G\DATA\BG070517\
Data File : BG027847.D
Acq On : 5 Jul 2017 14:35
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 06 05:58:23 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 19:26:37 2017
Response via : Initial Calibration

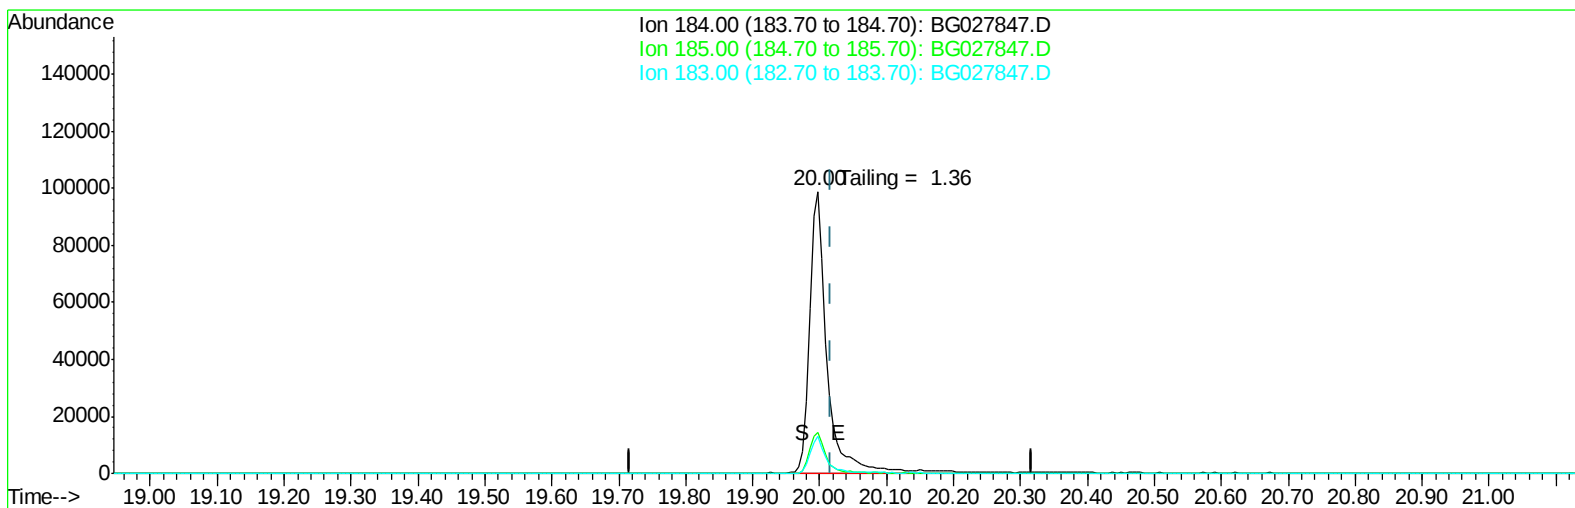

TIC: BG027847.D

(76) Benzidine



19.997min (-0.020) 0.00ng

response 179624

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.61
183.00	13.80	13.07
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070517\
Data File : BG027847.D
Acq On : 5 Jul 2017 14:35
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 06 05:58:23 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 19:26:37 2017
Response via : Initial Calibration

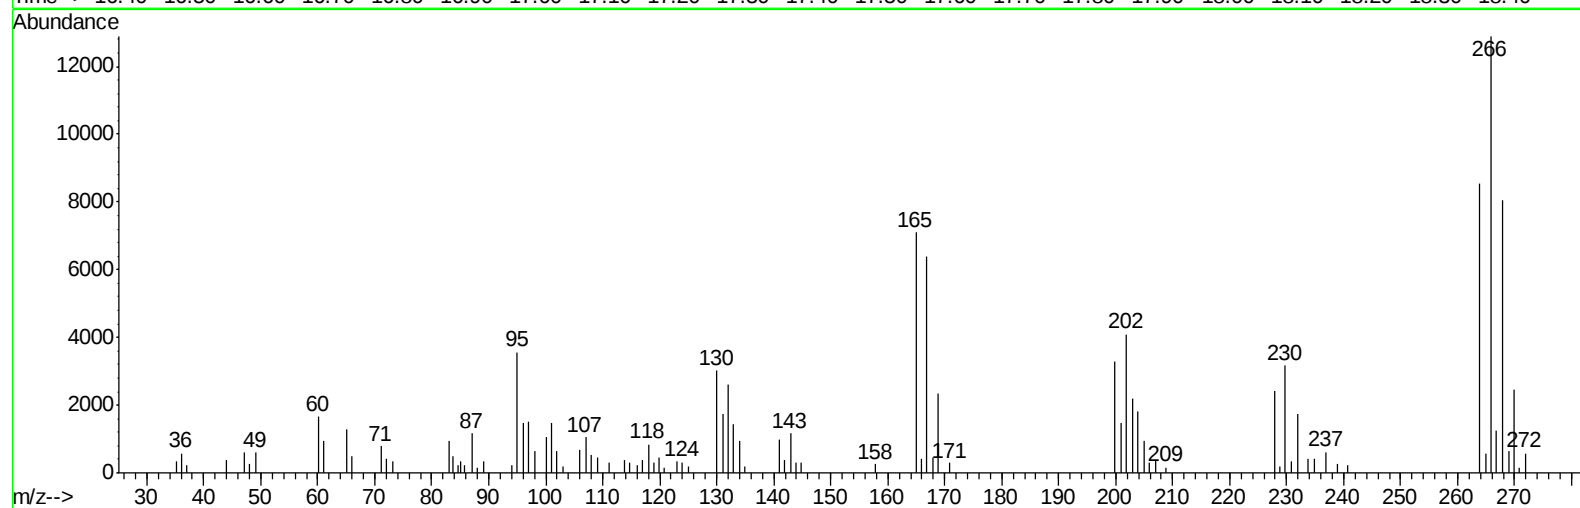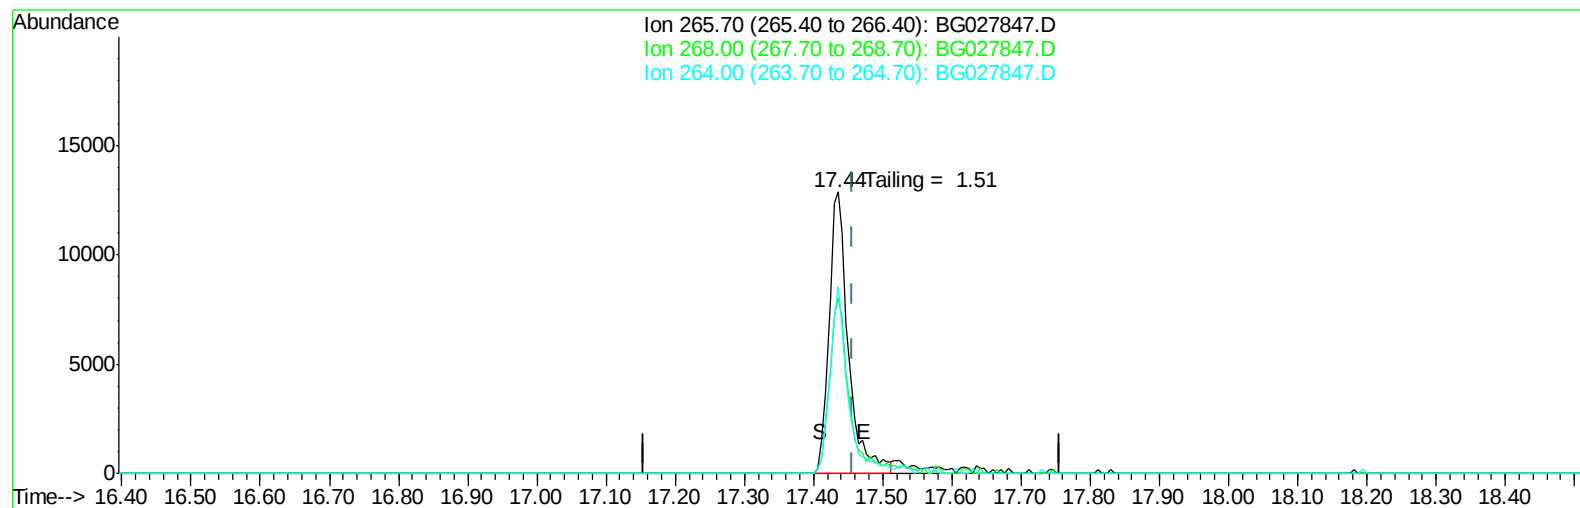

TIC: BG027847.D

(69) Pentachlorophenol (C)

17.436min (-0.020) 0.00ng

response 24945

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	62.47
264.00	62.60	66.25
0.00	0.00	0.00