


Data Path : Z:\HPCHEM1\BNA_G\Data\BG070517\
 Data File : BG027847.D
 Acq On : 5 Jul 2017 14:35
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 28 19:26:37 2017

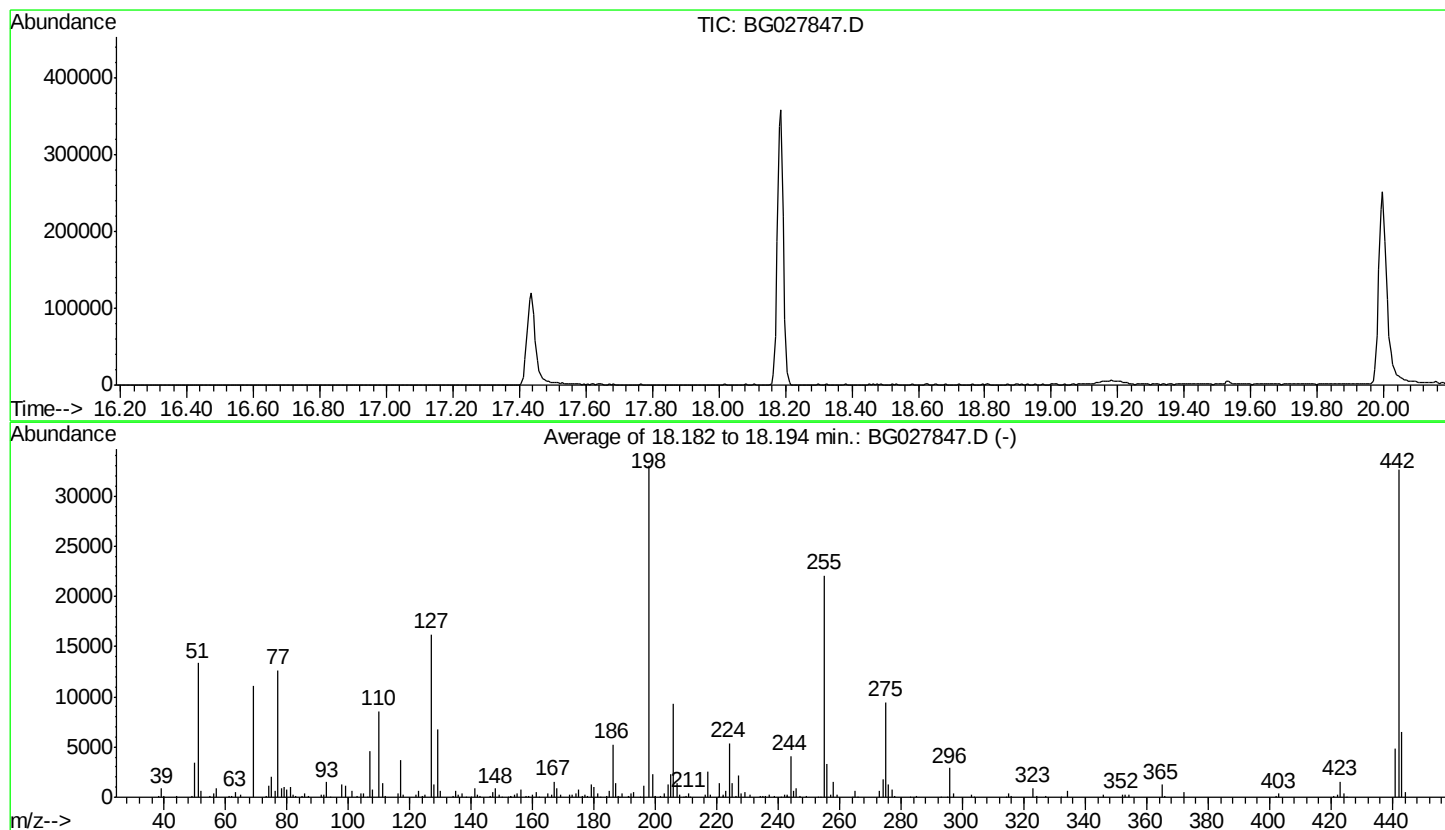

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	13376	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.7	11139	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.0	16192	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	33018	PASS
199	198	5	9	6.9	2279	PASS
275	198	10	60	28.7	9489	PASS
365	198	1	100	3.7	1222	PASS
441	442	0.01	24	14.7	4813	PASS
442	198	50	100	99.0	32672	PASS
443	442	15	24	19.9	6493	PASS