
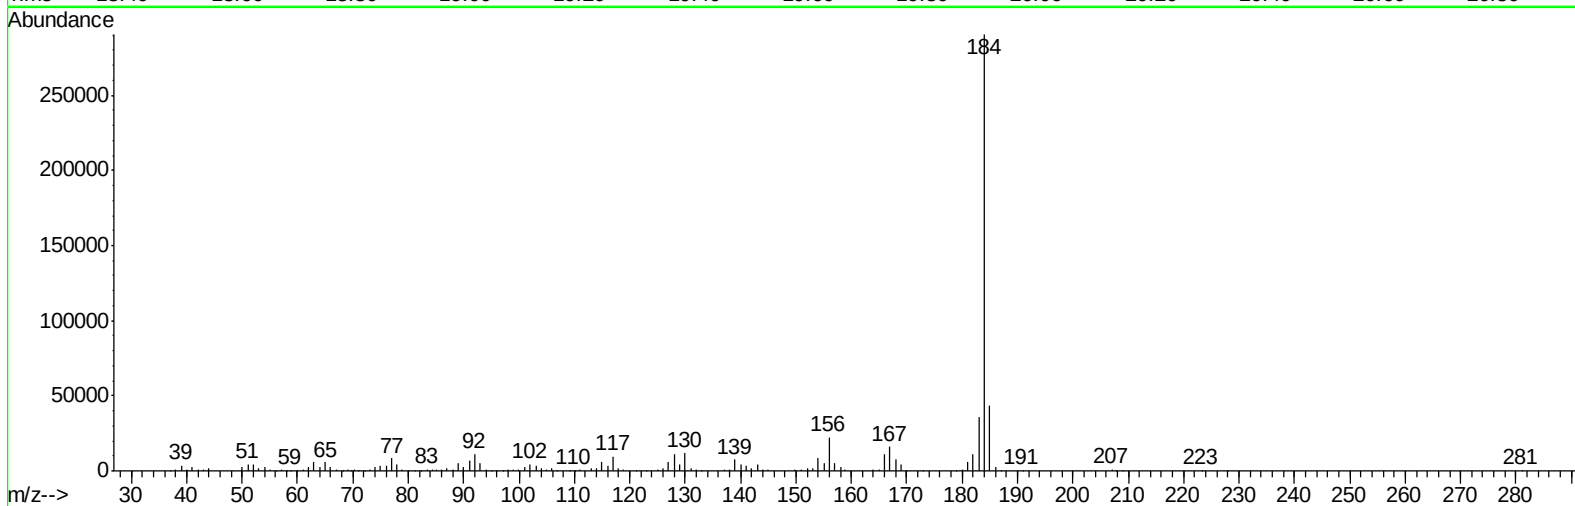


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070519\
Data File : BG041608.D
Acq On : 5 Jul 2019 11:32
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 06 06:33:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG062619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:25:55 2019
Response via : Initial Calibration

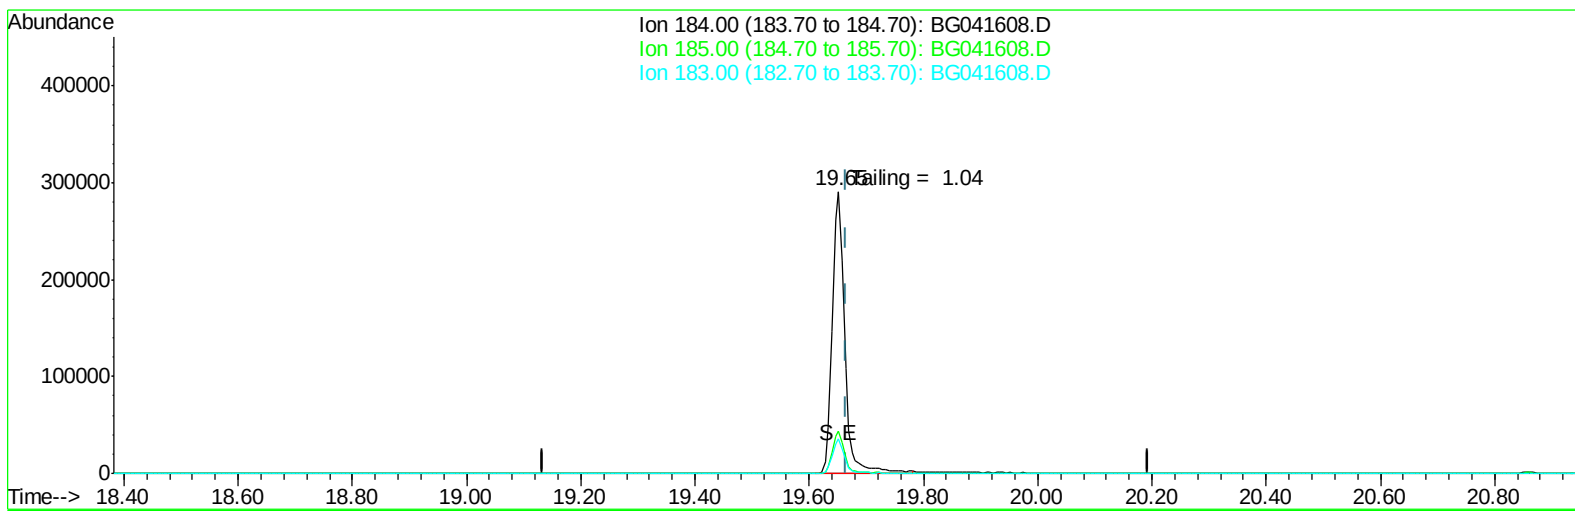

TIC: BG041608.D

(77) Benzidine



19.651min (-0.013) 22602.88ng

response 433807

Ion	Exp%	Act%
184.00	100	100
185.00	15.90	14.96
183.00	11.80	12.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070519\
Data File : BG041608.D
Acq On : 5 Jul 2019 11:32
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 06 06:33:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG062619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:25:55 2019
Response via : Initial Calibration

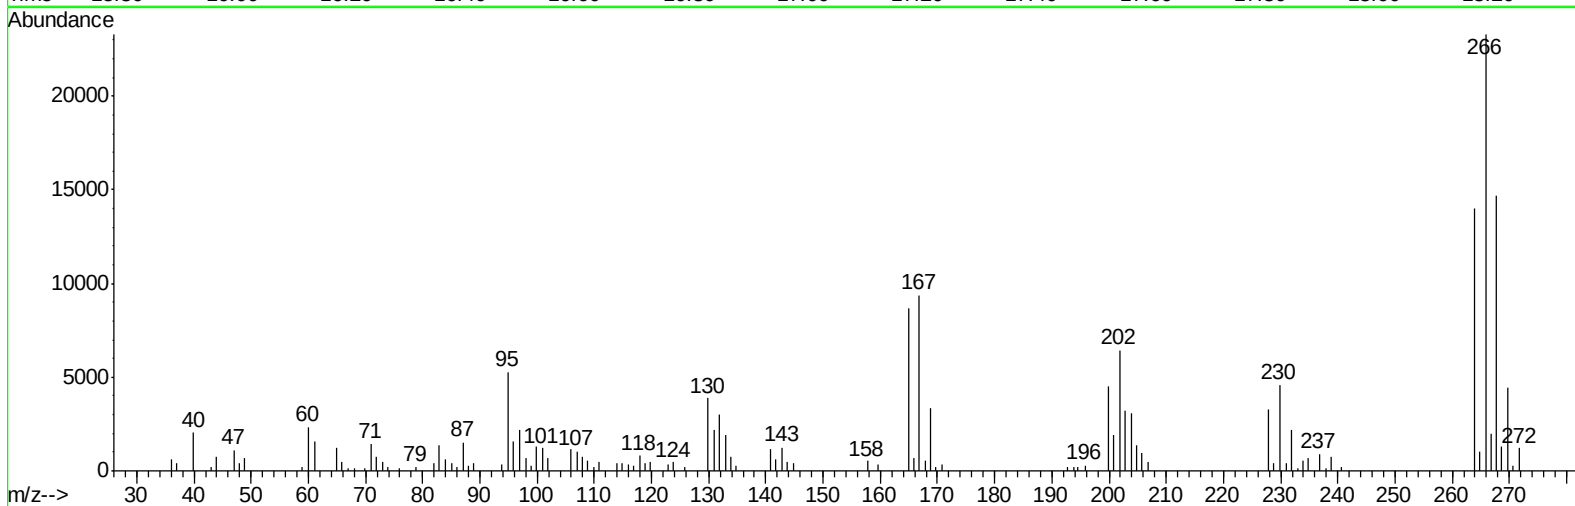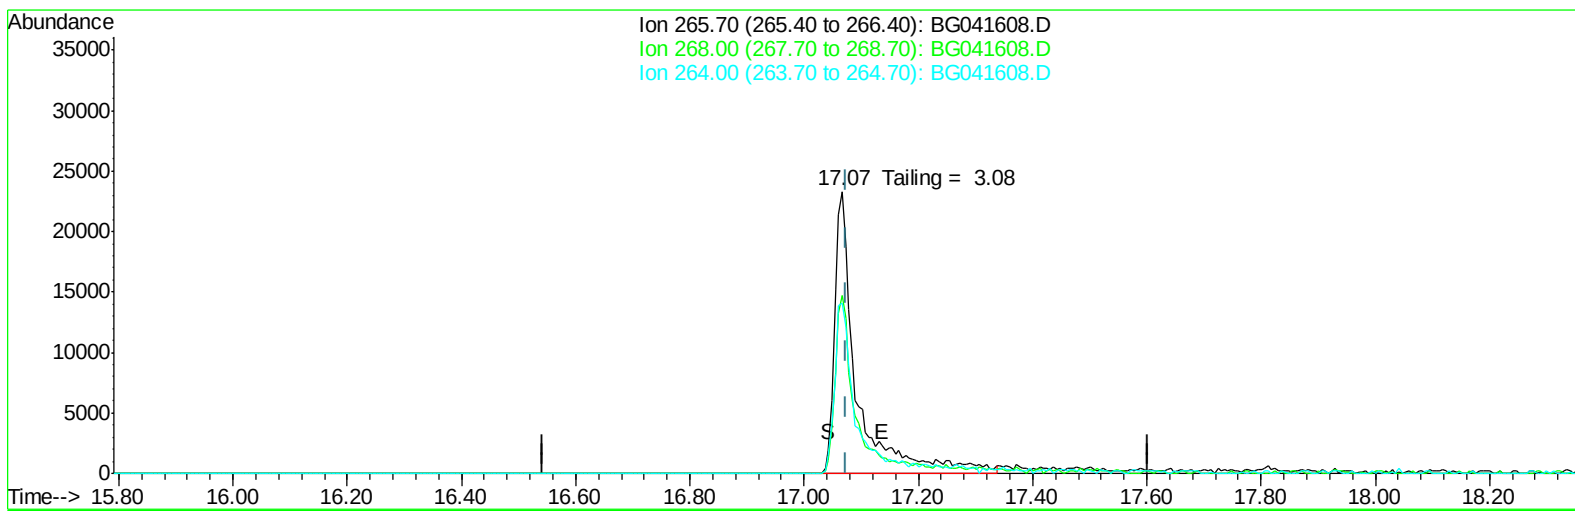

TIC: BG041608.D

(70) Pentachlorophenol (C)

17.066min (-0.007) 35218.58ng

response 57800

Ion	Exp%	Act%
265.70	100	100
268.00	58.70	68.65
264.00	59.20	60.27
0.00	0.00	0.00