


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070519\
 Data File : BG041608.D
 Acq On : 5 Jul 2019 11:32
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG062619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 27 13:25:55 2019

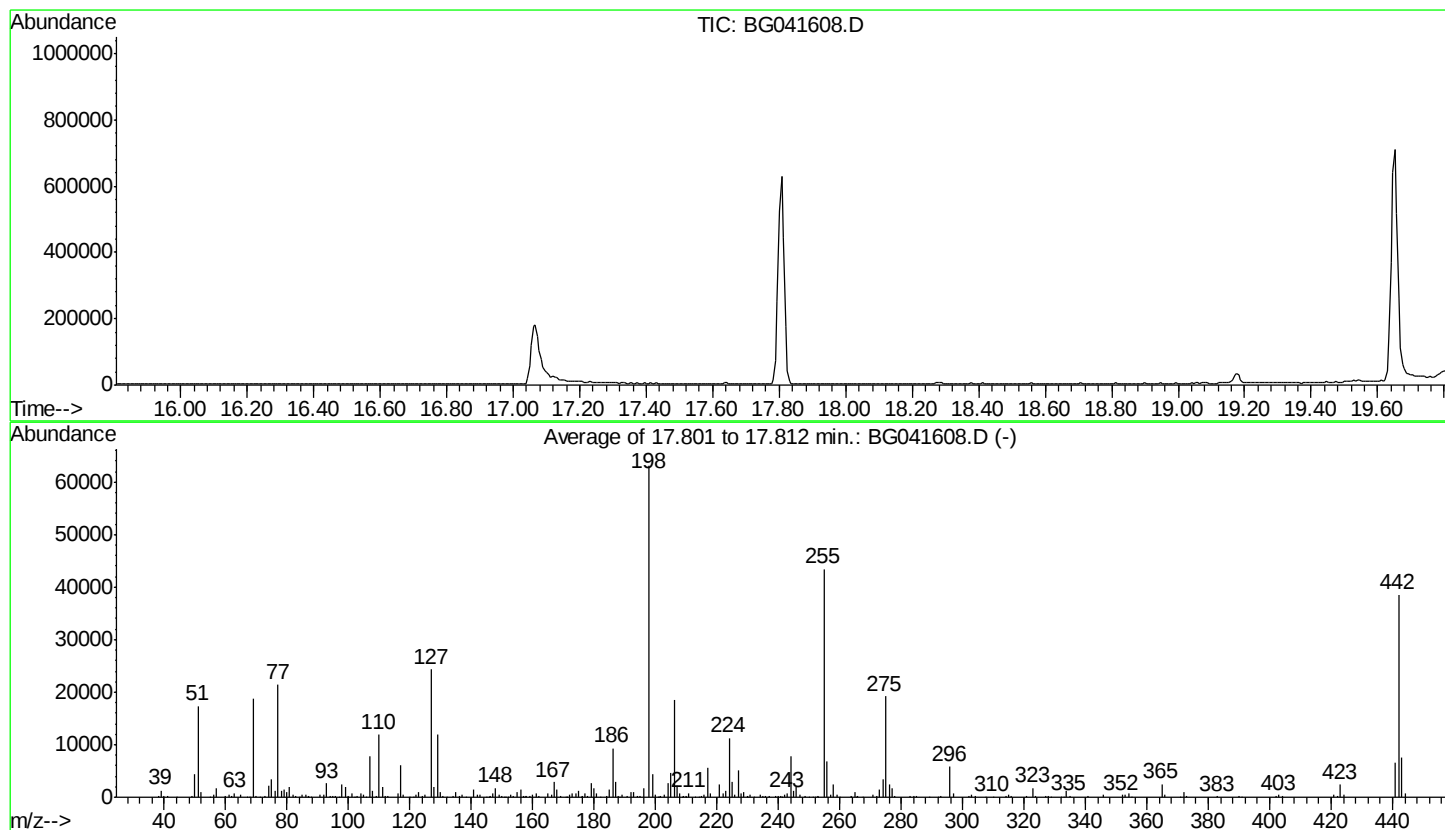

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.5	17338	PASS
68	69	0.00	2	0.7	126	PASS
69	198	0.00	100	29.7	18763	PASS
70	69	0.00	2	0.7	139	PASS
127	198	10	80	38.5	24325	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	63101	PASS
199	198	5	9	6.8	4291	PASS
275	198	10	60	30.4	19197	PASS
365	198	1	100	4.0	2514	PASS
441	198	0.01	100	10.3	6485	PASS
442	198	50	100	61.1	38586	PASS
443	442	15	24	19.3	7459	PASS