
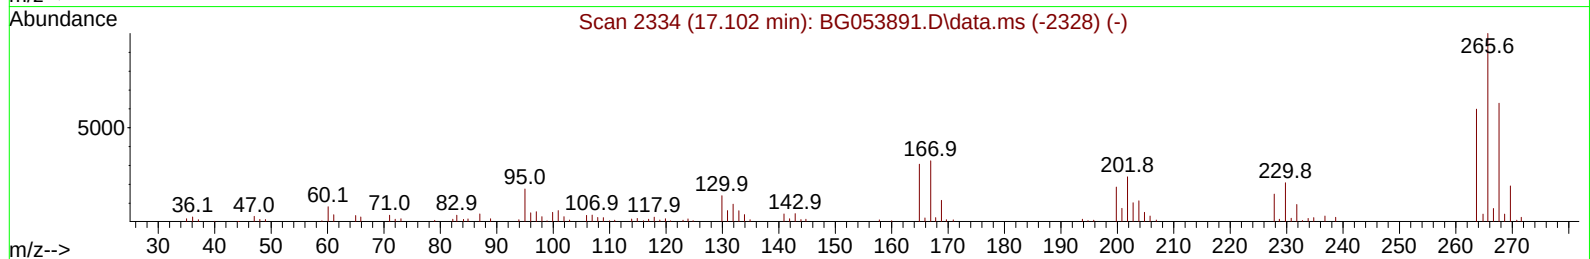
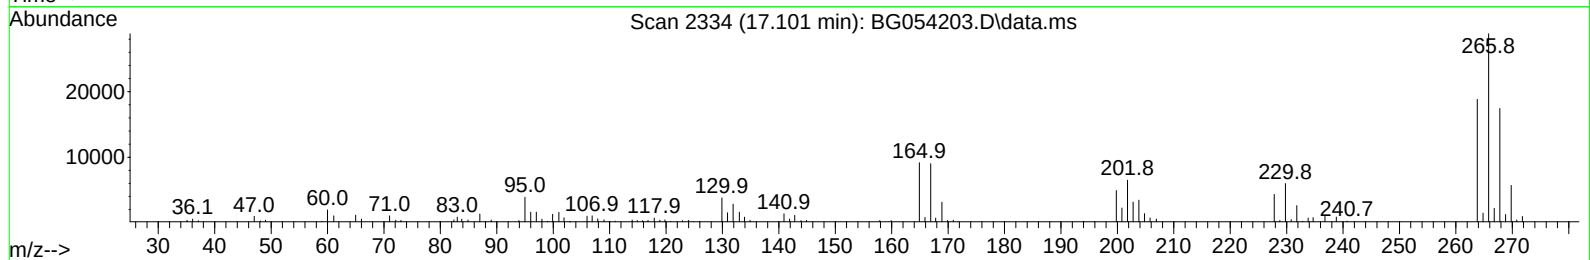


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070522\
Data File : BG054203.D
Acq On : 5 Jul 2022 9:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 06 02:59:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

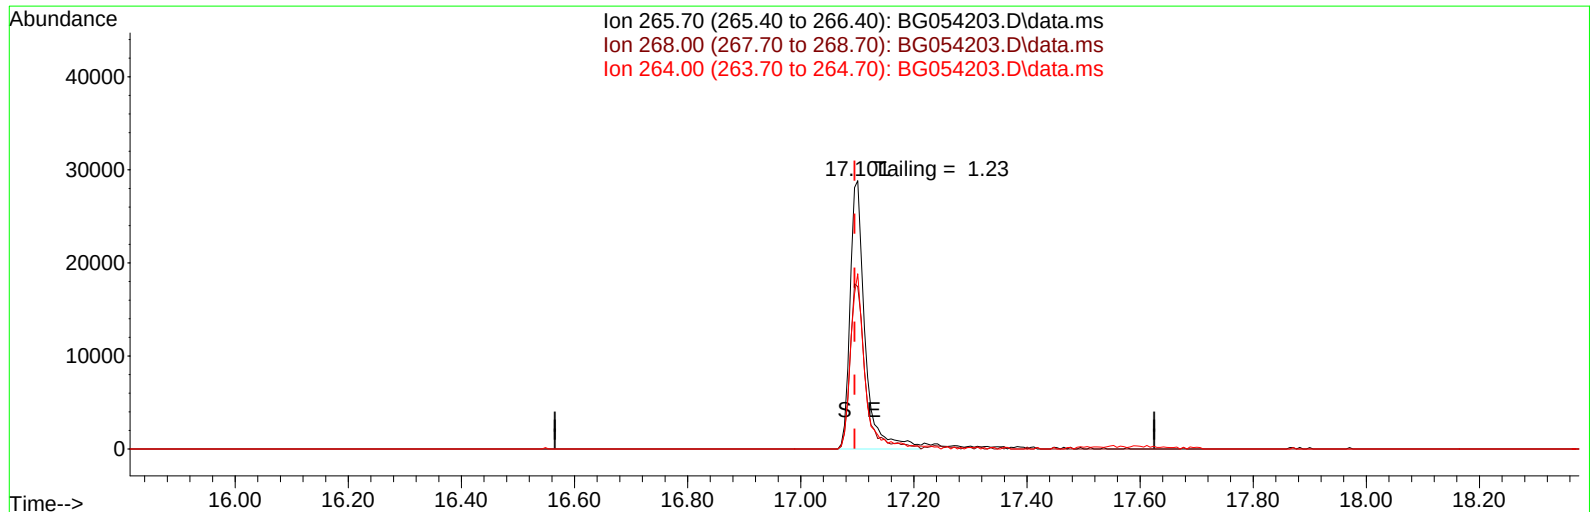

TIC: BG054203.D\data.ms

(70) Pentachlorophenol (C)




17.101min (+ 0.006) 66125.34 ng

response 53099

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	60.50
264.00	66.20	65.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070522\
Data File : BG054203.D
Acq On : 5 Jul 2022 9:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 06 02:59:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

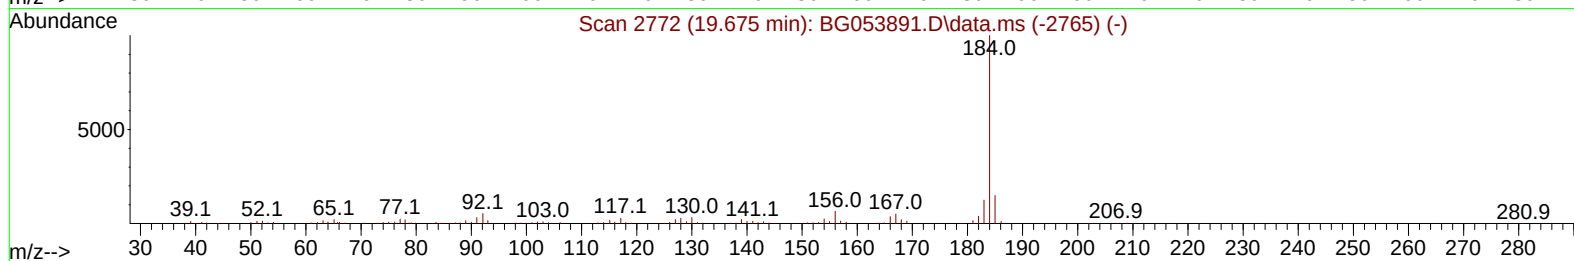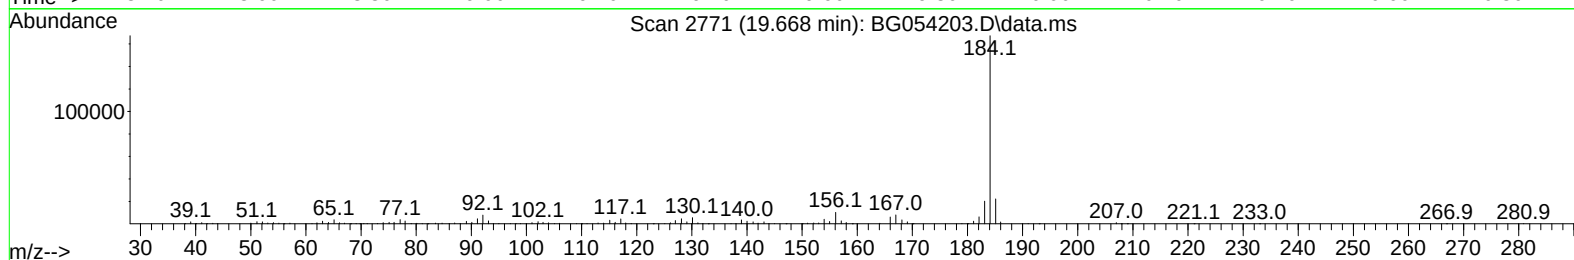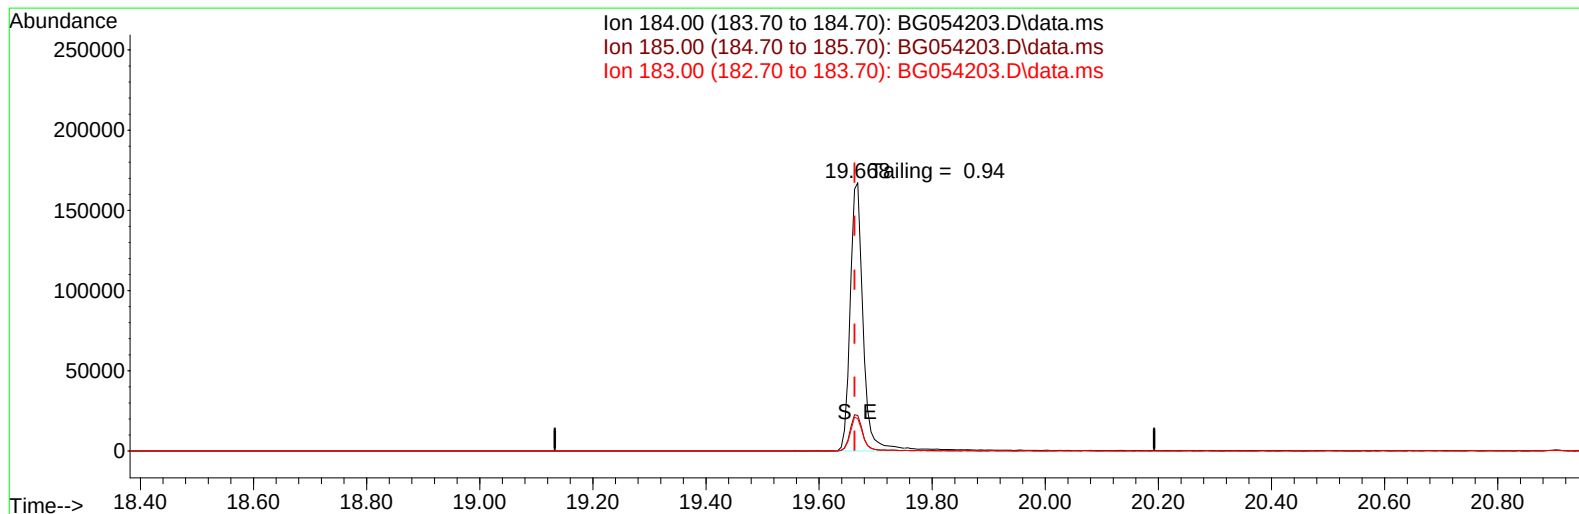

TIC: BG054203.D\data.ms

(77) Benzidine**19.668min (+ 0.006) 234335.50 ng****response 266906**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.26
183.00	11.10	12.07
0.00	0.00	0.00