
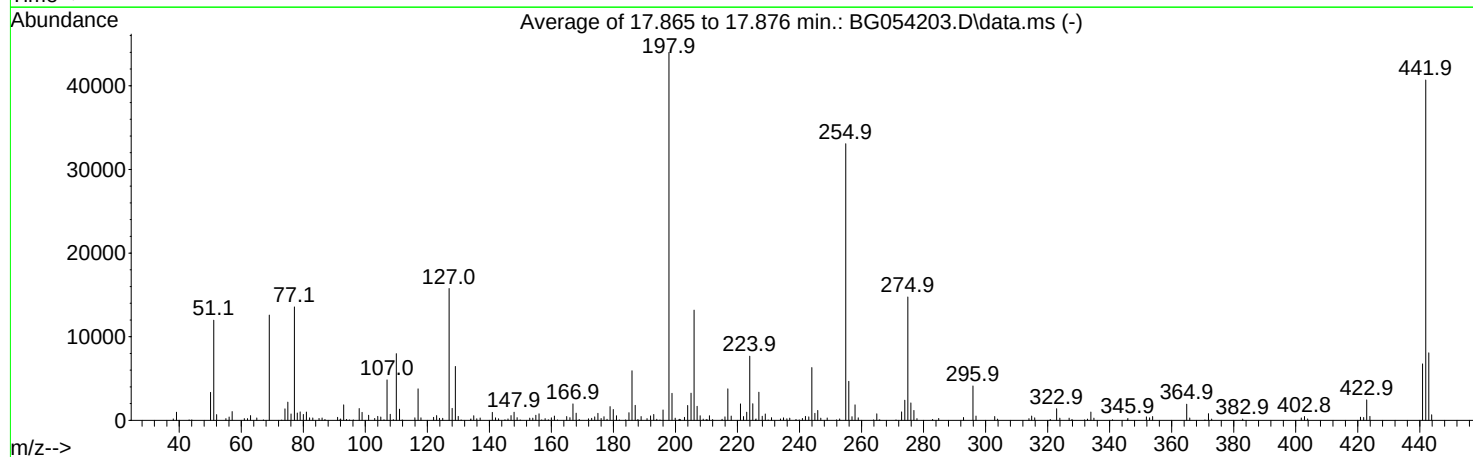


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070522\
 Data File : BG054203.D
 Acq On : 5 Jul 2022 9:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 27 00:27:54 2022

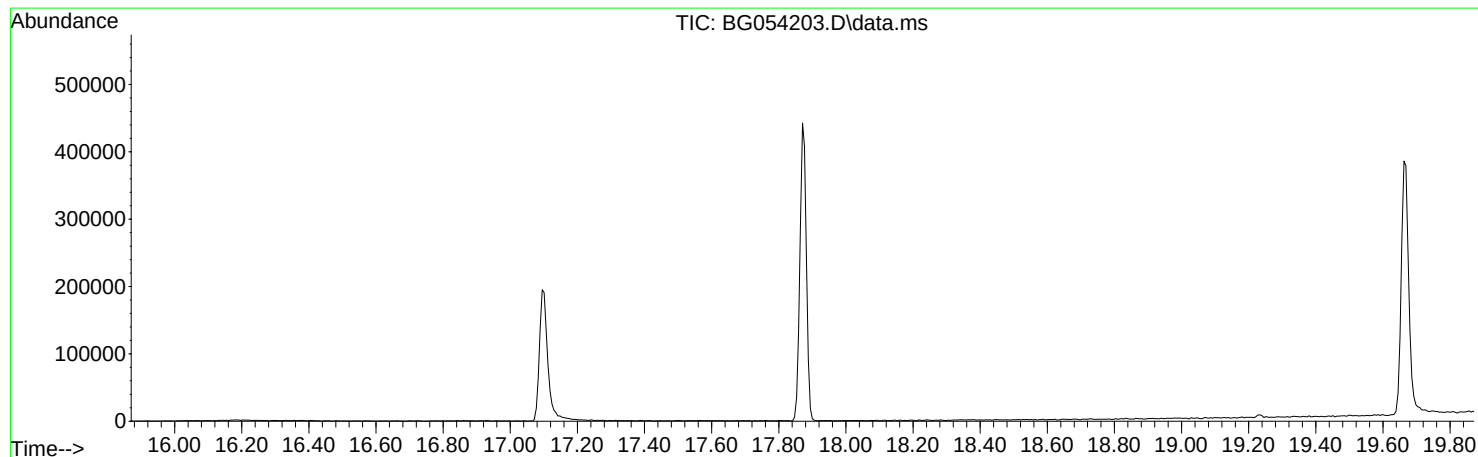




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.2	11977	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.6	12582	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	35.8	15755	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	43979	PASS
199	198	5	9	7.4	3234	PASS
275	198	10	60	33.5	14744	PASS
365	198	1	100	4.4	1928	PASS
441	198	0.01	100	15.4	6752	PASS
442	442	50	100	100.0	40688	PASS
443	442	15	24	19.8	8075	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070522\
Data File : BG054203.D
Acq On : 5 Jul 2022 9:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 06 02:59:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

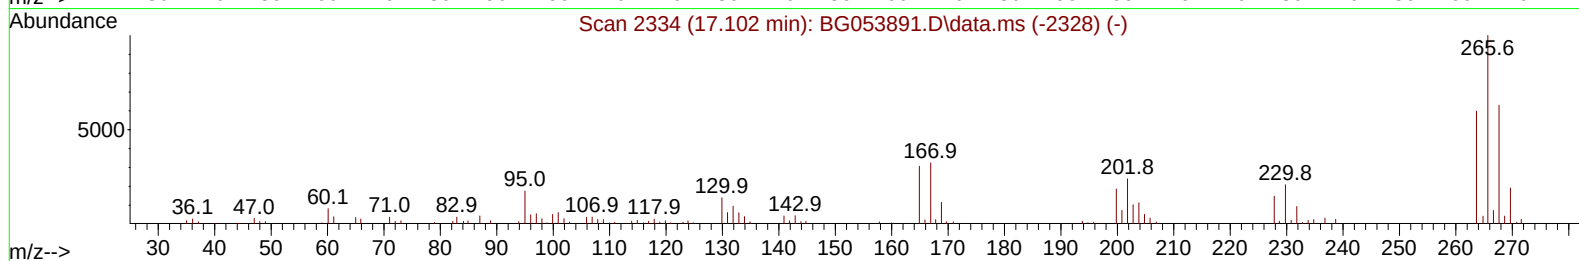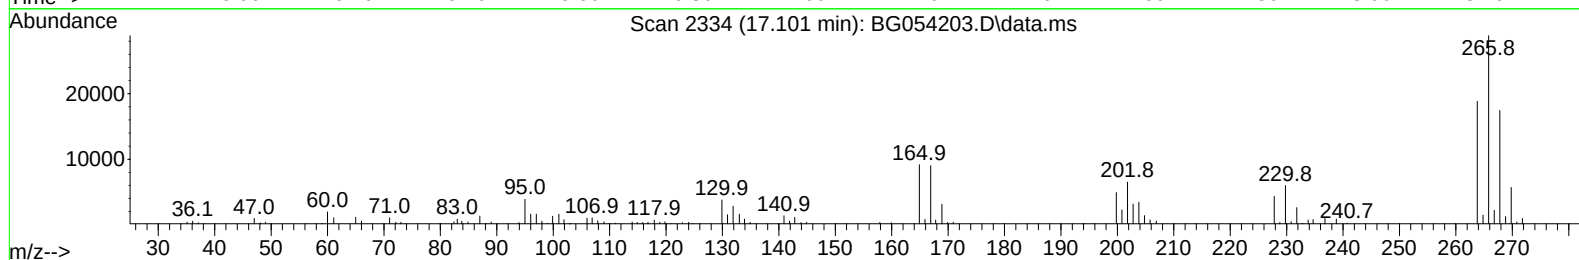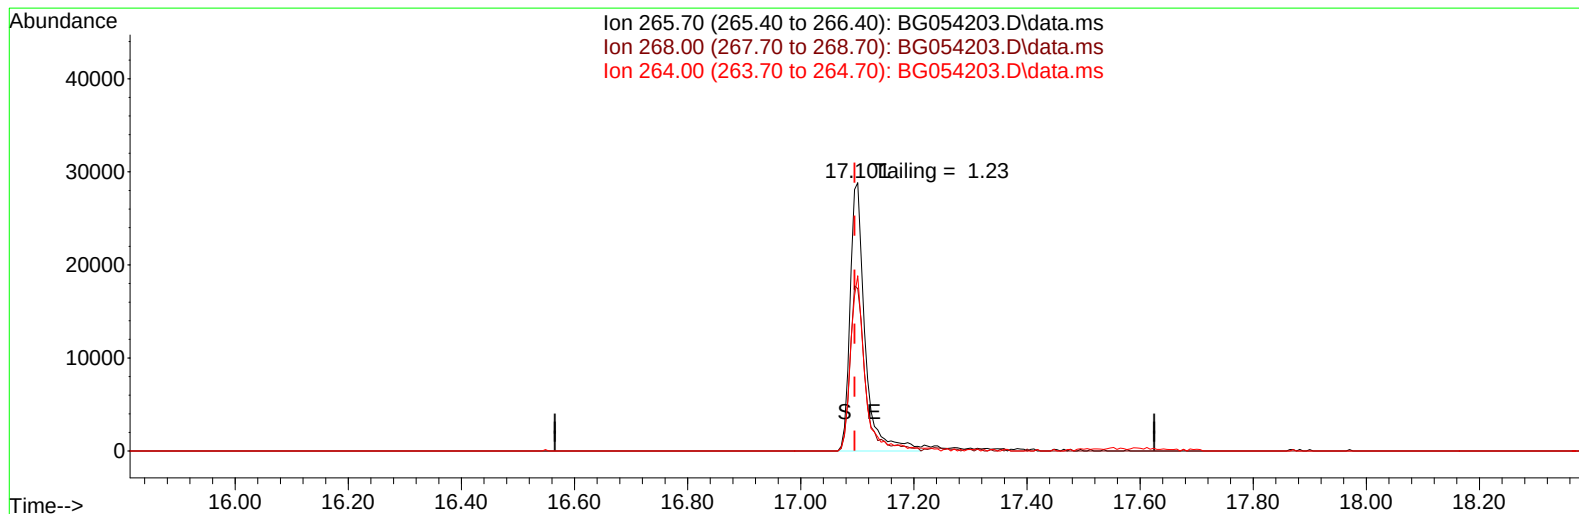

TIC: BG054203.D\data.ms

(70) Pentachlorophenol (C)

17.101min (+ 0.006) 66125.34 ng




response 53099

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	60.50
264.00	66.20	65.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070522\
Data File : BG054203.D
Acq On : 5 Jul 2022 9:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 06 02:59:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

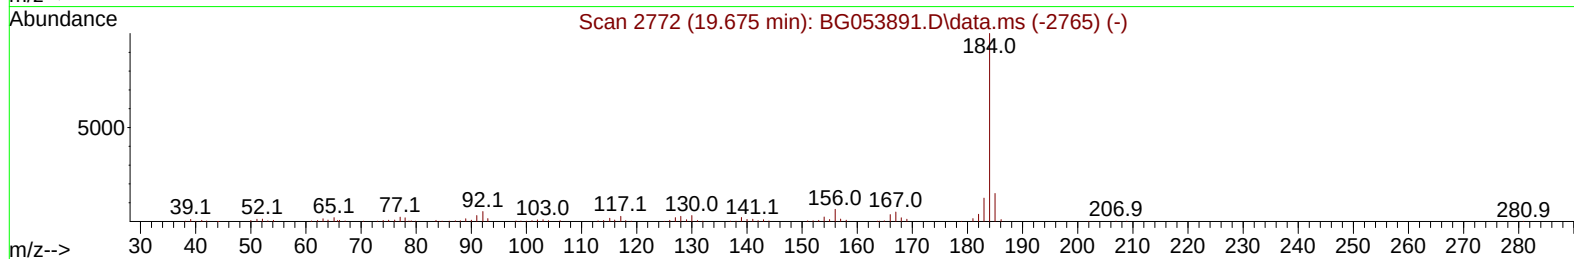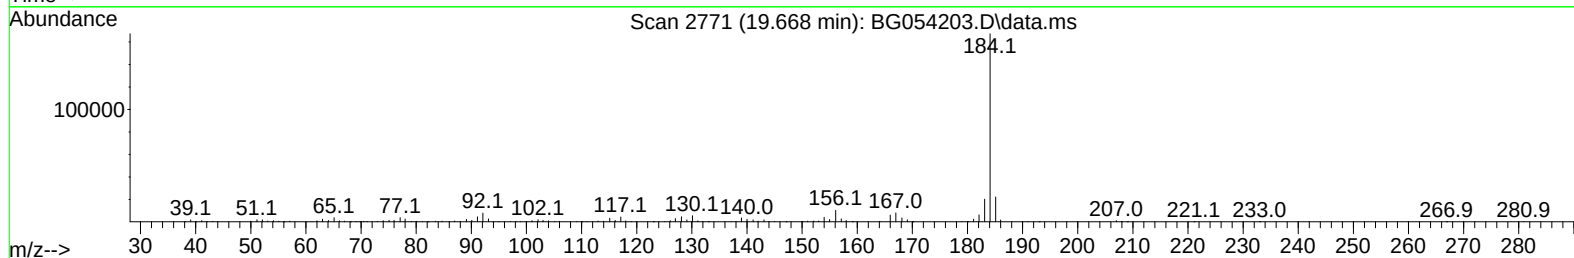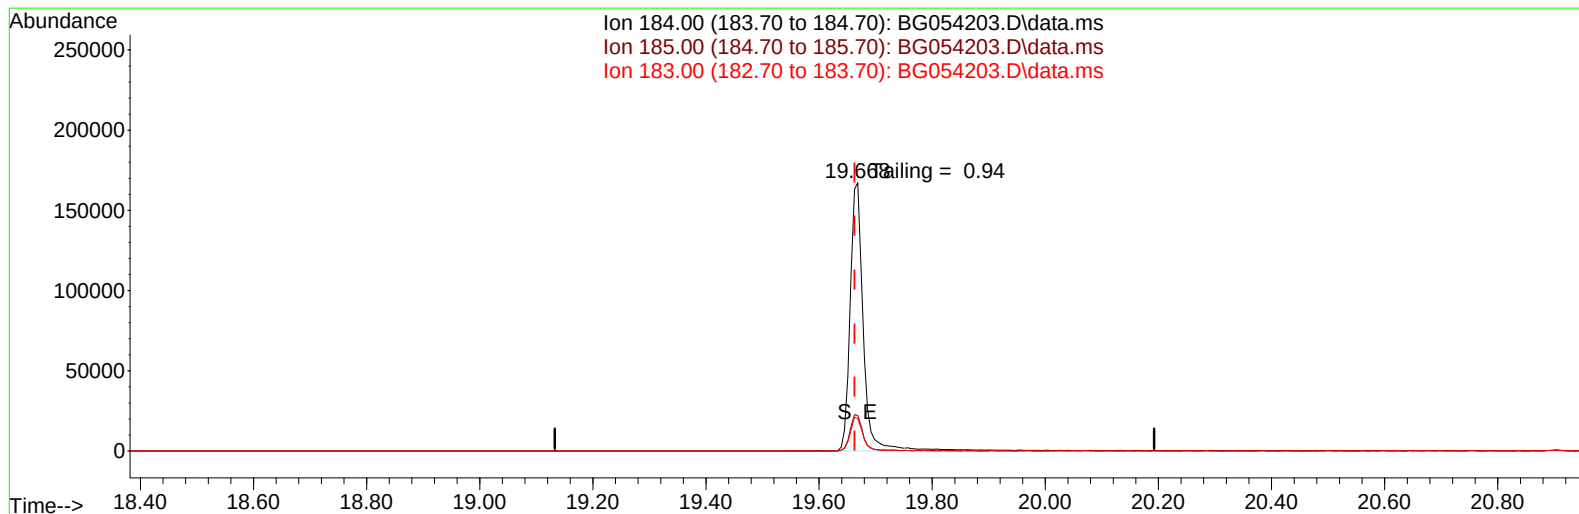

TIC: BG054203.D\data.ms

(77) Benzidine

19.668min (+ 0.006) 234335.50 ng

response 266906

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.26
183.00	11.10	12.07
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/5/2022	BNA_G	<u>BG054203.D</u>
Compound Name	Response	Retention Time
DDT	145786	20.902
DDD	6118	20.462
DDE	1350	19.956
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7468	153254	4.87

Instrument :
BNA_G
ClientSampleId :
DFTPP