

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070615\
 Data File : BG017780.D
 Acq On : 6 Jul 2015 21:54
 Operator : TP/UM
 Sample : G2860-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jul 07 03:05:18 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG070615.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 07 01:50:10 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	111846	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	531988	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	338669	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.01	188	711021	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	724122	20.00	ng/ul	0.00
85) Perylene-d12	23.43	264	723576	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	3749	1.33	ng/uL	0.00
5) Phenol-d5	6.78	99	84895	8.99	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	55083	9.73	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	69721	8.63	ng/ul	0.00
13) 4-Methylphenol-d8	8.31	113	47844	6.19	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	35924	9.02	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	36189	9.10	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.01	165	64554	8.50	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	64781	6.28	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	195252	8.71	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	252333	8.35	ng/ul	0.00
51) 4-Nitrophenol-d4	14.46	143	27931	6.21	ng/ul	0.00
57) Fluorene-d10	15.26	176	185279	8.10	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	10618	3.22	ng/ul	0.00
70) Anthracene-d10	17.11	188	257850	7.96	ng/ul	0.00
78) Pyrene-d10	19.41	212	276617	8.04	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.29	264	245767	7.71	ng/ul	0.00

Target Compounds


						Qvalue
14) Acetophenone	8.42	105	20619	1.81	ng/ul	93
28) Naphthalene	10.43	128	39692	1.44	ng/ul#	93
40) 1,1'-Biphenyl	13.08	154	56903	2.27	ng/ul	99
44) Dimethylphthalate	13.72	163	65129	2.62	ng/ul#	97
47) Acenaphthylene	13.98	152	103426	3.13	ng/ul#	94
49) Acenaphthene	14.32	153	126528	5.69	ng/ul	99
53) Dibenzofuran	14.66	168	65487	2.18	ng/ul#	86
58) Fluorene	15.31	166	184479m	6.92	ng/ul	
69) Phenanthrene	17.06	178	1021665	26.29	ng/ul	98
71) Anthracene	17.14	178	370475	9.27	ng/ul	99
76) Fluoranthene	19.08	202	650928	17.38	ng/ul	98
79) Pyrene	19.44	202	1160697	26.27	ng/ul	98
82) Benzo(a)anthracene	21.19	228	395124m	9.90	ng/ul	
84) Chrysene	21.24	228	288671	7.64	ng/ul	99
87) Benzo(b)fluoranthene	22.77	252	303402	7.34	ng/ul	96
88) Benzo(k)fluoranthene	22.80	252	73320m	1.88	ng/ul	
90) Benzo(a)pyrene	23.34	252	362388	9.22	ng/ul	96
91) Indeno(1,2,3-cd)pyrene	25.67	276	146797	3.42	ng/ul	98
92) Dibenzo(a,h)anthracene	25.69	278	42779	1.18	ng/ul#	79
93) Benzo(g,h,i)perylene	26.37	276	127624	3.56	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070615\
Data File : BG017780.D
Acq On : 6 Jul 2015 21:54
Operator : TP/UM
Sample : G2860-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jul 07 03:05:18 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG070615.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 07 01:50:10 2015
Response via : Initial Calibration

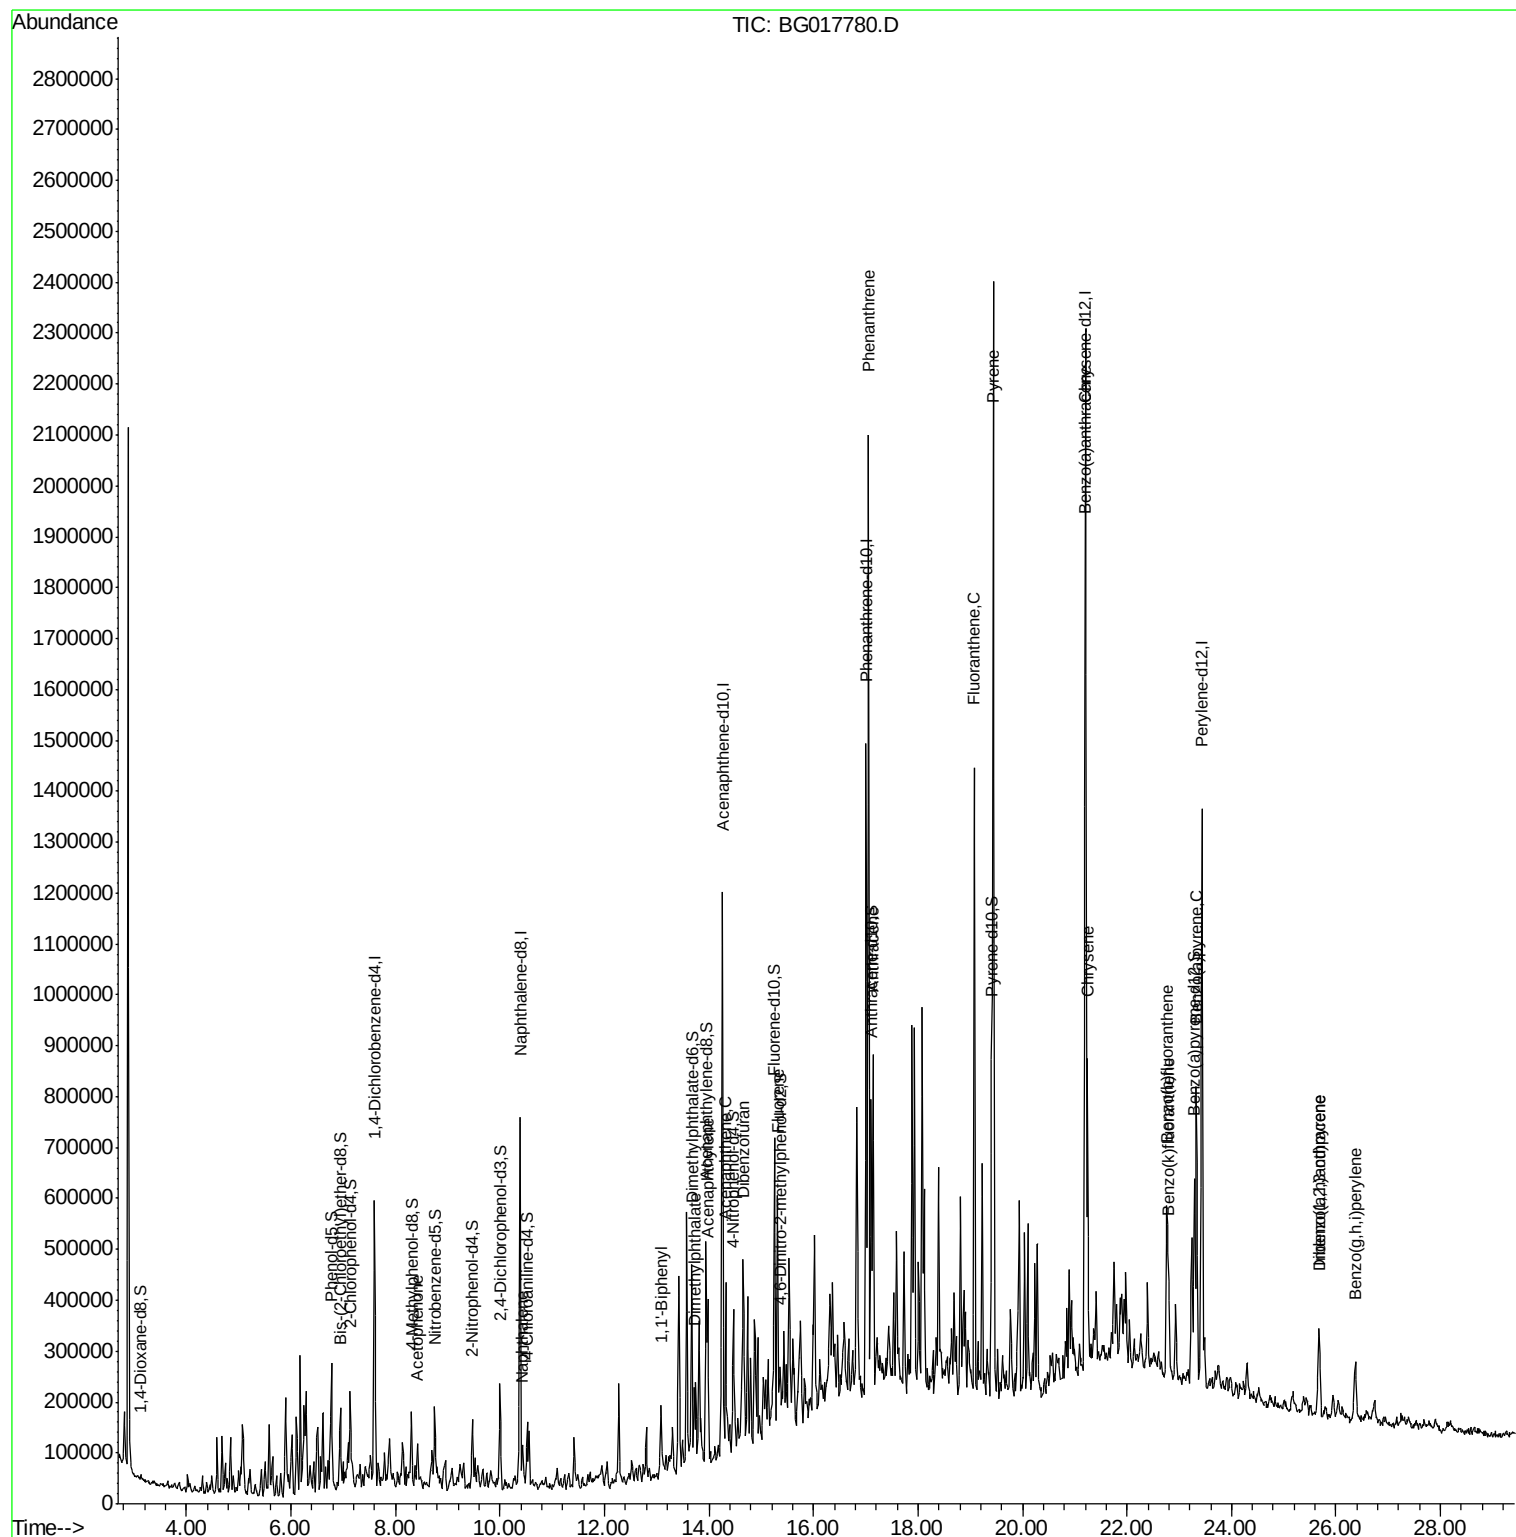

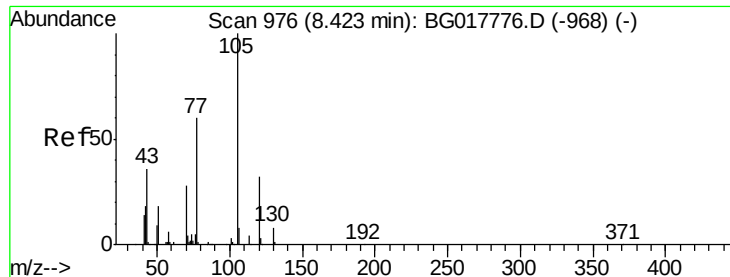

#14

Acetophenone

Concen: 1.81 ng/ul

RT: 8.42 min Scan# 975

Delta R.T. -0.00 min

Lab File: BG017780.D

Acq: 6 Jul 2015 21:54

Instrument :

BNA_G

ClientSampleId :


Tgt Ion:105 Resp: 20619

Ion Ratio Lower Upper

105 100

77 82.4 69.5 104.3




51 40.0 26.7 40.1

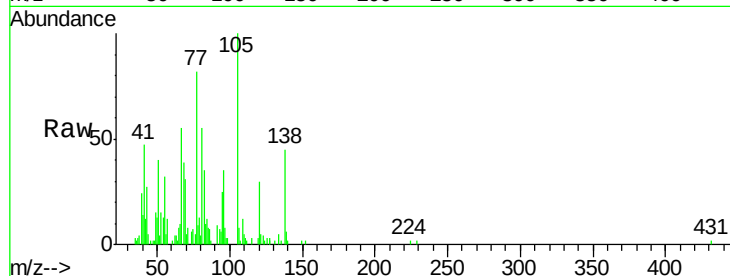

Abundance Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BG017776.D (-968) (-)

Ion 51.00 (50.70 to 51.70): BG017776.D (-968) (-)

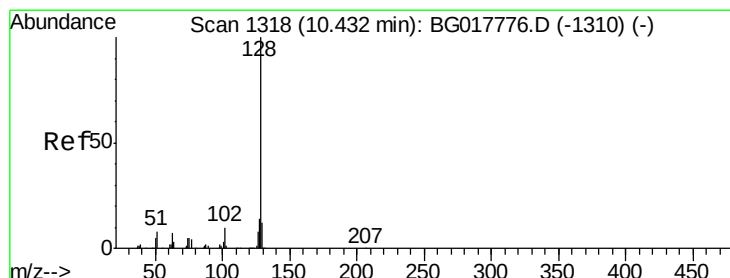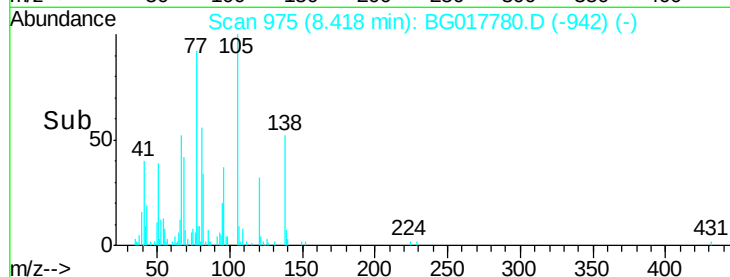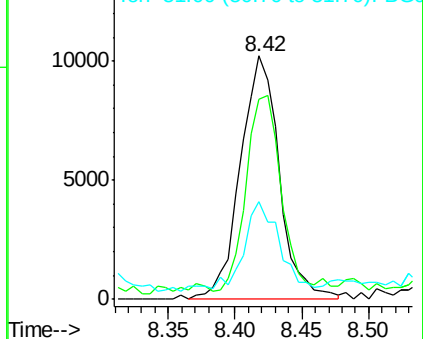

#28

Naphthalene

Concen: 1.44 ng/ul

RT: 10.43 min Scan# 1318

Delta R.T. 0.00 min

Lab File: BG017780.D

Acq: 6 Jul 2015 21:54


Tgt Ion:128 Resp: 39692

Ion Ratio Lower Upper

128 100

129 15.5 8.7 13.1#



127 15.2 11.0 16.6

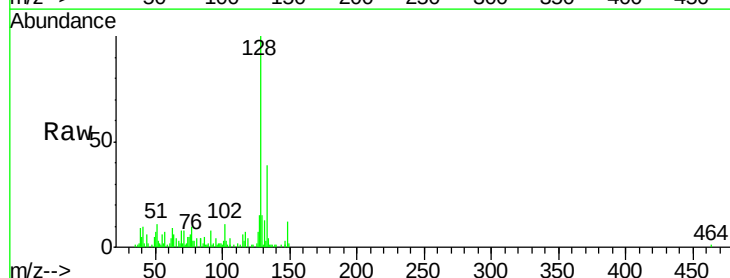


Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E



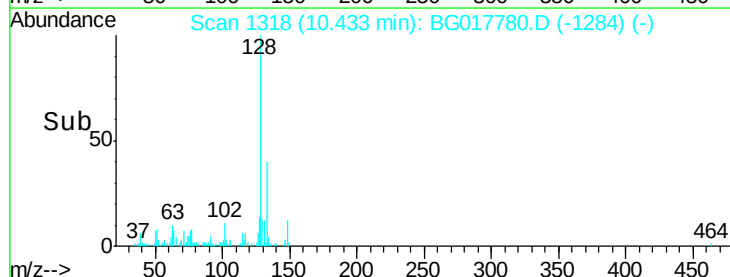
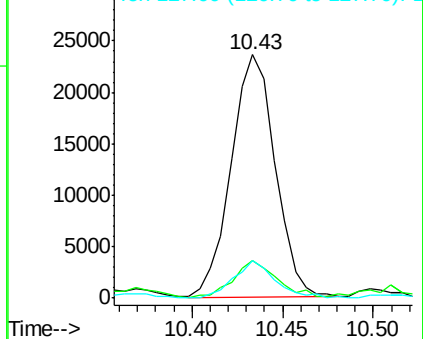




#40
 1,1'-Biphenyl
 Concen: 2.27 ng/ul
 RT: 13.08 min Scan# 1769
 Delta R.T. 0.00 min
 Lab File: BG017780.D
 Acq: 6 Jul 2015 21:54




Instrument :
 BNA_G
 ClientSampleId :


Tgt Ion	Ratio	Lower	Upper
154	100		
153	40.5	33.3	49.9
76	15.9	12.4	18.6

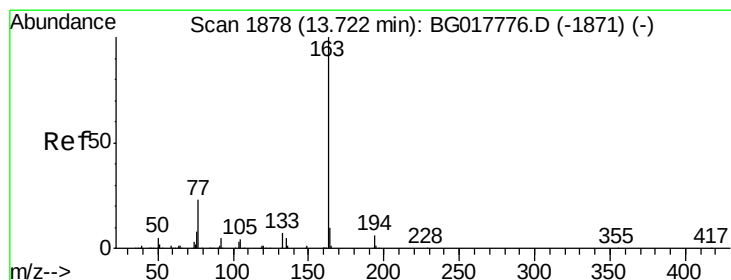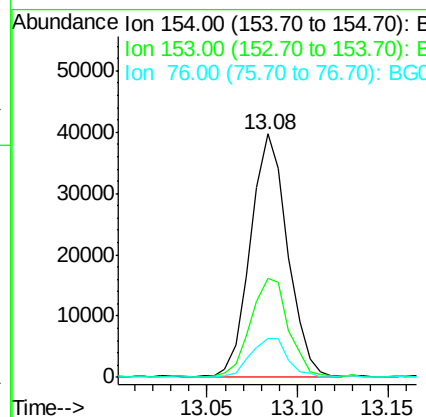

#44
 Dimethylphthalate
 Concen: 2.62 ng/ul
 RT: 13.72 min Scan# 1877
 Delta R.T. -0.00 min
 Lab File: BG017780.D
 Acq: 6 Jul 2015 21:54

Tgt Ion	Ratio	Lower	Upper
163	100		
194	6.6	5.4	8.0
164	11.6	7.7	11.5#



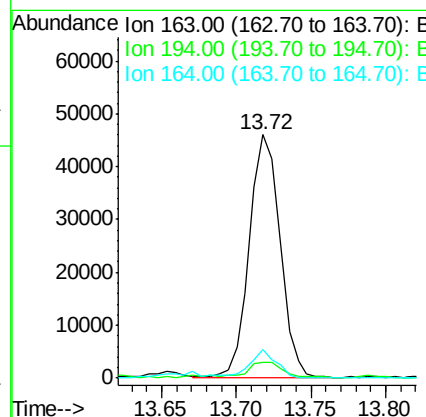
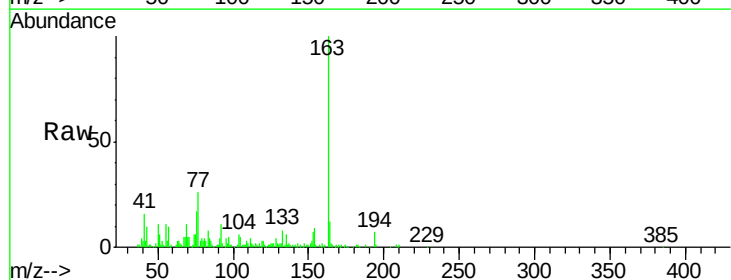




#47
Acenaphthylene
Concen: 3.13 ng/ul
RT: 13.98 min Scan# 1921
Delta R.T. 0.00 min
Lab File: BG017780.D
Acq: 6 Jul 2015 21:54




Instrument :
BNA_G
ClientSampleId :


Tgt Ion	Ratio	Lower	Upper
152	100		
151	22.2	17.0	25.6
153	18.6	11.2	16.8#

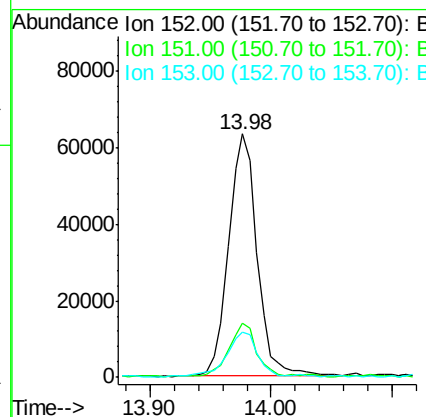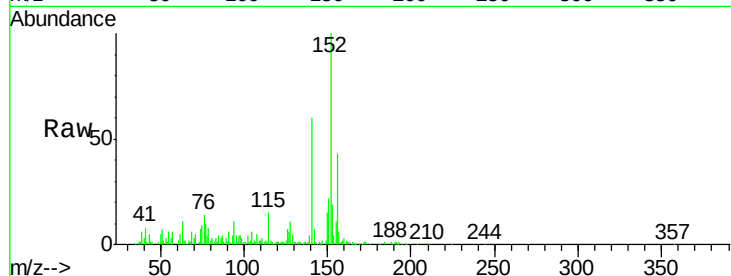

#49
Acenaphthene
Concen: 5.69 ng/ul
RT: 14.32 min Scan# 1980
Delta R.T. 0.00 min
Lab File: BG017780.D
Acq: 6 Jul 2015 21:54

Tgt Ion	Ratio	Lower	Upper
153	100		
152	47.2	37.8	56.6
154	87.3	71.2	106.8

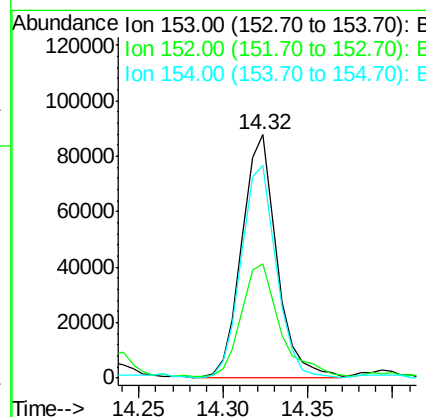



#53

Dibenzenofuran

Concen: 2.18 ng/ul

RT: 14.66 min Scan# 2037

Delta R.T. 0.00 min

Lab File: BG017780.D

Acq: 6 Jul 2015 21:54

Instrument :

BNA_G





ClientSampleId :

Tgt Ion:168 Resp: 65487

Ion Ratio Lower Upper

168 100

139 49.9 32.7 49.1#

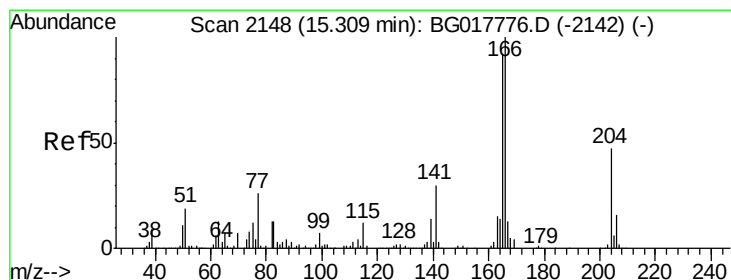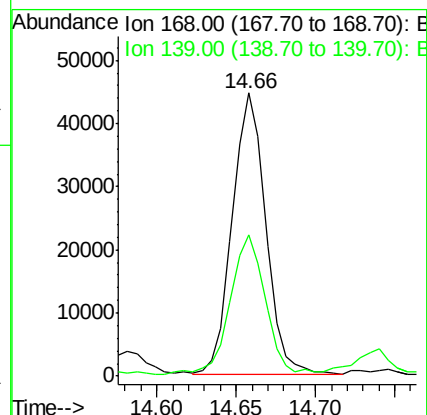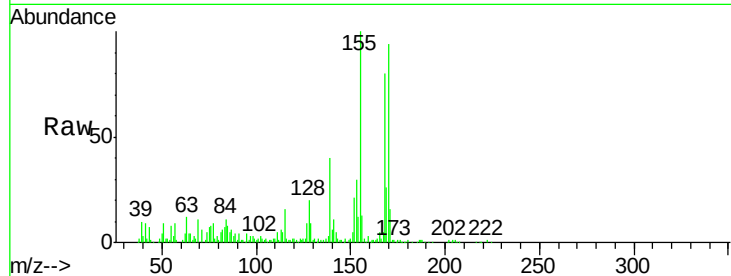

#58

Fluorene

Concen: 6.92 ng/ul m

RT: 15.31 min Scan# 2148

Delta R.T. 0.00 min

Lab File: BG017780.D

Acq: 6 Jul 2015 21:54




Tgt Ion:166 Resp: 184479


Ion Ratio Lower Upper

166 100

165 99.4 75.7 113.5

167 16.4 10.1 15.1#

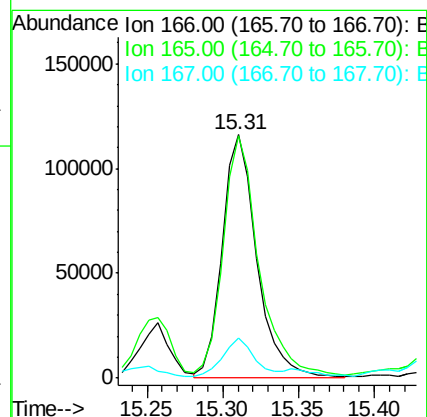



#69

Phenanthrene

Concen: 26.29 ng/ul

RT: 17.06 min Scan# 2445

Delta R.T. 0.01 min

Lab File: BG017780.D

Acq: 6 Jul 2015 21:54

Instrument :

BNA_G

ClientSampleId :


Tgt Ion:178 Resp: 1021665

Ion Ratio Lower Upper

178 100

179 16.8 13.0 19.4




176 19.8 17.0 25.4

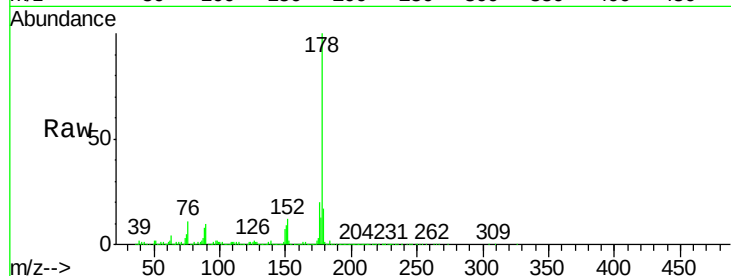

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

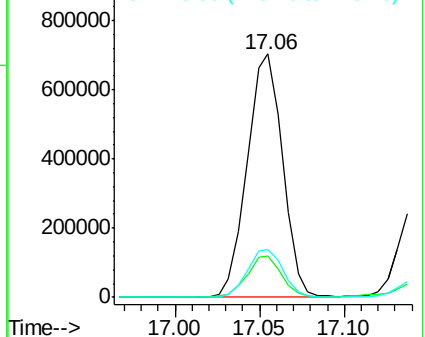

#71

Anthracene

Concen: 9.27 ng/ul

RT: 17.14 min Scan# 2460

Delta R.T. 0.00 min

Lab File: BG017780.D

Acq: 6 Jul 2015 21:54


Tgt Ion:178 Resp: 370475

Ion Ratio Lower Upper

178 100

179 15.7 12.4 18.6



176 19.5 15.3 22.9




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

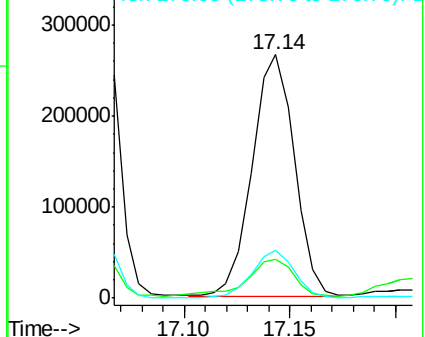







#76
Fluoranthene
Concen: 17.38 ng/ul
RT: 19.08 min Scan# 2789
Delta R.T. 0.00 min
Lab File: BG017780.D
Acq: 6 Jul 2015 21:54

Instrument :
BNA_G
ClientSampleId :

Tgt Ion	Ratio	Lower	Upper
202	100		
101	14.5	12.6	18.8
100	11.0	9.1	13.7




Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

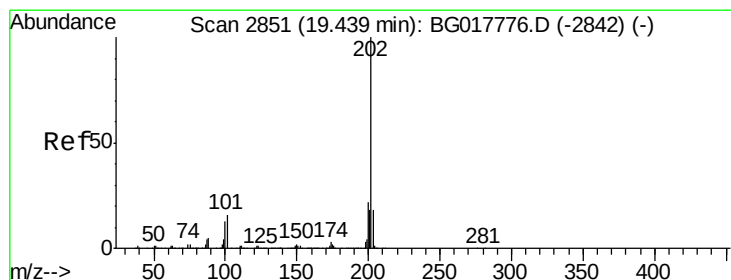
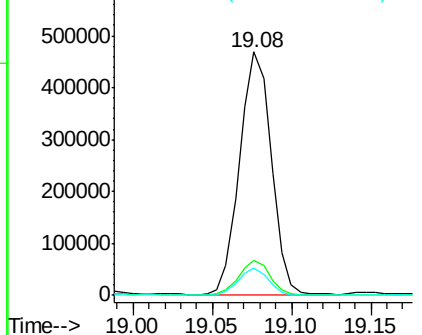



#79
Pyrene
Concen: 26.27 ng/ul
RT: 19.44 min Scan# 2851
Delta R.T. 0.00 min
Lab File: BG017780.D
Acq: 6 Jul 2015 21:54

Tgt Ion	Ratio	Lower	Upper
202	100		
101	17.2	13.1	19.7
100	14.7	11.3	16.9

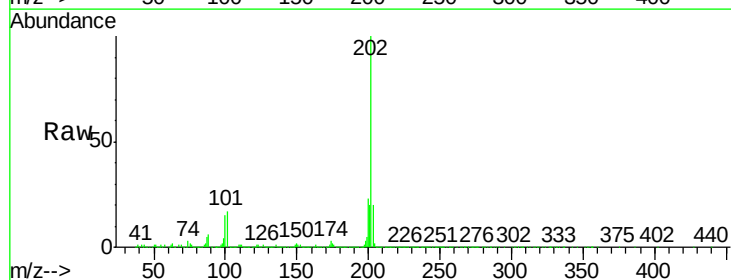

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

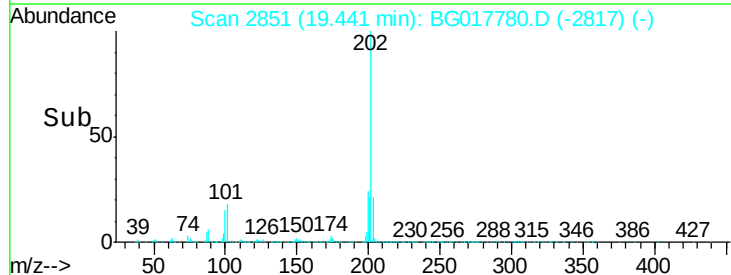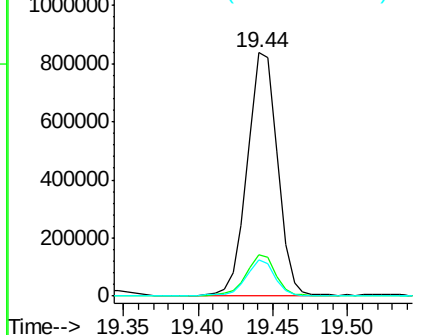

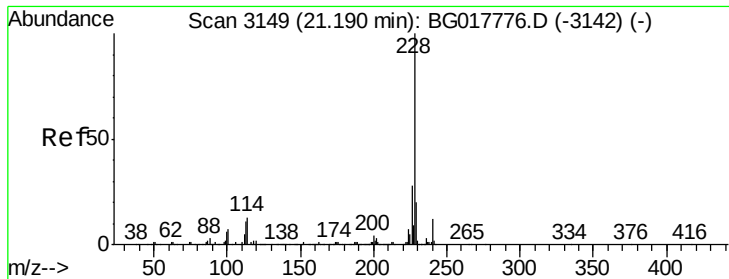

#82

Benzo(a)anthracene

Concen: 9.90 ng/ul m

RT: 21.19 min Scan# 3149

Delta R.T. 0.00 min

Lab File: BG017780.D





Acq: 6 Jul 2015 21:54

Instrument :

BNA_G

ClientSampleId :

Tgt Ion:	228	Resp:	395124
Ion	Ratio	Lower	Upper
228	100		
229	20.4	15.8	23.8
226	39.9	22.2	33.2#

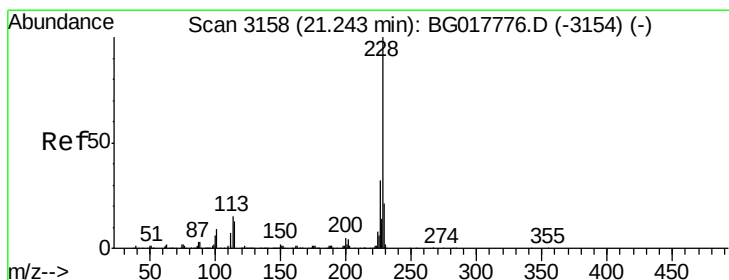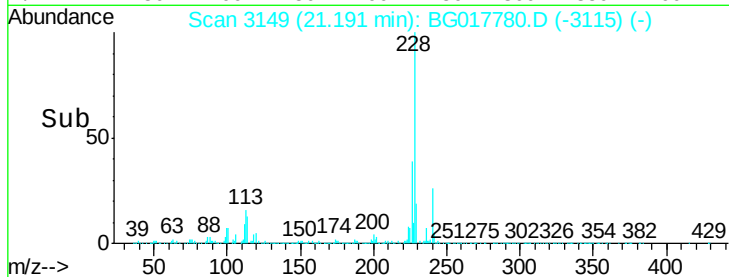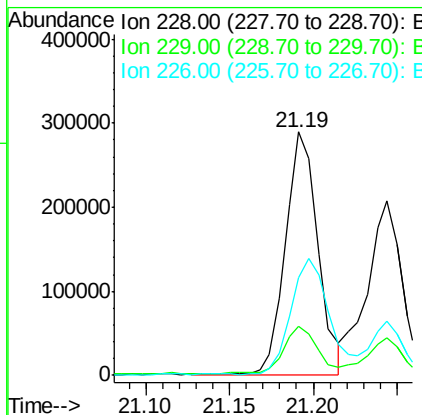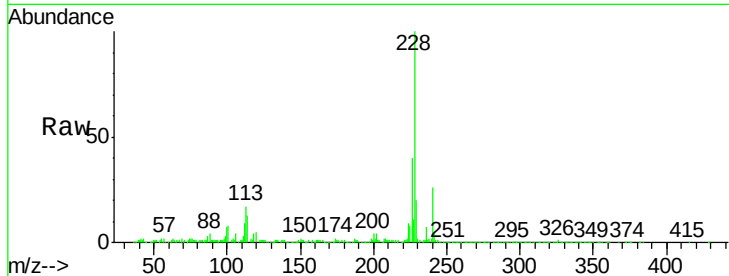

#84

Chrysene

Concen: 7.64 ng/ul




RT: 21.24 min Scan# 3158


Delta R.T. 0.00 min

Lab File: BG017780.D

Acq: 6 Jul 2015 21:54

Tgt Ion:	228	Resp:	288671
Ion	Ratio	Lower	Upper
228	100		
226	31.3	25.6	38.4
229	21.2	16.4	24.6

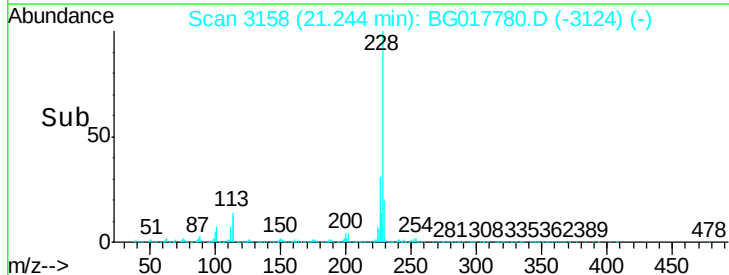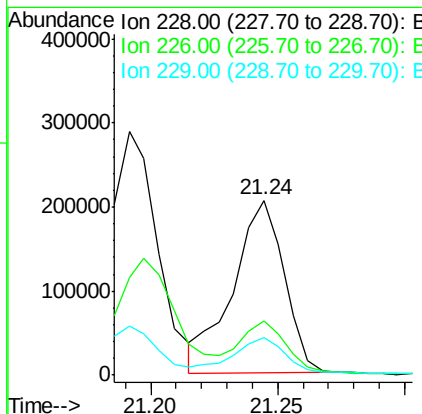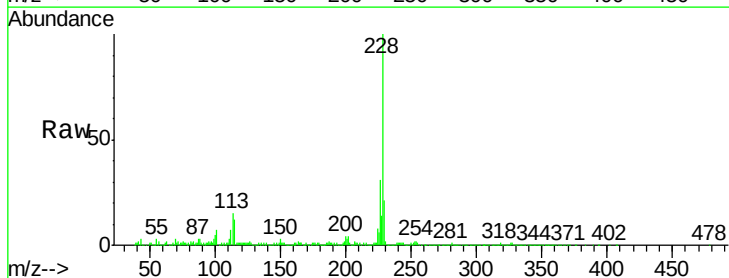



#87

Benzo(b)fluoranthene

Concen: 7.34 ng/ul

RT: 22.77 min Scan# 3417

Delta R.T. 0.01 min

Lab File: BG017780.D


Acq: 6 Jul 2015 21:54

Instrument :




BNA_G

ClientSampleId :

Tgt Ion:	252	Resp:	303402
Ion Ratio		Lower	Upper
252	100		
253	22.6	16.8	25.2
125	15.2	10.4	15.6

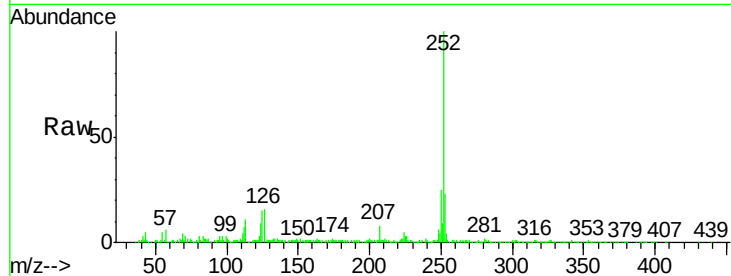

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

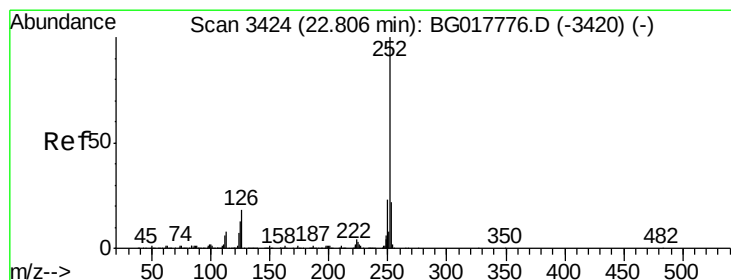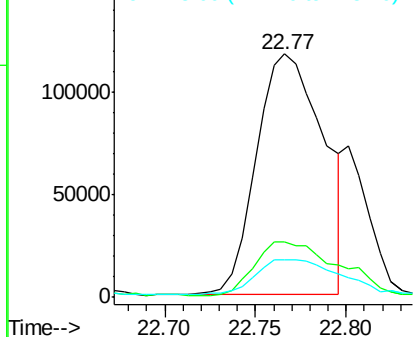

#88

Benzo(k)fluoranthene

Concen: 1.88 ng/ul m


RT: 22.80 min Scan# 3423

Delta R.T. -0.00 min



Lab File: BG017780.D


Acq: 6 Jul 2015 21:54

Tgt Ion:	252	Resp:	73320
Ion Ratio		Lower	Upper
252	100		
253	18.8	17.6	26.4
125	13.3	11.6	17.4



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

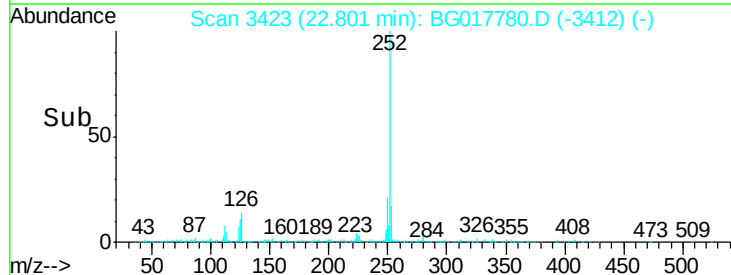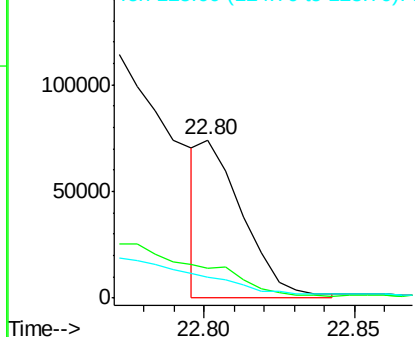



#90

Benzo(a)pyrene

Concen: 9.22 ng/ul

RT: 23.34 min Scan# 3514

Delta R.T. 0.01 min

Lab File: BG017780.D


Acq: 6 Jul 2015 21:54

Instrument :




BNA_G

ClientSampleId :

Tgt Ion:	252	Resp:	362388
Ion Ratio	Lower	Upper	
252	100		
253	21.1	18.3	27.5
125	16.5	12.1	18.1



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

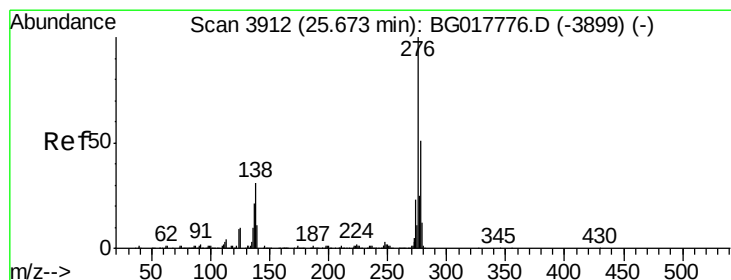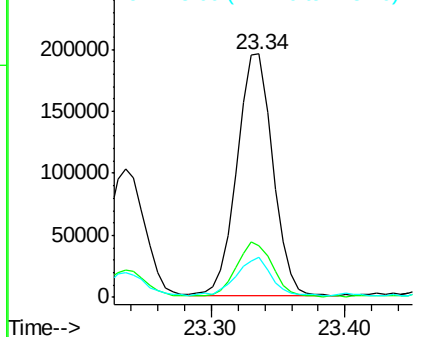

#91

Indeno(1,2,3-cd)pyrene

Concen: 3.42 ng/ul


RT: 25.67 min Scan# 3912

Delta R.T. 0.00 min



Lab File: BG017780.D


Acq: 6 Jul 2015 21:54

Tgt Ion:	276	Resp:	146797
Ion Ratio	Lower	Upper	
276	100		
138	32.1	26.1	39.1
277	28.0	20.9	31.3



Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E




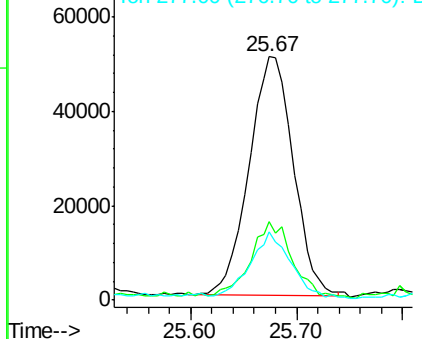




#92
Dibenzo(a,h)anthracene
Concen: 1.18 ng/ul
RT: 25.69 min Scan# 3914
Delta R.T. -0.00 min
Lab File: BG017780.D
Acq: 6 Jul 2015 21:54

Instrument :
BNA_G
ClientSampleId :

Tgt Ion:278 Resp: 42779
Ion Ratio Lower Upper
278 100
139 0.0 16.3 24.5#
279 23.3 18.7 28.1

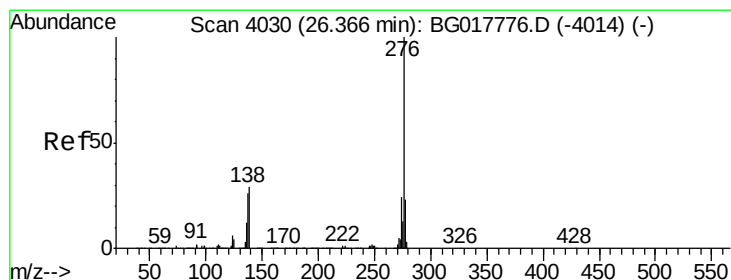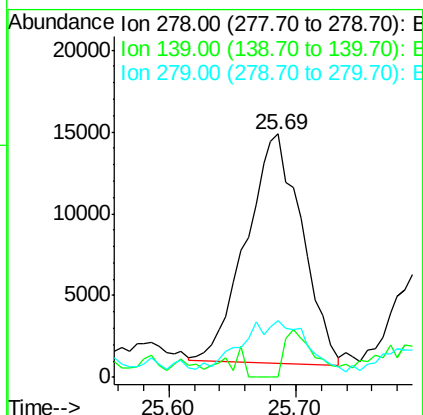

#93
Benzo(g,h,i)perylene
Concen: 3.56 ng/ul
RT: 26.37 min Scan# 4030
Delta R.T. 0.00 min
Lab File: BG017780.D
Acq: 6 Jul 2015 21:54

Tgt Ion:276 Resp: 127624
Ion Ratio Lower Upper
276 100
138 25.7 25.1 37.7
277 23.6 18.7 28.1

