

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070616\
 Data File : BG022870.D
 Acq On : 6 Jul 2016 9:42
 Operator : UM/SJ
 Sample : H3818-22
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHT7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.961	19	21	23	rBV3	15662	11371	0.32%	0.027%
2	4.242	237	239	241	rBV2	9593	9964	0.28%	0.024%
3	4.365	257	260	262	rVB3	7084	7330	0.20%	0.017%
4	4.389	262	264	266	rBV3	8586	8478	0.24%	0.020%
5	4.612	300	302	305	rBV3	6912	9154	0.26%	0.022%
6	4.841	338	341	343	rVB4	10896	9578	0.27%	0.023%
7	4.870	343	346	347	rBV3	11352	9301	0.26%	0.022%
8	4.994	364	367	371	rBV4	5034	7359	0.21%	0.017%
9	5.799	498	504	506	rBV5	6639	12330	0.34%	0.029%
10	5.846	509	512	514	rVV2	8967	7322	0.20%	0.017%
11	6.139	560	562	564	rBV3	7441	8670	0.24%	0.021%
12	6.198	570	572	579	rVV7	7774	13181	0.37%	0.031%
13	6.345	594	597	600	rBV4	6203	8424	0.24%	0.020%
14	6.480	619	620	625	rBV4	5361	8706	0.24%	0.021%
15	6.774	668	670	671	rBV2	9943	7072	0.20%	0.017%
16	6.986	704	706	710	rBV2	5820	7333	0.20%	0.017%
17	7.109	725	727	729	rBV2	9236	6712	0.19%	0.016%
18	7.315	754	762	775	rBV	490095	914210	25.53%	2.171%
19	7.479	784	790	800	rBV	332128	565324	15.79%	1.342%
20	7.691	817	826	834	rBV	428338	789114	22.04%	1.874%
21	7.767	837	839	842	rVB2	8926	8432	0.24%	0.020%
22	7.808	845	846	850	rBV3	7875	10447	0.29%	0.025%
23	7.990	873	877	880	rVB4	5788	6558	0.18%	0.016%
24	8.072	886	891	893	rBV4	5891	9711	0.27%	0.023%
25	8.166	896	907	918	rVB	485976	878521	24.54%	2.086%
26	8.290	922	928	929	rBV3	6246	10972	0.31%	0.026%
27	8.337	931	936	939	rBV5	8512	13694	0.38%	0.033%
28	8.396	942	946	951	rVV6	10654	19888	0.56%	0.047%
29	8.454	951	956	962	rVV8	8770	13572	0.38%	0.032%
30	8.631	984	986	989	rVB3	8778	8670	0.24%	0.021%
31	8.872	1017	1027	1034	rBV2	642427	1148150	32.07%	2.726%
32	9.036	1054	1055	1060	rVB3	8799	6887	0.19%	0.016%
33	9.336	1099	1106	1116	rVB	493926	879281	24.56%	2.088%
34	9.436	1118	1123	1130	rVB5	24561	39492	1.10%	0.094%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070616\
 Data File : BG022870.D
 Acq On : 6 Jul 2016 9:42
 Operator : UM/SJ
 Sample : H3818-22
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHT7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
 Title : SVOA CALIBRATION

35	9.641	1152	1158	1159	rBV3	7380	11802	0.33%	0.028%
36	9.676	1162	1164	1166	rBV2	8952	7608	0.21%	0.018%
37	9.723	1168	1172	1175	rBV4	18212	25650	0.72%	0.061%
38	9.906	1200	1203	1206	rBV5	6207	8135	0.23%	0.019%
39	10.064	1222	1230	1240	rBV2	452252	821043	22.93%	1.949%
40	10.282	1264	1267	1270	rBV4	6942	8284	0.23%	0.020%
41	10.405	1285	1288	1289	rBV2	7282	6578	0.18%	0.016%
42	10.611	1316	1323	1333	rVV	681267	1278235	35.70%	3.035%
43	10.681	1333	1335	1337	rVB3	9760	7709	0.22%	0.018%
44	10.716	1339	1341	1345	rVB4	9013	8426	0.24%	0.020%
45	10.904	1368	1373	1374	rBV2	7421	9690	0.27%	0.023%
46	10.993	1380	1388	1395	rBV	780559	1379835	38.54%	3.276%
47	11.128	1403	1411	1419	rBV	590759	1087953	30.39%	2.583%
48	11.721	1510	1512	1514	rBV2	6724	6724	0.19%	0.016%
49	11.768	1518	1520	1525	rVV5	8593	14864	0.42%	0.035%
50	11.827	1525	1530	1534	rVB7	6783	13447	0.38%	0.032%
51	11.986	1554	1557	1561	rBV4	7790	14318	0.40%	0.034%
52	12.162	1585	1587	1592	rBV5	6410	8217	0.23%	0.020%
53	12.567	1651	1656	1663	rVB6	14681	29315	0.82%	0.070%
54	12.649	1669	1670	1676	rVB7	7305	7982	0.22%	0.019%
55	12.738	1683	1685	1688	rVB3	7600	7454	0.21%	0.018%
56	12.767	1688	1690	1692	rBV2	8221	8866	0.25%	0.021%
57	13.102	1743	1747	1748	rVB4	8552	7987	0.22%	0.019%
58	13.155	1754	1756	1759	rBV4	6901	8138	0.23%	0.019%
59	13.319	1781	1784	1790	rVB7	12072	20996	0.59%	0.050%
60	13.390	1794	1796	1798	rBV3	8010	9956	0.28%	0.024%
61	13.454	1805	1807	1808	rBV2	8810	7704	0.22%	0.018%
62	13.496	1812	1814	1816	rBV3	8050	7826	0.22%	0.019%
63	13.578	1824	1828	1829	rBV3	5594	6854	0.19%	0.016%
64	13.613	1830	1834	1836	rVB4	11813	15558	0.43%	0.037%
65	13.830	1869	1871	1874	rBV4	6728	8768	0.24%	0.021%
66	14.118	1918	1920	1924	rVB5	8711	10601	0.30%	0.025%
67	14.201	1927	1934	1938	rVV	1358144	2040366	56.99%	4.844%
68	14.248	1938	1942	1949	rVB	678486	970635	27.11%	2.304%
69	14.389	1964	1966	1969	rVB4	9914	8668	0.24%	0.021%
70	14.436	1972	1974	1977	rBV4	6854	8374	0.23%	0.020%
71	14.500	1978	1985	1992	rVV	1403268	2224510	62.13%	5.281%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070616\
 Data File : BG022870.D
 Acq On : 6 Jul 2016 9:42
 Operator : UM/SJ
 Sample : H3818-22
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHT7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
 Title : SVOA CALIBRATION

72	14.671	2011	2014	2018	rBV3	28483	38617	1.08%	0.092%
73	14.753	2023	2028	2029	rBV5	6384	9694	0.27%	0.023%
74	14.806	2030	2037	2044	rVB2	1444957	2308758	64.48%	5.481%
75	14.947	2059	2061	2063	rBV3	7983	6784	0.19%	0.016%
76	15.000	2063	2070	2076	rBV	457575	823518	23.00%	1.955%
77	15.211	2102	2106	2111	rVB6	36221	55907	1.56%	0.133%
78	15.276	2114	2117	2119	rBV4	15911	18449	0.52%	0.044%
79	15.352	2128	2130	2133	rBV4	7872	7485	0.21%	0.018%
80	15.411	2139	2140	2143	rBV3	10250	12518	0.35%	0.030%
81	15.581	2165	2169	2172	rBV4	20129	35452	0.99%	0.084%
82	15.622	2172	2176	2182	rVB4	53135	80121	2.24%	0.190%
83	15.675	2182	2185	2190	rBV7	16958	33673	0.94%	0.080%
84	15.793	2198	2205	2212	rBV	1955779	3031570	84.67%	7.198%
85	15.904	2218	2224	2230	rBV	524152	788861	22.03%	1.873%
86	16.028	2242	2245	2250	rVB8	49906	75692	2.11%	0.180%
87	16.251	2280	2283	2285	rBV4	14977	11387	0.32%	0.027%
88	16.486	2319	2323	2326	rBV4	51061	91242	2.55%	0.217%
89	16.997	2406	2410	2413	rBV6	19670	31726	0.89%	0.075%
90	17.279	2455	2458	2464	rBV	90636	124085	3.47%	0.295%
91	17.338	2464	2468	2472	rVV7	37089	62708	1.75%	0.149%
92	17.555	2498	2505	2511	rBV	1820490	2783155	77.74%	6.608%
93	17.655	2516	2522	2531	rVB	1888510	3006988	83.99%	7.139%
94	18.026	2582	2585	2590	rVB2	66020	76584	2.14%	0.182%
95	18.419	2648	2652	2657	rBV3	168954	235178	6.57%	0.558%
96	19.212	2785	2787	2788	rBV2	33599	23231	0.65%	0.055%
97	19.935	2904	2910	2920	rBV	2333033	3580310	100.00%	8.500%
98	21.856	3231	3237	3243	rBV	1857882	2989051	83.49%	7.097%
99	25.000	3763	3772	3783	rVB2	1053537	2981520	83.28%	7.079%
100	25.229	3803	3811	3825	rVB2	1074828	3191009	89.13%	7.576%


Sum of corrected areas: 42119557

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070616\
Data File : BG022870.D
Acq On : 6 Jul 2016 9:42
Operator : UM/SJ
Sample : H3818-22
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDHT7

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

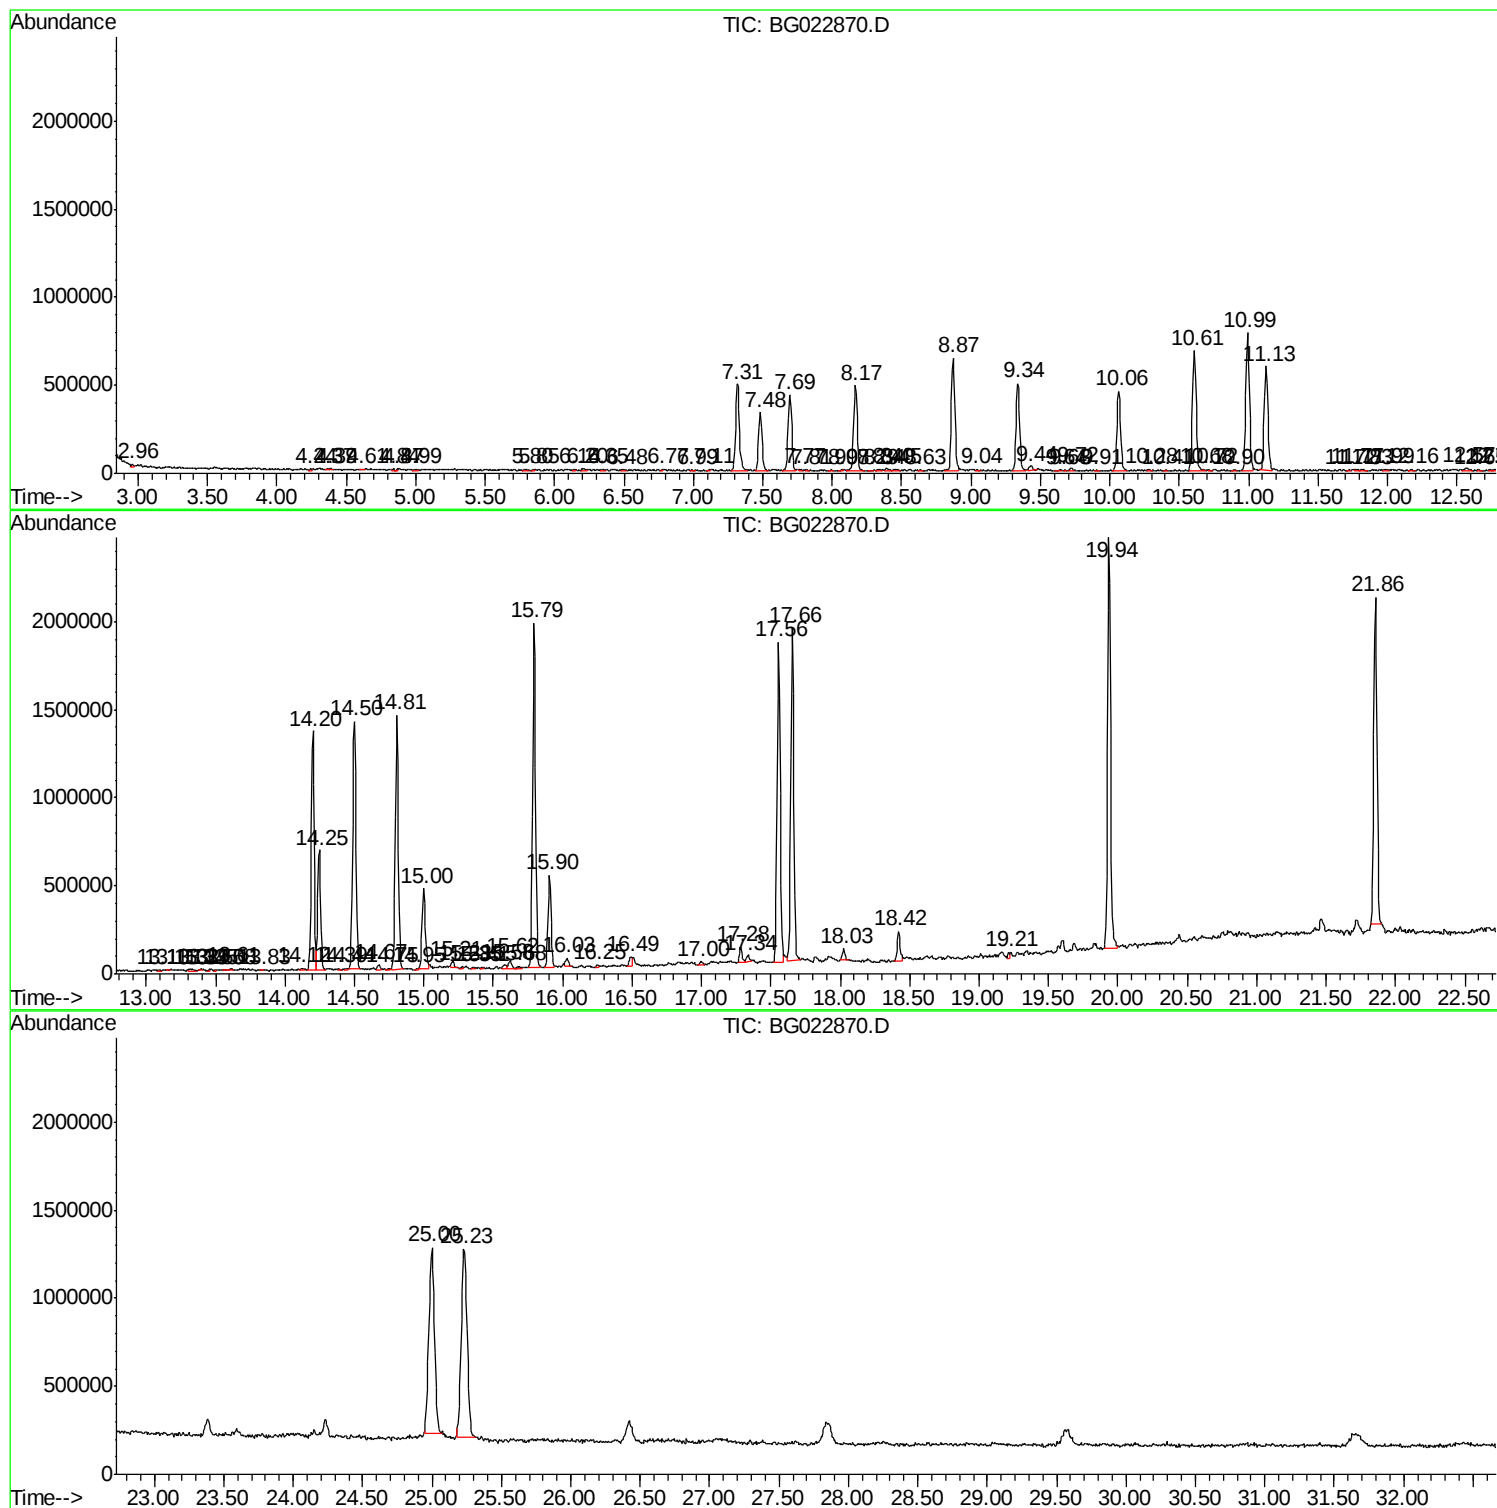

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070616\
Data File : BG022870.D
Acq On : 6 Jul 2016 9:42
Operator : UM/SJ
Sample : H3818-22
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDHT7

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070616\
Data File : BG022870.D
Acq On : 6 Jul 2016 9:42
Operator : UM/SJ
Sample : H3818-22
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDHT7

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc