



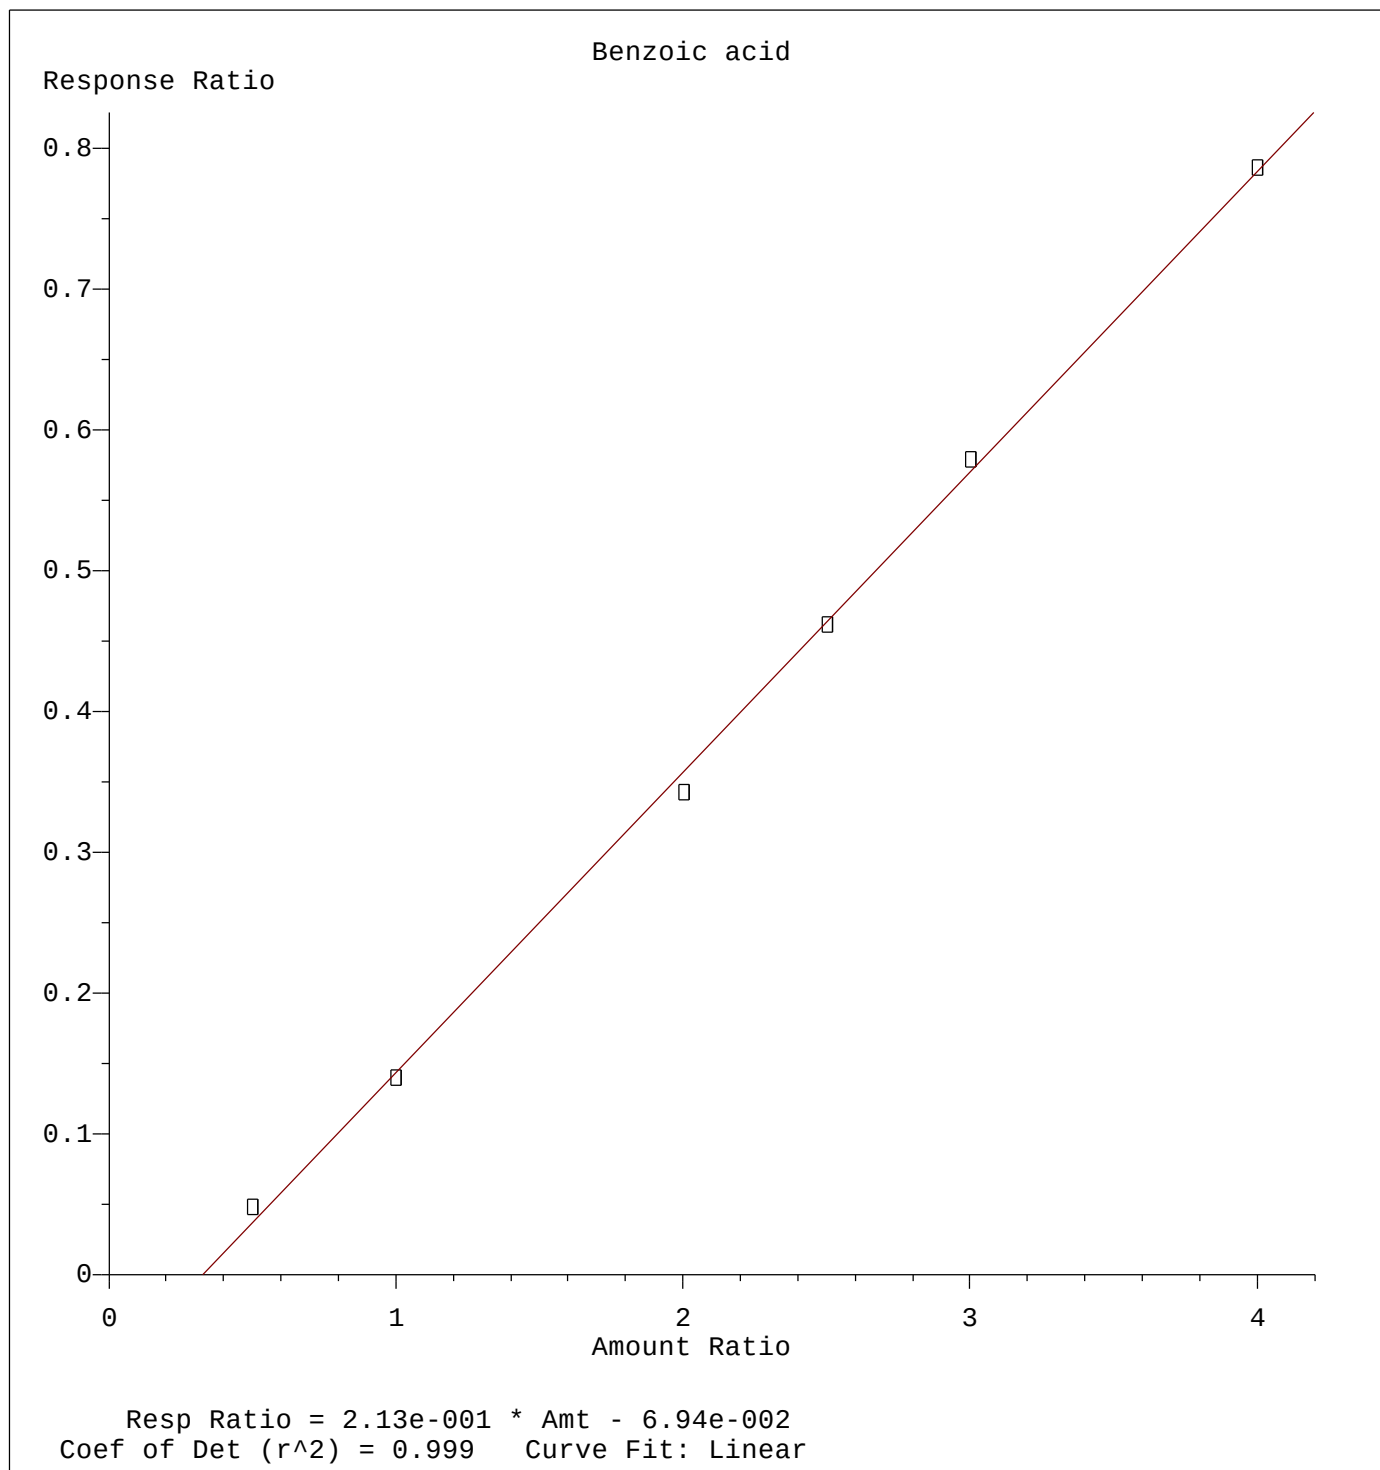


Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG070620.M
Calibration Table Last Updated: Tue Jul 07 09:58:42 2020

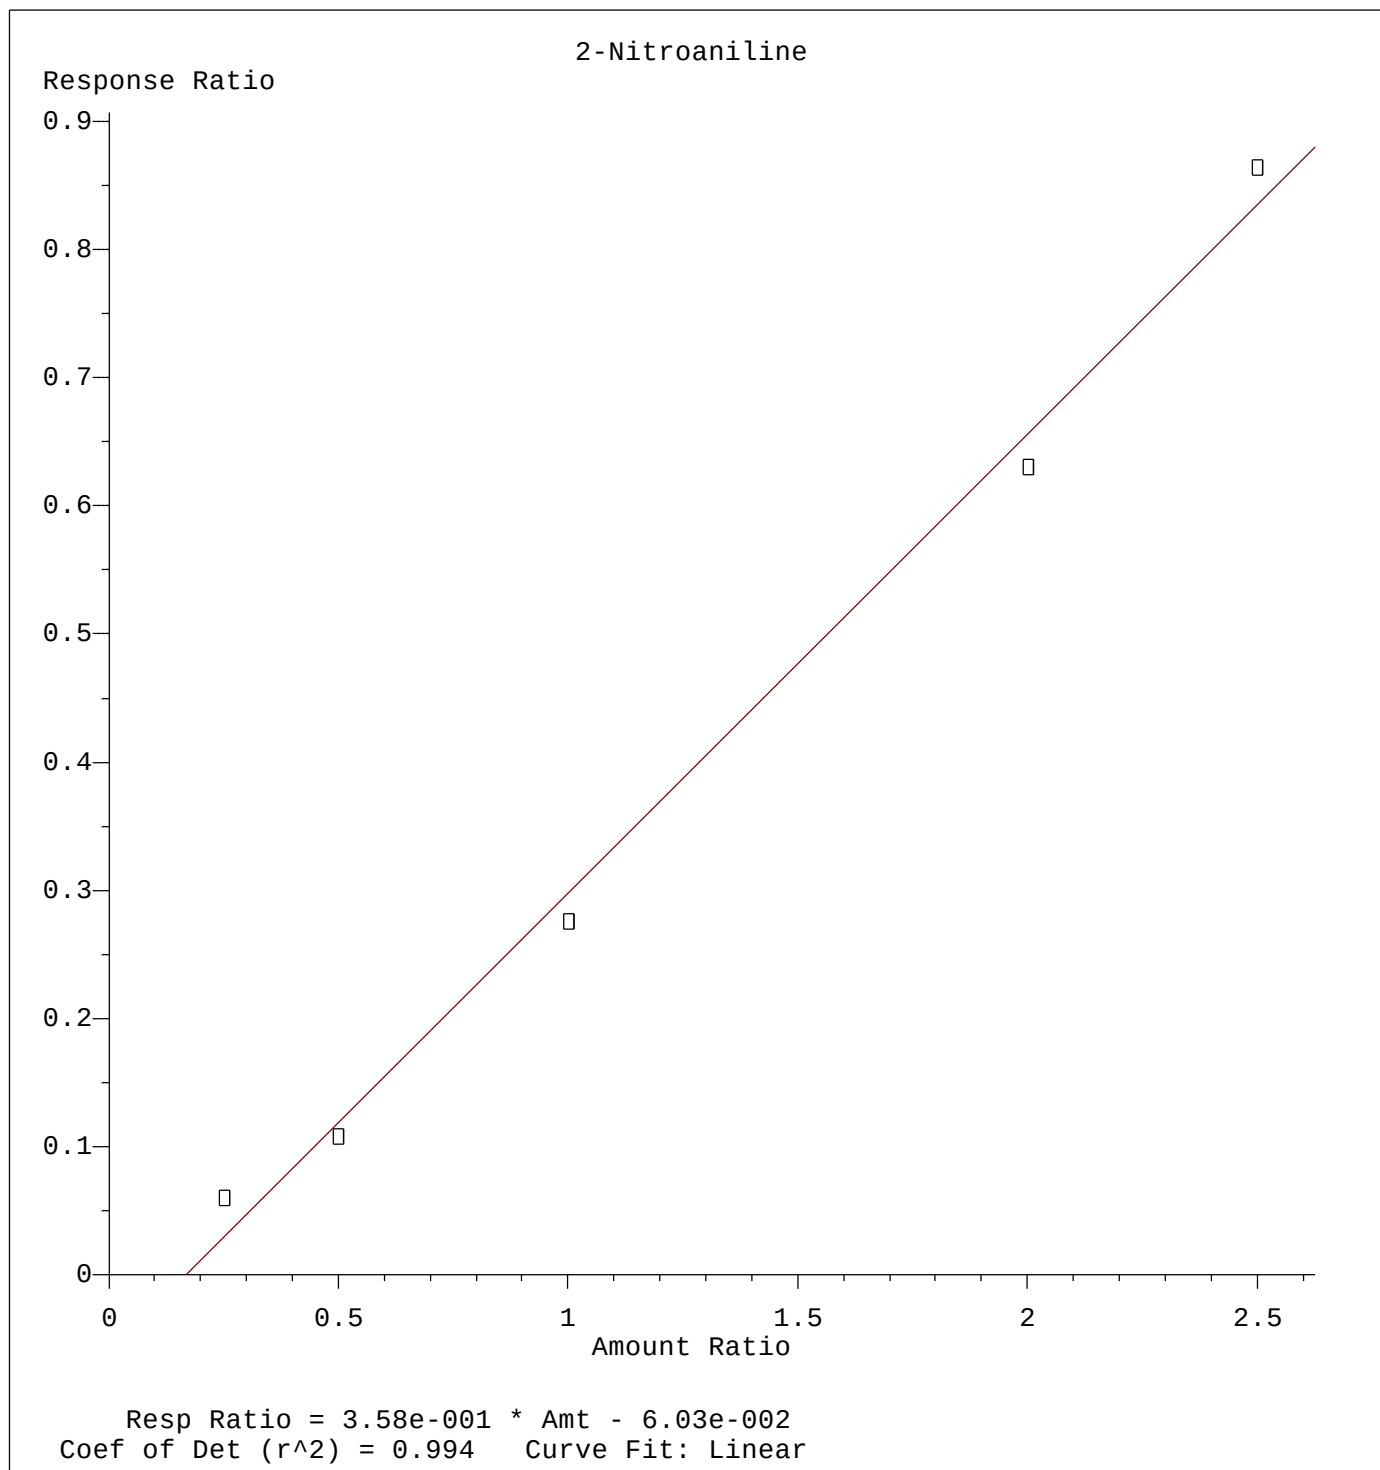

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG070620.M
Calibration Table Last Updated: Tue Jul 07 09:58:42 2020


2,6-Dinitrotoluene

Response Ratio

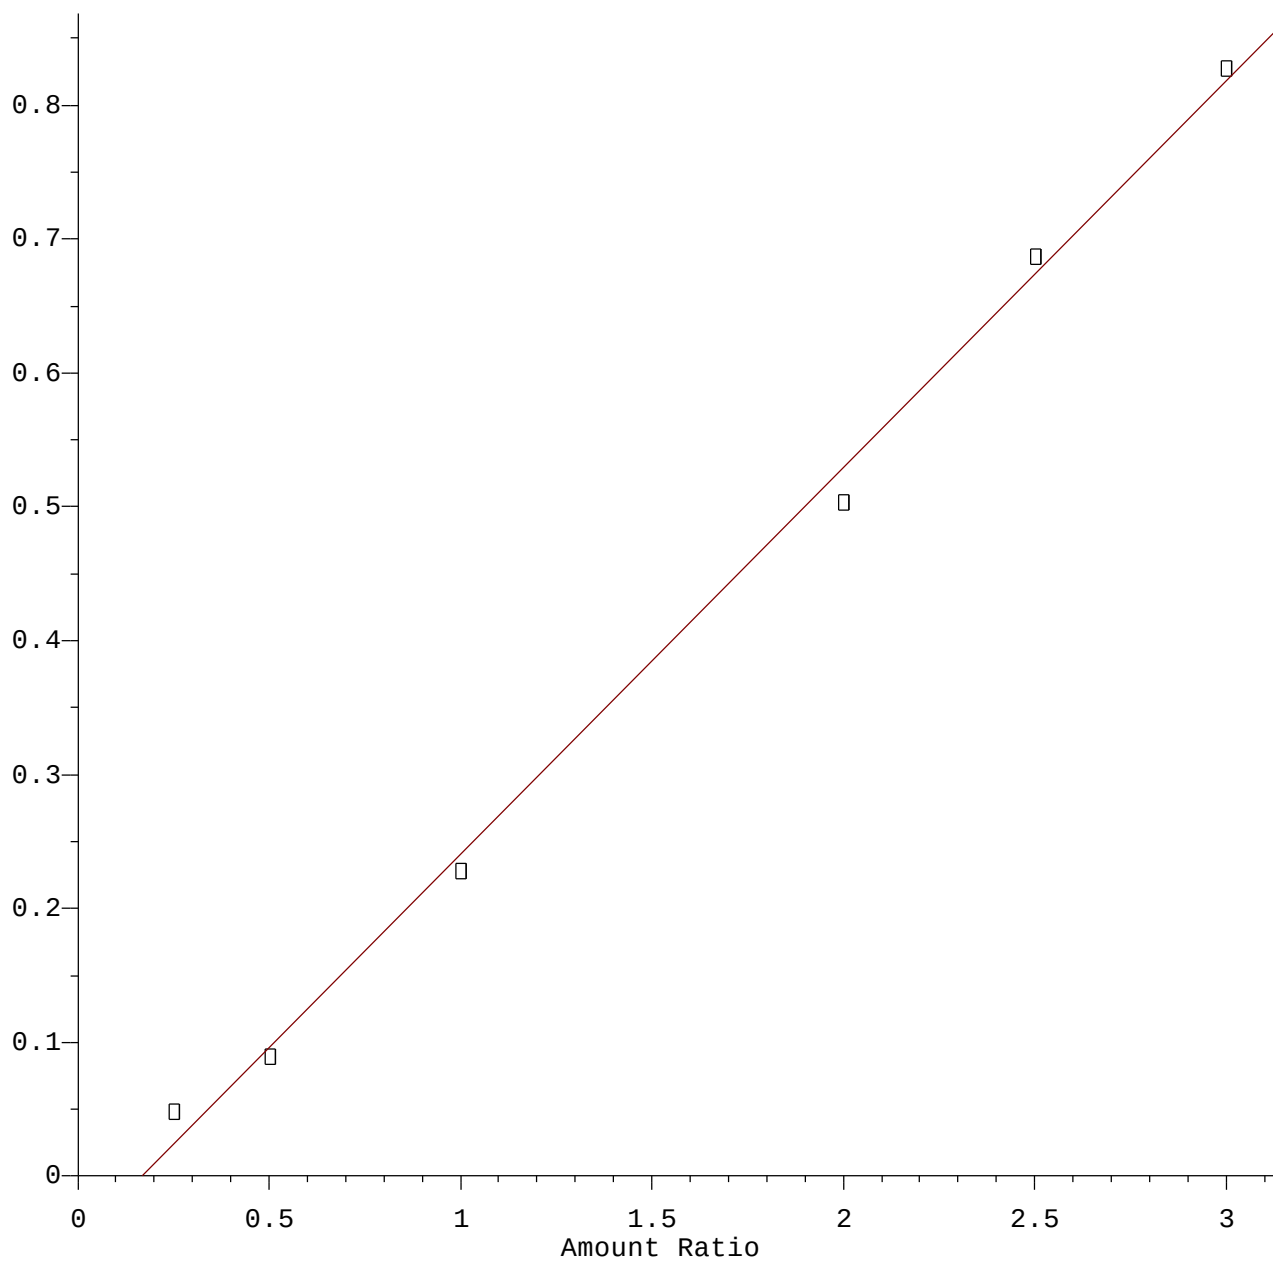


Resp Ratio = $2.88 \times 10^{-1} \times \text{Amt} - 4.77 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG070620.M
Calibration Table Last Updated: Tue Jul 07 09:58:42 2020

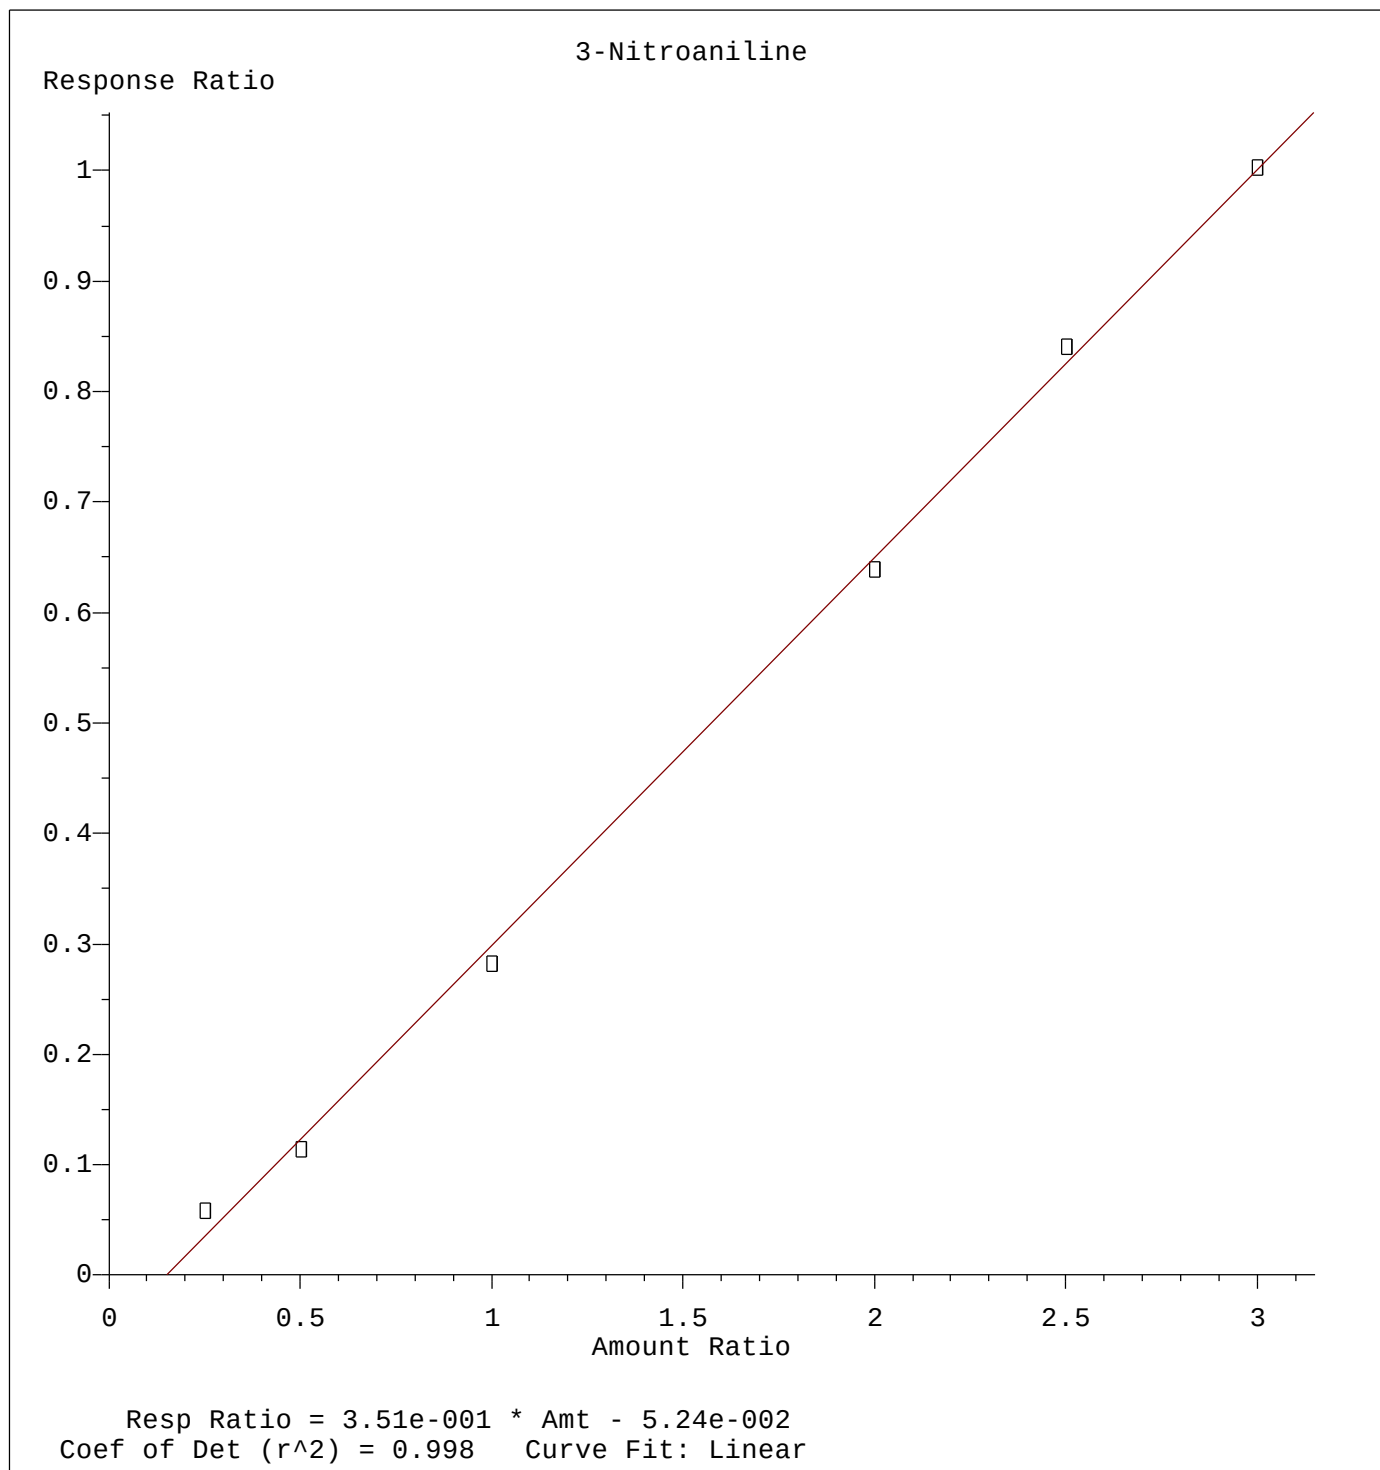


Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG070620.M
Calibration Table Last Updated: Tue Jul 07 09:58:42 2020

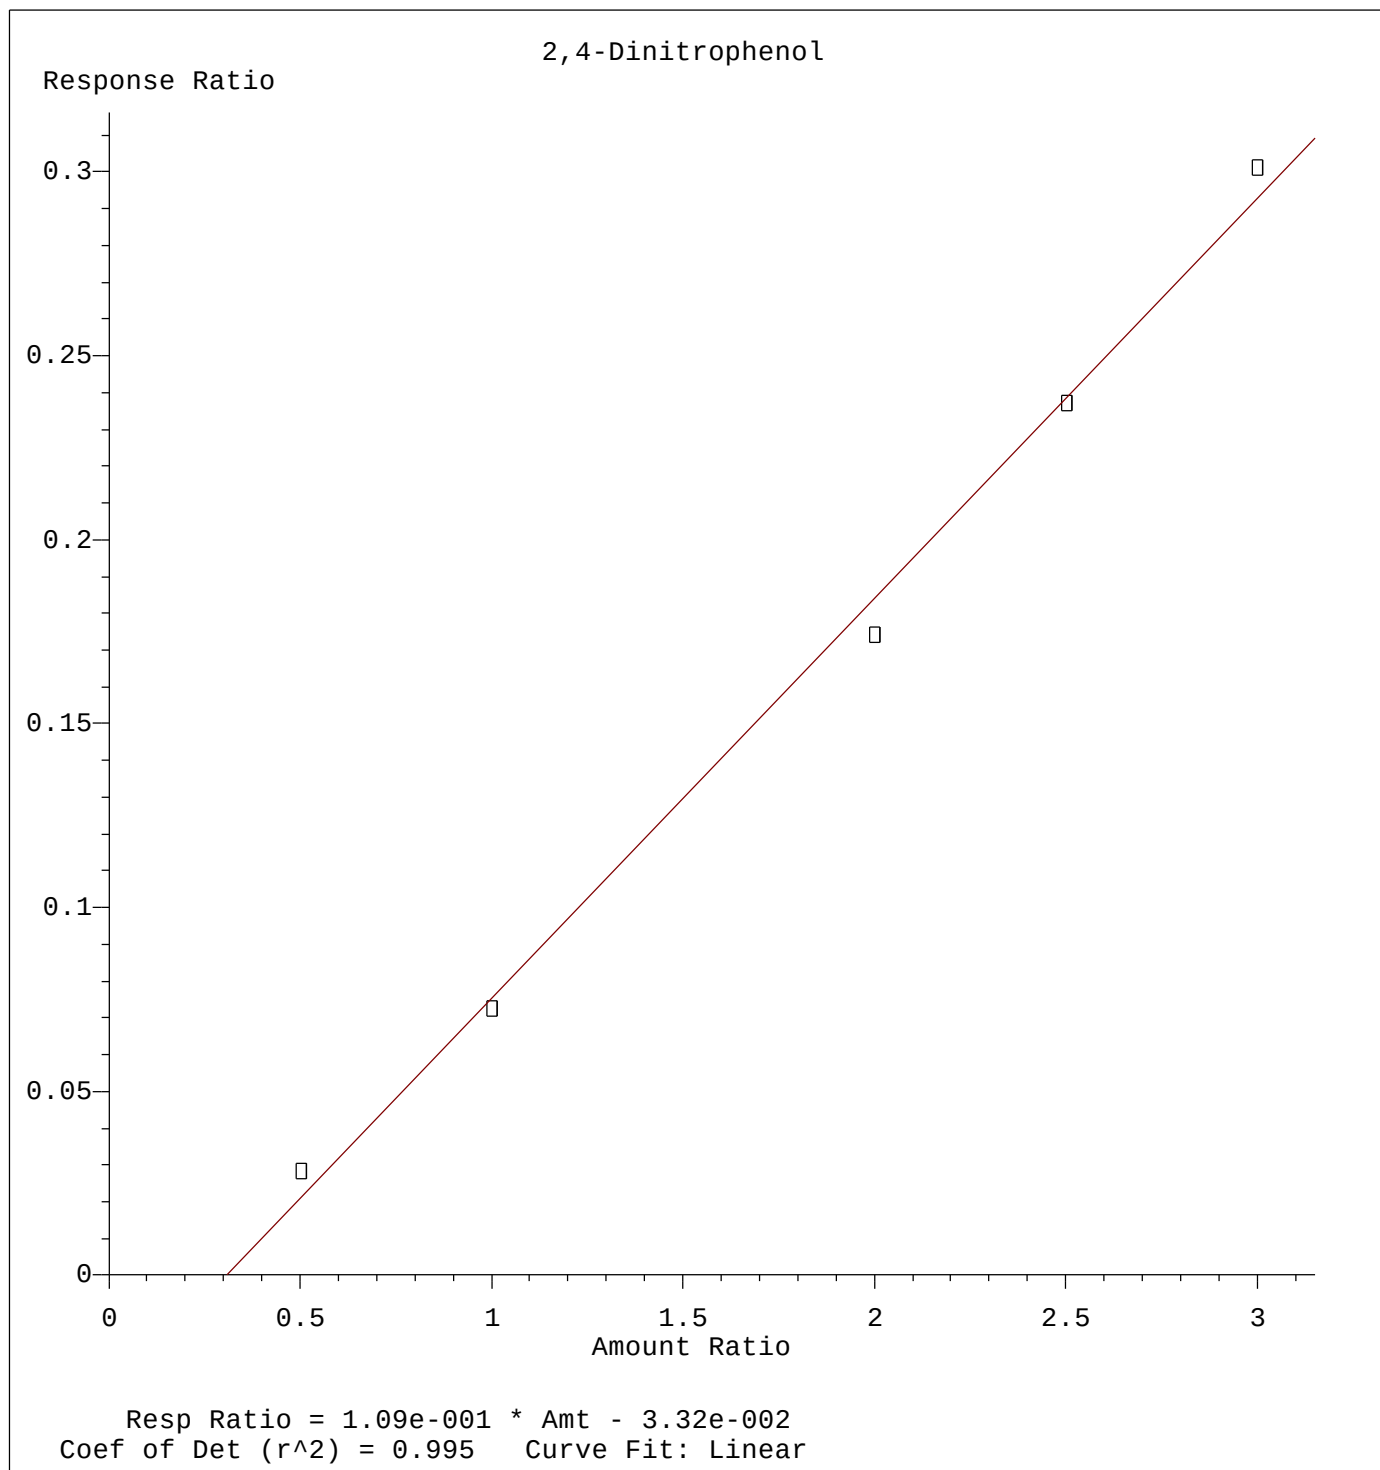

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG070620.M
Calibration Table Last Updated: Tue Jul 07 09:58:42 2020

2,4-Dinitrotoluene


Response Ratio

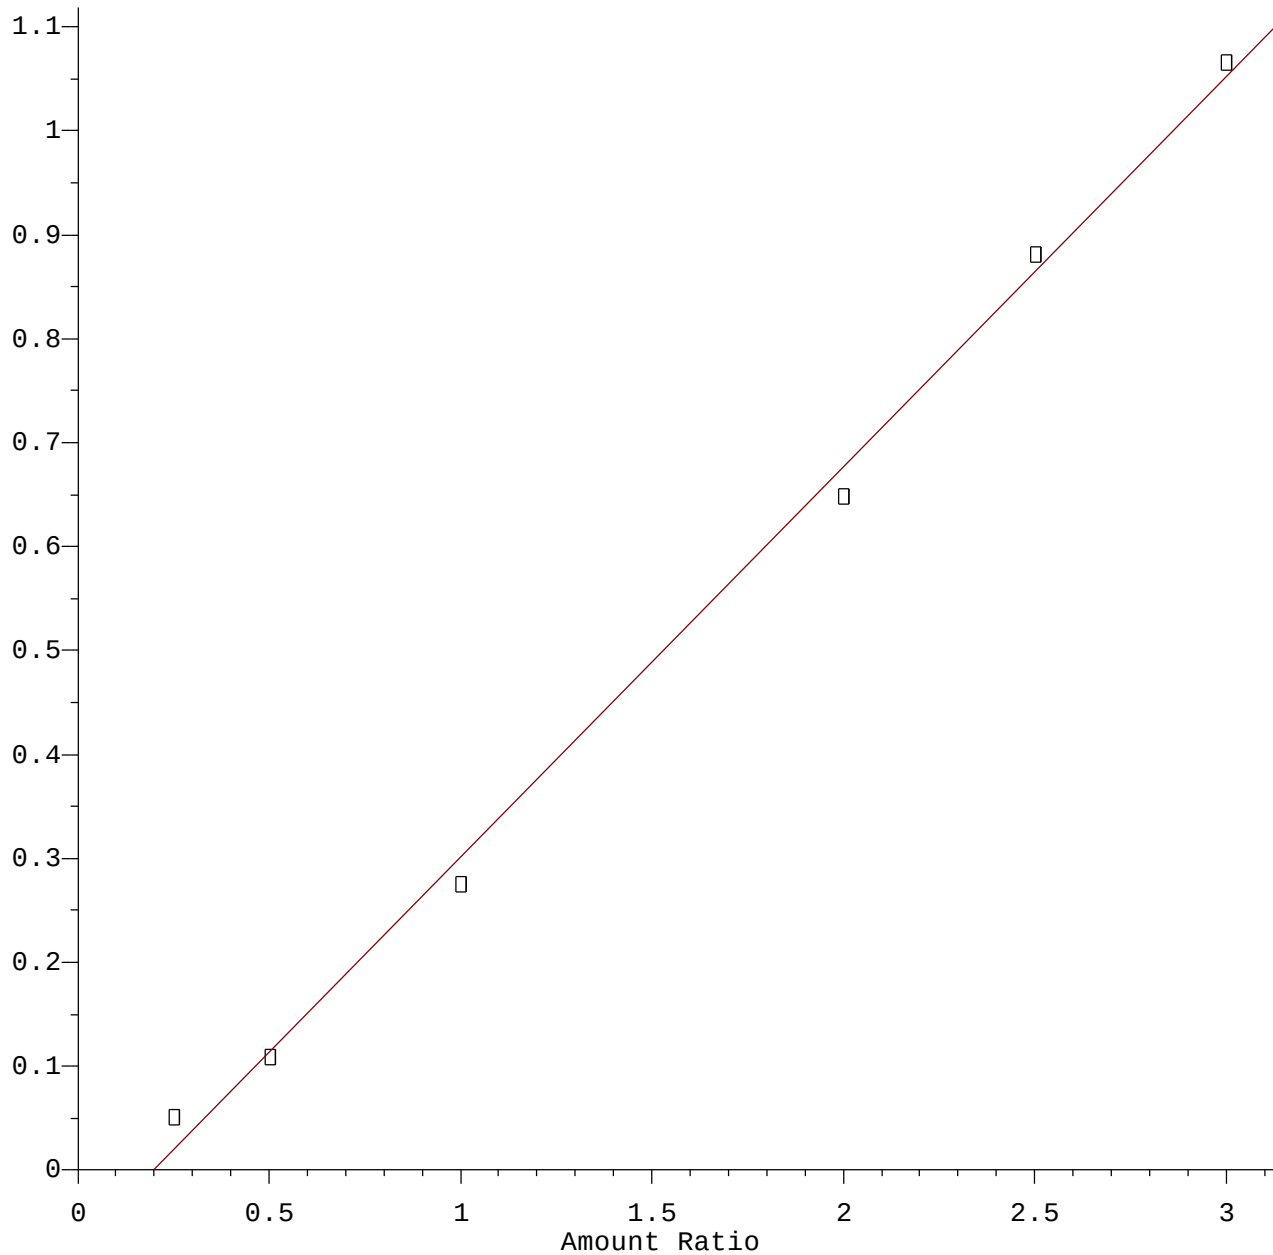

Resp Ratio = $3.76 \times 10^{-1} \times \text{Amt} - 7.45 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG070620.M
Calibration Table Last Updated: Tue Jul 07 09:58:42 2020

4,6-Dinitro-2-methylphenol

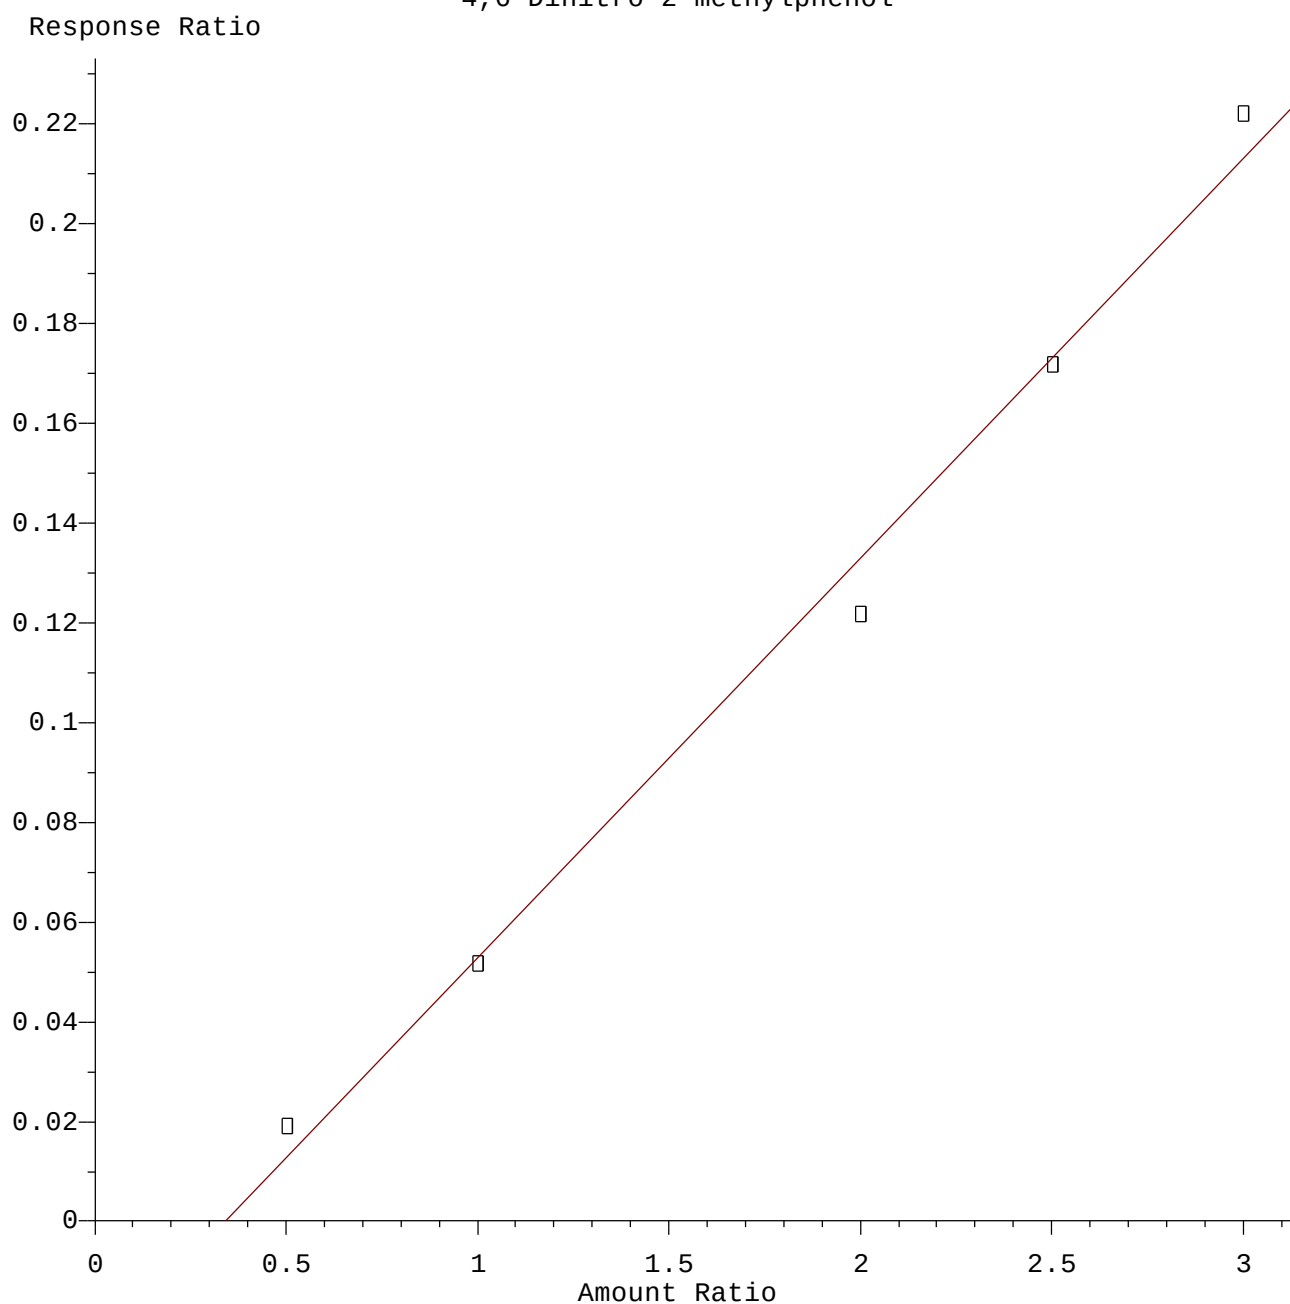

Resp Ratio = 8.02×10^{-2} * Amt - 2.72×10^{-2}
Coef of Det (r^2) = 0.991 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG070620.M
Calibration Table Last Updated: Tue Jul 07 09:58:42 2020