


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG070620\  
 Data File : BG045943.D  
 Acq On : 6 Jul 2020 16:59  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG070620.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Jul 07 09:58:42 2020

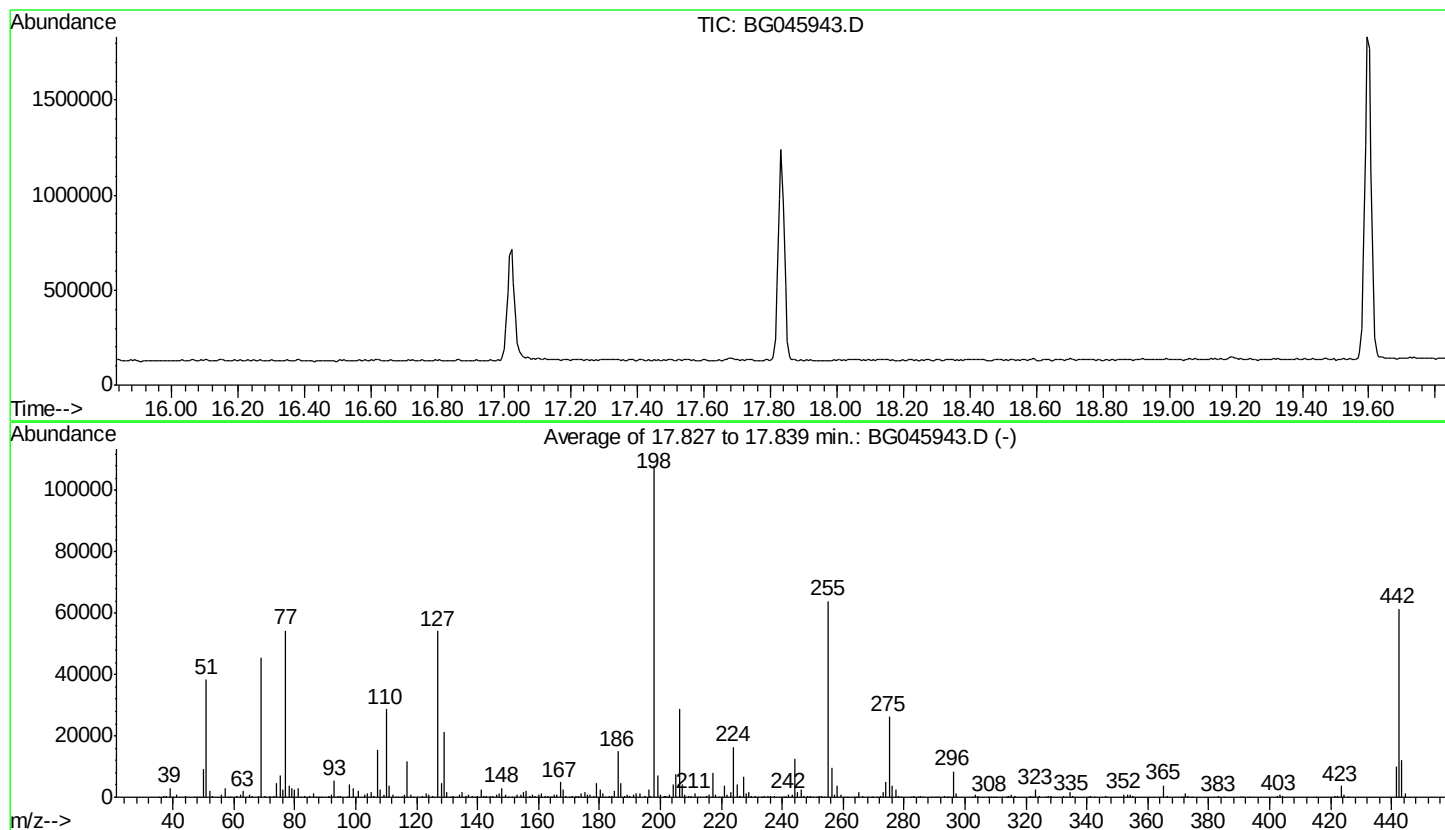

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2502

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 35.5      | 38347   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.3       | 573     | PASS             |
| 69          | 198          | 0.00         | 100          | 41.9      | 45299   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.9       | 387     | PASS             |
| 127         | 198          | 10           | 80           | 50.0      | 54048   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.4       | 407     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 108085  | PASS             |
| 199         | 198          | 5            | 9            | 6.5       | 7044    | PASS             |
| 275         | 198          | 10           | 60           | 24.3      | 26274   | PASS             |
| 365         | 198          | 1            | 100          | 3.5       | 3781    | PASS             |
| 441         | 198          | 0.01         | 100          | 9.2       | 9958    | PASS             |
| 442         | 198          | 50           | 100          | 56.9      | 61498   | PASS             |
| 443         | 442          | 15           | 24           | 19.9      | 12254   | PASS             |