


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070622\
 Data File : BG054211.D
 Acq On : 6 Jul 2022 8:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 27 00:27:54 2022

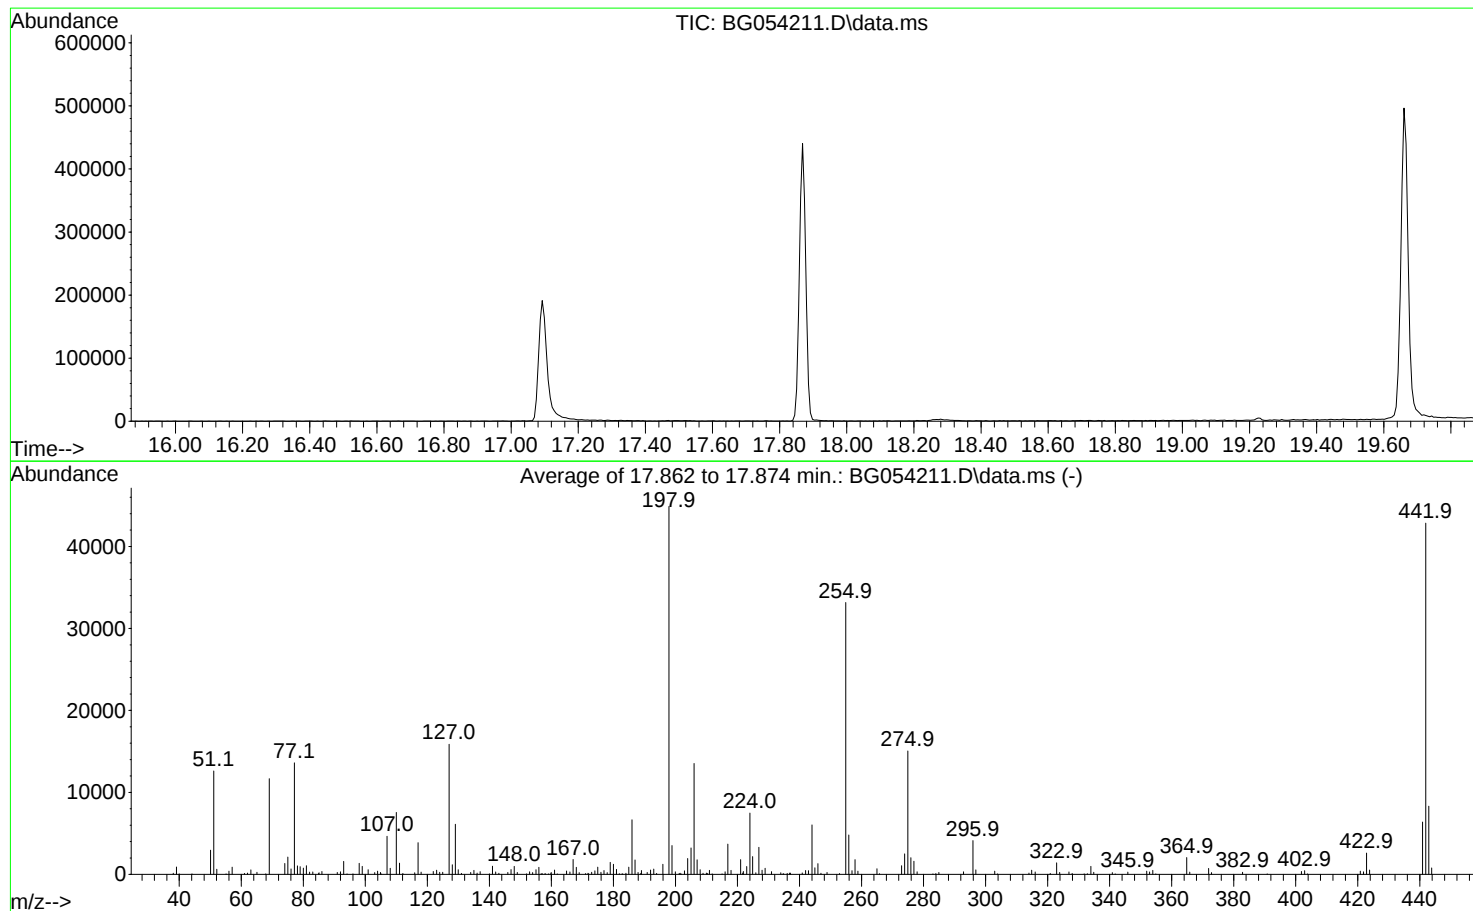




AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	12613	PASS
68	69	0.00	2	0.5	61	PASS
69	198	0.00	100	26.0	11664	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	35.4	15874	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	44875	PASS
199	198	5	9	7.8	3510	PASS
275	198	10	60	33.5	15041	PASS
365	198	1	100	4.6	2052	PASS
441	198	0.01	100	14.2	6379	PASS
442	442	50	100	100.0	42848	PASS
443	442	15	24	19.4	8321	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070622\
Data File : BG054211.D
Acq On : 6 Jul 2022 8:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 06 14:21:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

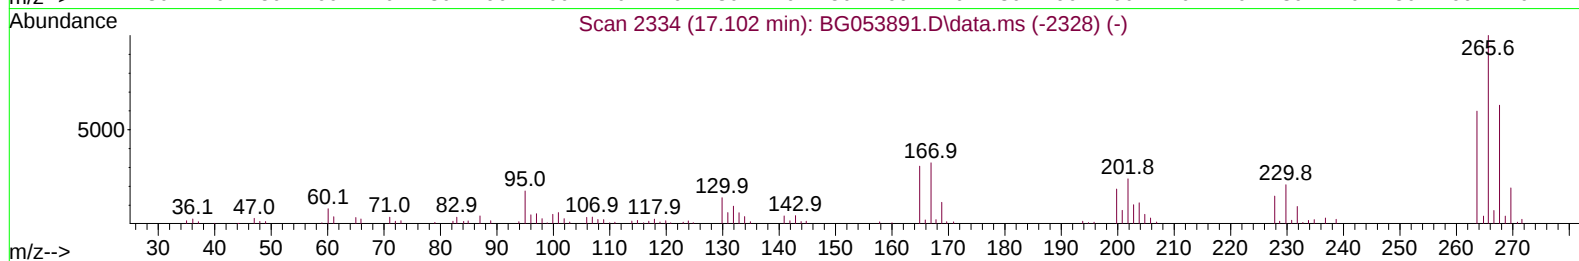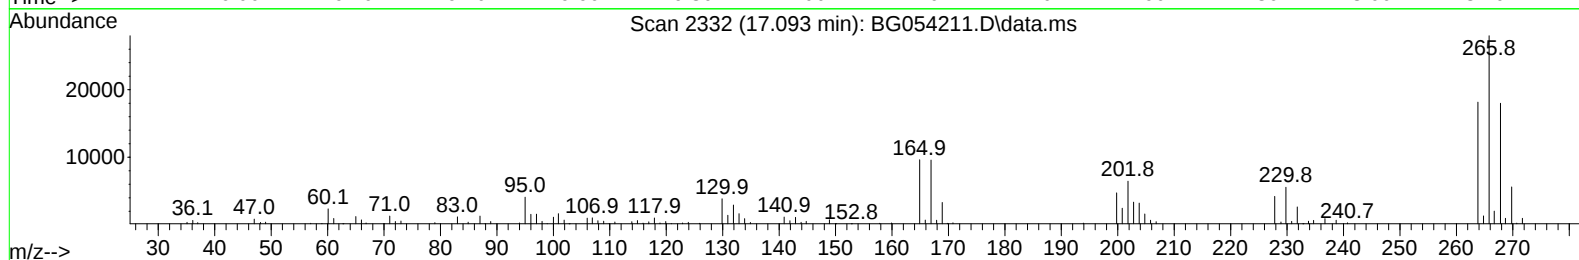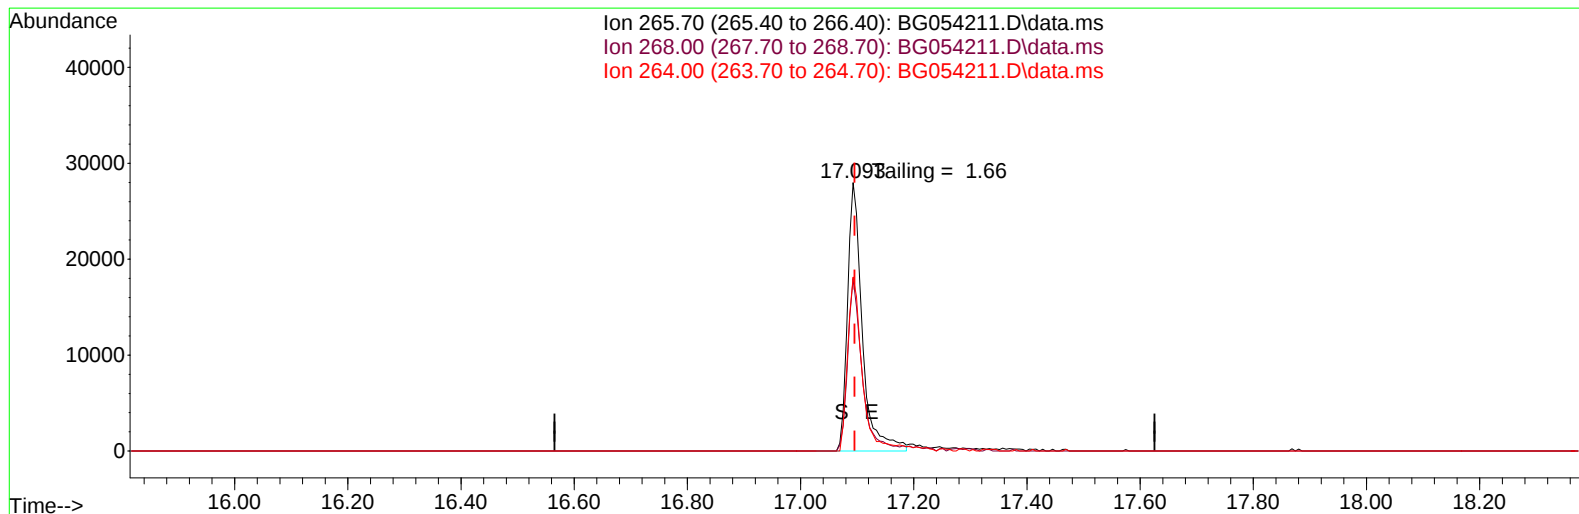

TIC: BG054211.D\data.ms

(70) Pentachlorophenol (C)

17.093min (-0.002) 32198.81 ng




response 52139

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	67.76
264.00	66.20	64.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070622\
Data File : BG054211.D
Acq On : 6 Jul 2022 8:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 06 14:21:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

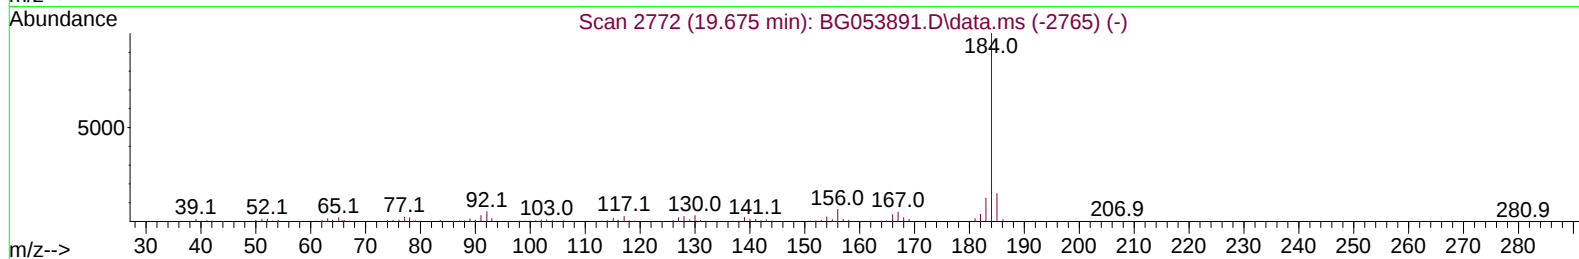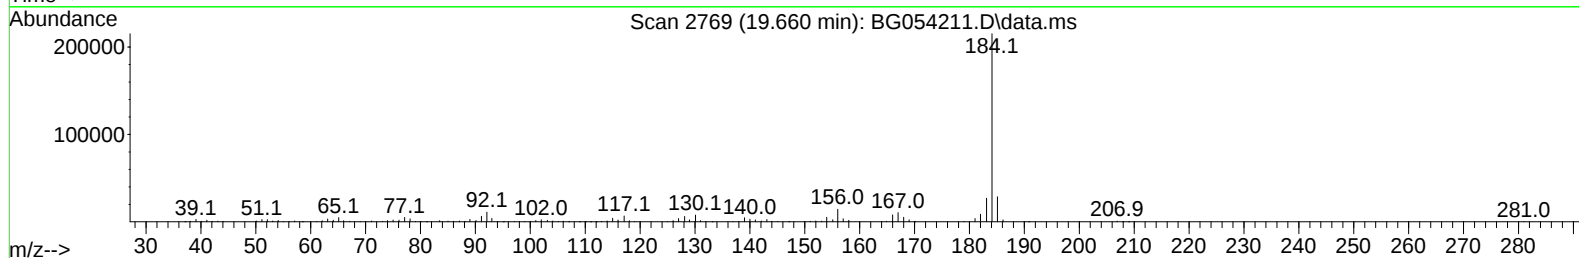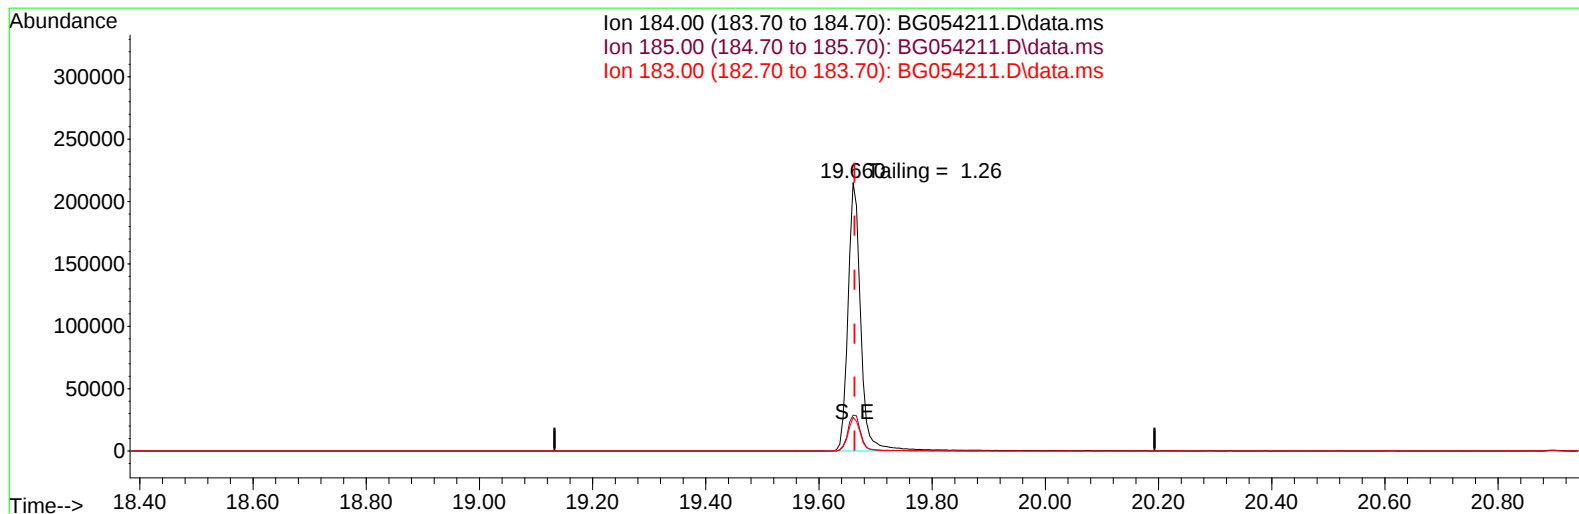

TIC: BG054211.D\data.ms

(77) Benzidine

19.660min (-0.002) 0.00 ng

response 335936

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.38
183.00	11.10	12.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/6/2022	BNA_G	BG054211.D
Compound Name	Response	Retention Time
DDT	179007	20.9
DDD	4203	20.45
DDE	1550	19.94
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5753	184760	3.11

Instrument :
BNA_G
ClientSampleId :
DFTPP