

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070716\
 Data File : BG022882.D
 Acq On : 6 Jul 2016 18:45
 Operator : UM/SJ
 Sample : H3805-01 50X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 LAR9943

Quant Time: Jul 07 02:31:22 2016
 Quant Method : Z:\HPCHEM1\BNA_G\Methods\8270-BG062516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 20:14:59 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	127387	20.00	ng	-0.01
21) Naphthalene-d8	10.98	136	538746	20.00	ng	0.00
38) Acenaphthene-d10	14.80	164	407452	20.00	ng	0.00
63) Phenanthrene-d10	17.55	188	967716	20.00	ng	0.00
75) Chrysene-d12	21.84	240	1114380	20.00	ng	0.00
86) Perylene-d12	25.21	264	1117114	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.70	112	24820	3.13	ng	0.00
7) Phenol-d6	7.31	99	34031	3.04	ng	0.00
23) Nitrobenzene-d5	9.32	82	105271	8.27	ng	-0.01
41) 2,4,6-Tribromophenol	16.28	330	17660	2.76	ng	0.00
44) 2-Fluorobiphenyl	13.42	172	61013	2.37	ng	0.00
78) Terphenyl-d14	20.14	244	106248	2.53	ng	-0.01
Target Compounds						Qvalue
18) Hexachloroethane	9.27	117	9977	2.40	ng	# 1
19) n-Nitroso-di-n-propylamine	8.92	70	95624	10.26	ng	# 44
22) Acetophenone	8.96	105	37514	2.41	ng	# 33
25) Isophorone	9.90	82	214406	8.68	ng	# 1
26) 2-Nitrophenol	10.09	139	21679	4.28	ng	# 24
32) Benzoic acid	10.20	122	13645	7.04	ng	# 42
35) Caprolactam	11.87	113	9554	3.22	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070716\
Data File : BG022882.D
Acq On : 6 Jul 2016 18:45
Operator : UM/SJ
Sample : H3805-01 50X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
LAR9943

Quant Time: Jul 07 02:31:22 2016
Quant Method : Z:\HPCHEM1\BNA_G\Methods\8270-BG062516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 20:14:59 2016
Response via : Initial Calibration

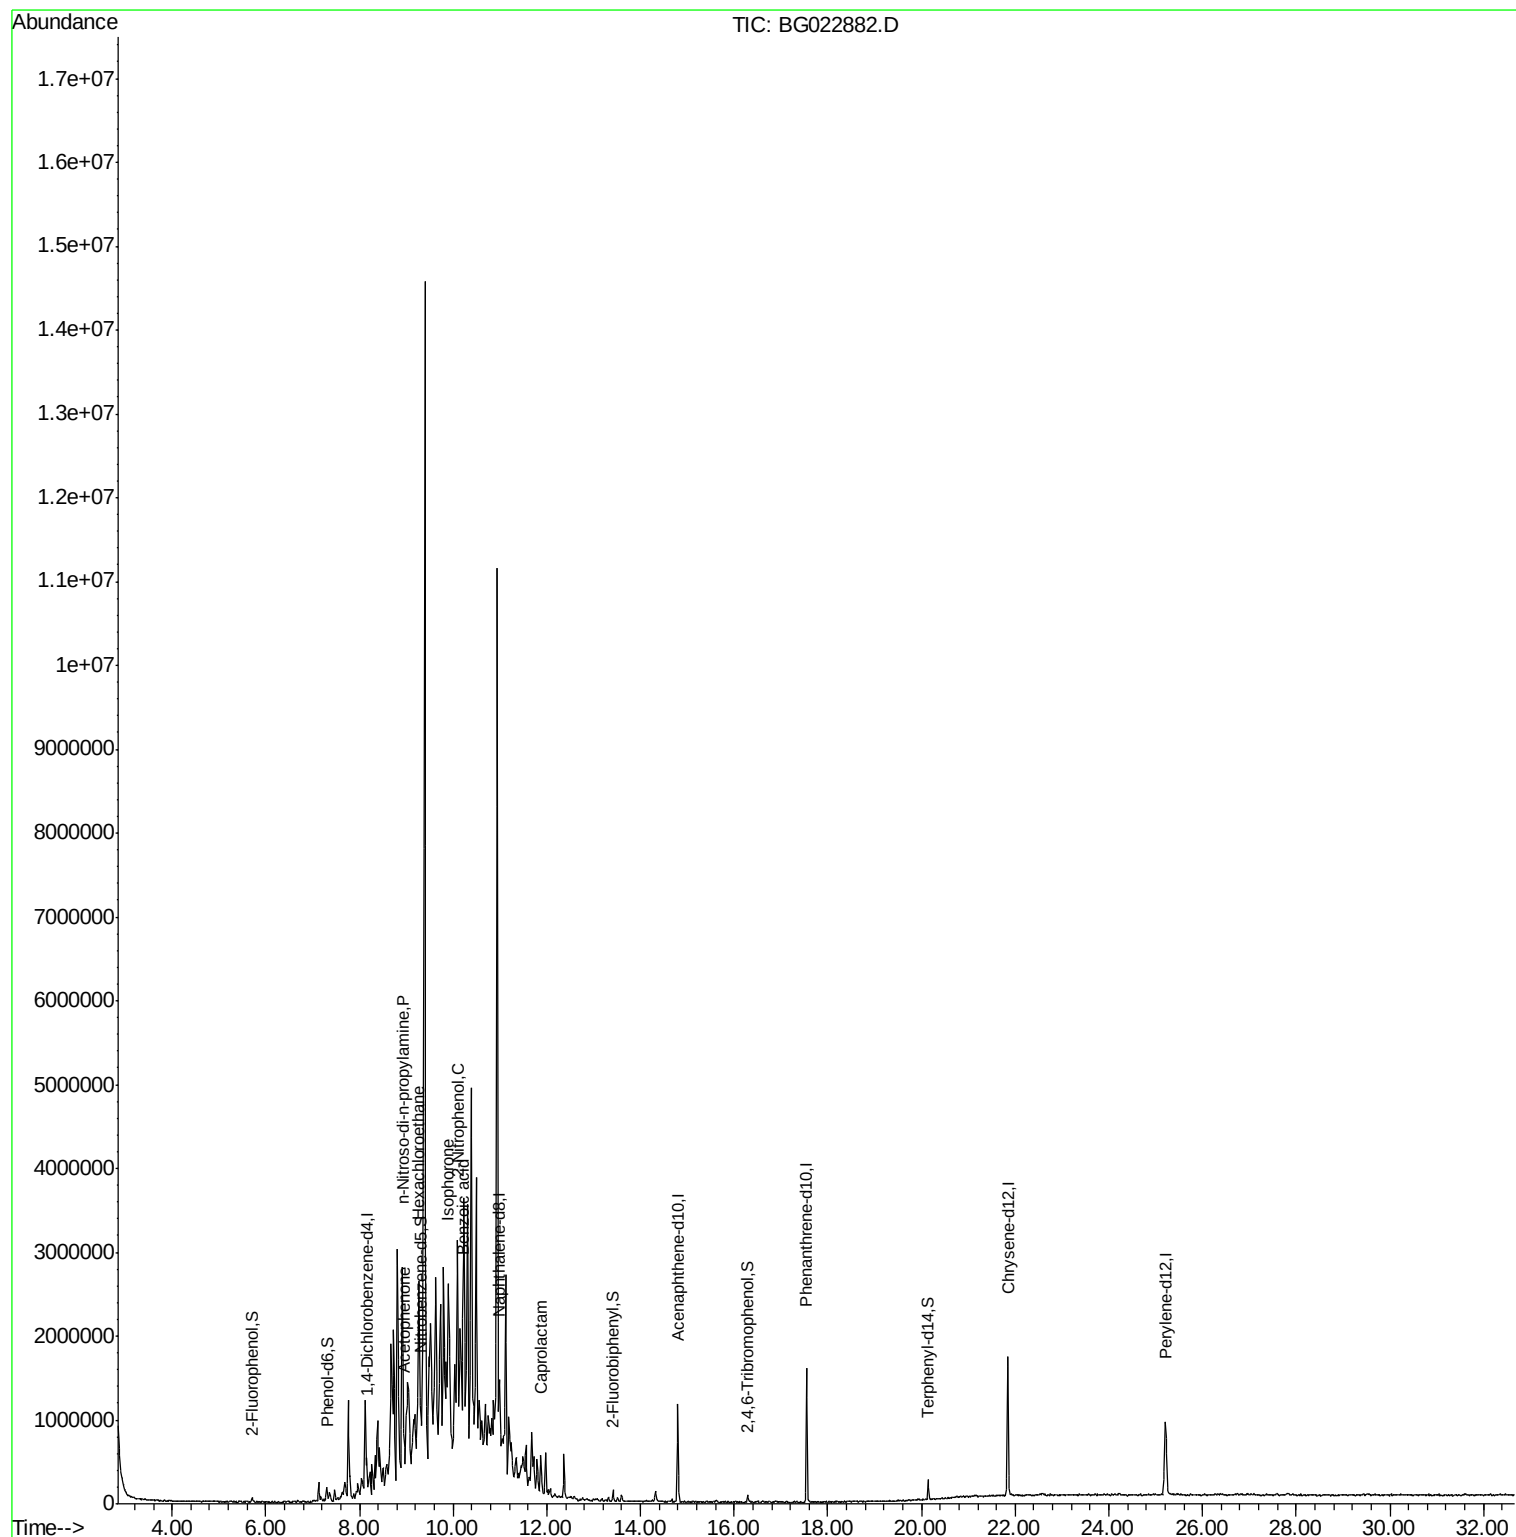

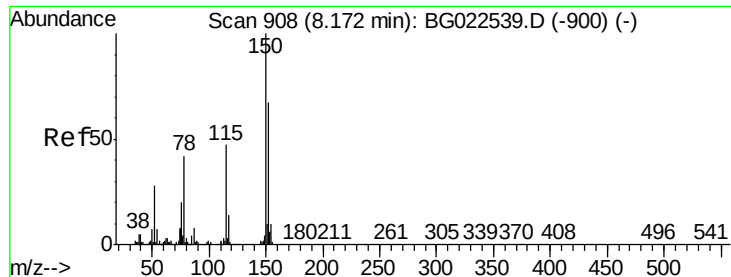

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.16 min Scan# 905

Delta R.T. -0.01 min

Lab File: BG022882.D

Acq: 6 Jul 2016 18:45

Instrument :

BNA_G

ClientSampleId :

LAR9943


Tgt Ion:152 Resp: 127387

Ion Ratio Lower Upper

152 100

150 144.3 144.7 217.1#




115 66.1 64.0 96.0

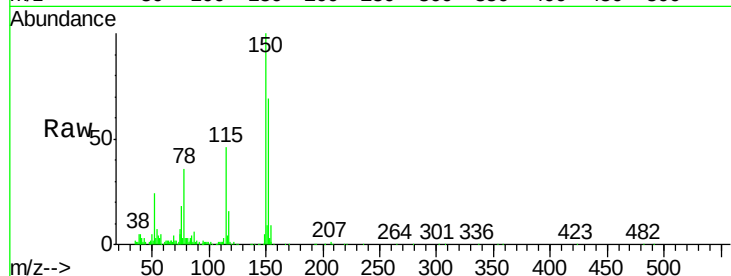

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

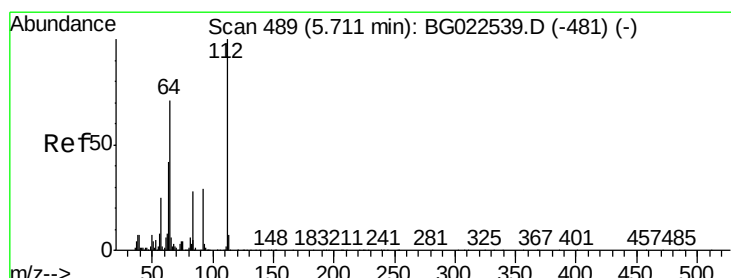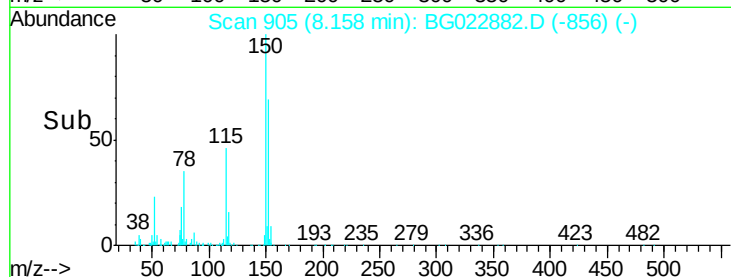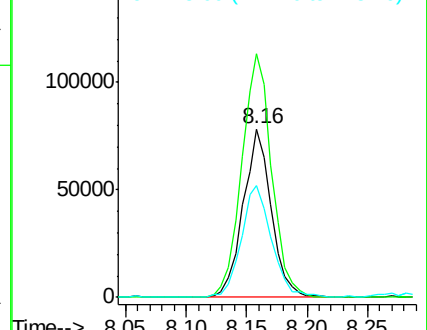

#5

2-Fluorophenol

Concen: 3.13 ng

RT: 5.70 min Scan# 487

Delta R.T. -0.00 min

Lab File: BG022882.D

Acq: 6 Jul 2016 18:45


Tgt Ion:112 Resp: 24820

Ion Ratio Lower Upper

112 100

64 62.4 59.0 88.4



63 32.2 37.8 56.8#

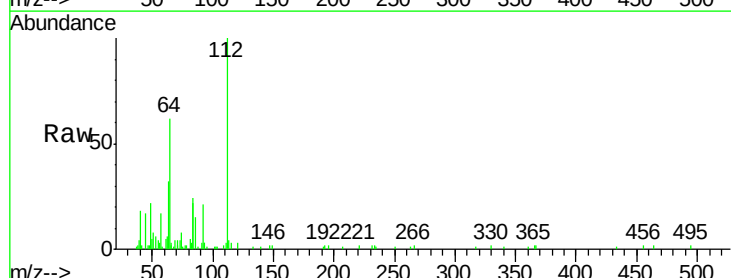


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG0

Ion 63.00 (62.70 to 63.70): BG0

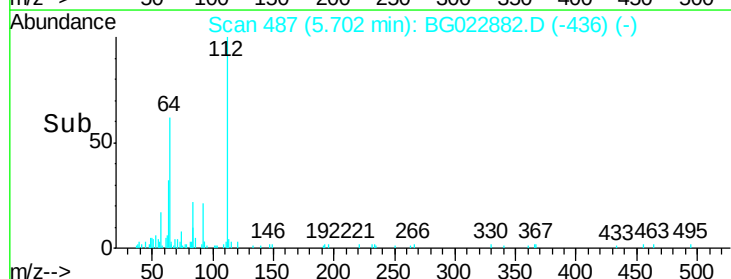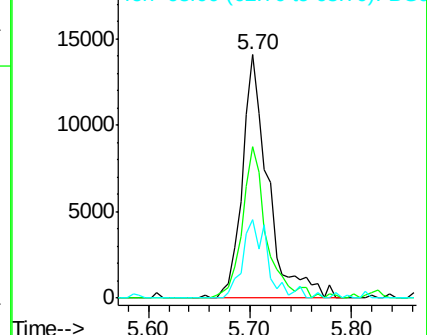

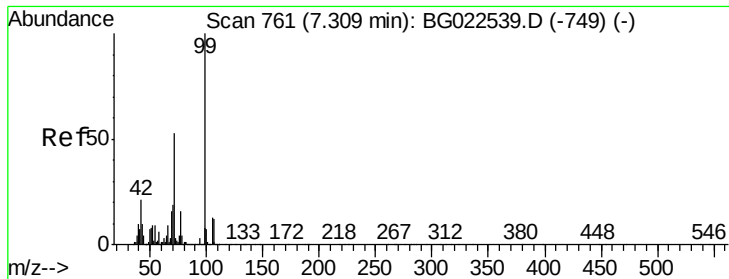

#7

Phenol-d6

Concen: 3.04 ng

RT: 7.31 min Scan# 761

Delta R.T. 0.01 min

Lab File: BG022882.D

Acq: 6 Jul 2016 18:45

Instrument :

BNA_G

ClientSampleId :

LAR9943


Tgt Ion: 99 Resp: 34031

Ion Ratio Lower Upper




99 100

42 16.8 17.8 26.6#

71 81.3 41.5 62.3#

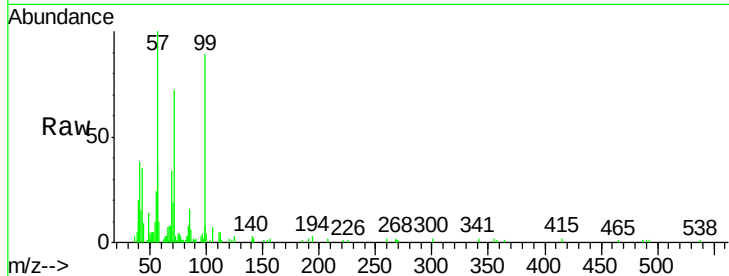

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

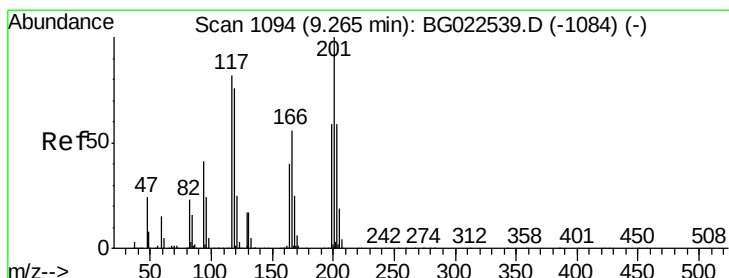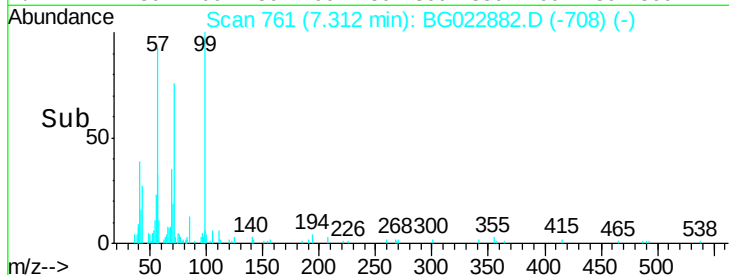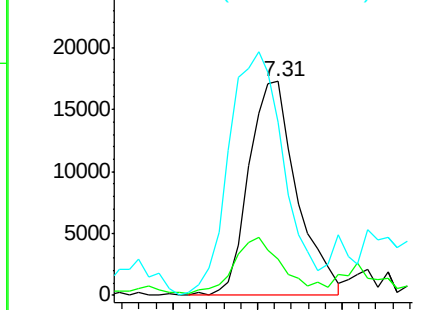

#18

Hexachloroethane

Concen: 2.40 ng

RT: 9.27 min Scan# 1095

Delta R.T. 0.01 min

Lab File: BG022882.D

Acq: 6 Jul 2016 18:45


Tgt Ion: 117 Resp: 9977

Ion Ratio Lower Upper



117 100


119 403.8 73.7 110.5#

201 0.0 88.7 133.1#

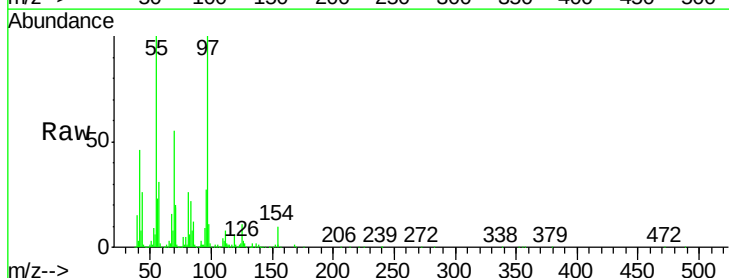

Abundance Ion 117.00 (116.70 to 117.70): E
Ion 119.00 (118.70 to 119.70): E
Ion 201.00 (200.70 to 201.70): E



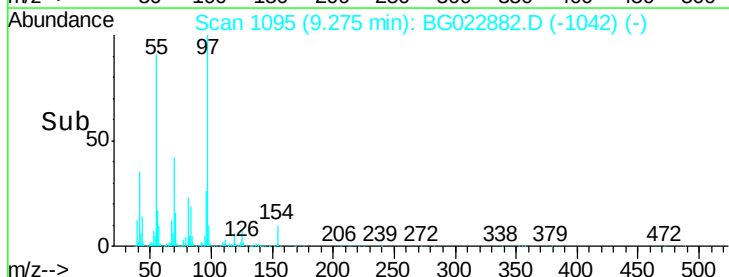
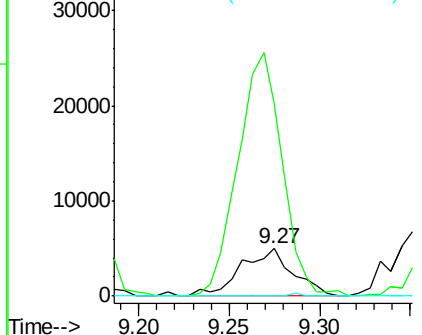


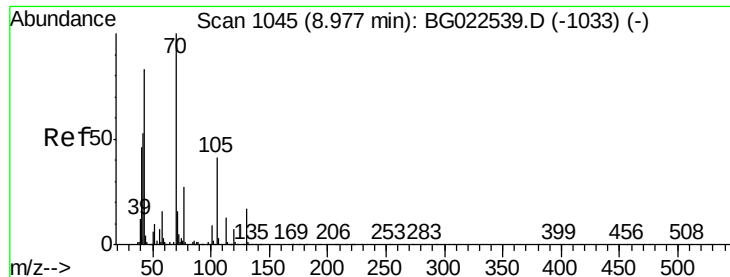

#19
n-Nitroso-di-n-propylamine
Concen: 10.26 ng
RT: 8.92 min Scan# 1034
Delta R.T. -0.06 min
Lab File: BG022882.D
Acq: 6 Jul 2016 18:45




Instrument :
BNA_G
ClientSampleId :
LAR9943


Tgt Ion:	70	Resp:	95624
Ion	Ratio	Lower	Upper
70	100		
42	99.6	42.1	63.1#
101	0.0	7.2	10.8#
130	0.0	14.2	21.2#

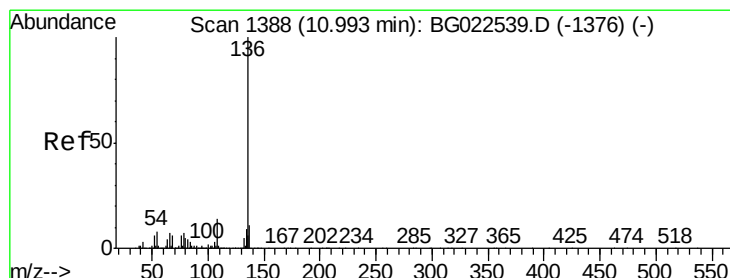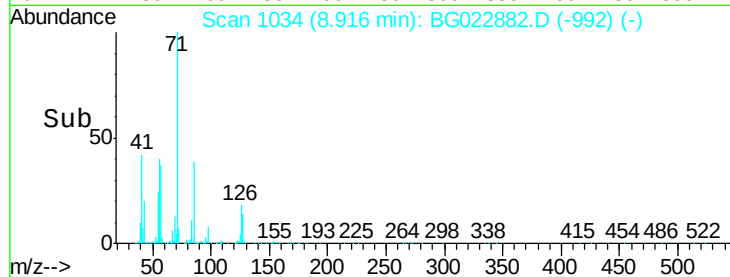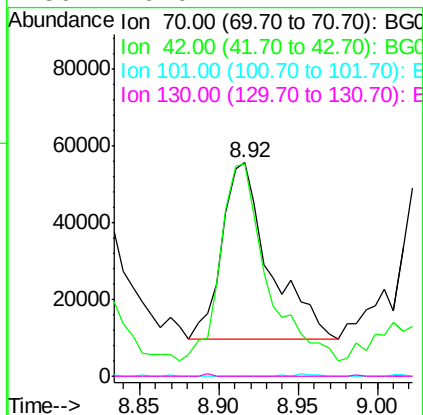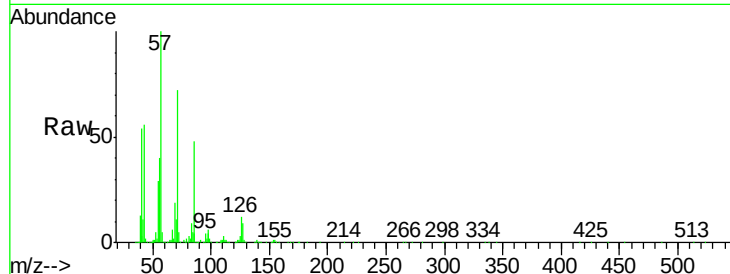

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.98 min Scan# 1386
Delta R.T. -0.01 min
Lab File: BG022882.D
Acq: 6 Jul 2016 18:45

Tgt Ion:	136	Resp:	538746
Ion	Ratio	Lower	Upper
136	100		
137	12.4	9.6	14.4
54	9.1	7.3	10.9
68	10.8	5.3	7.9#

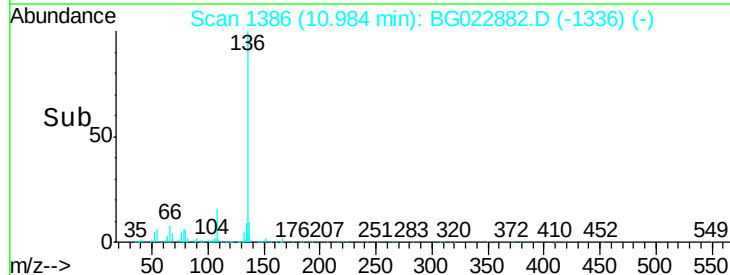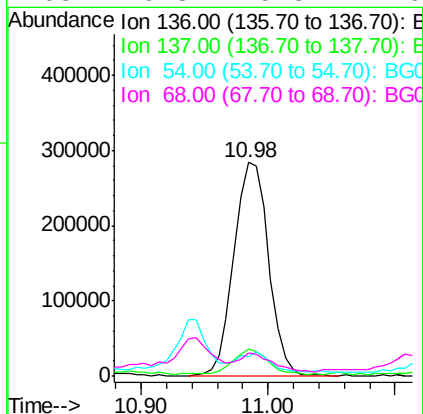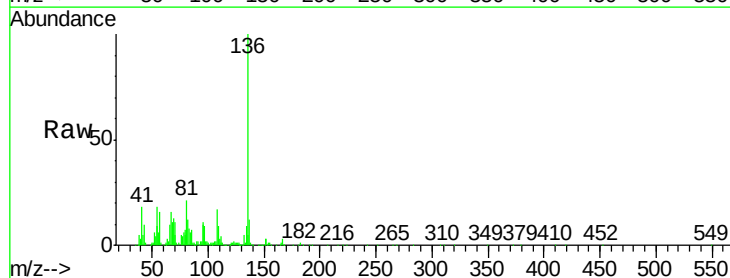

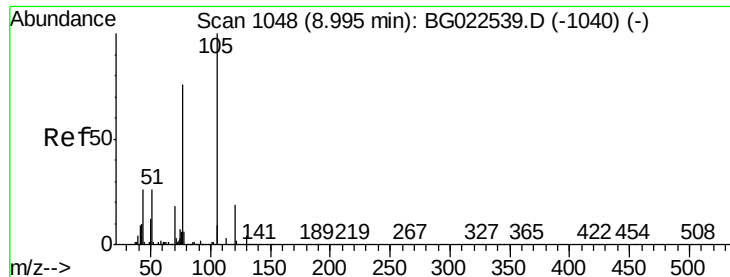

#22

Acetophenone

Concen: 2.41 ng

RT: 8.96 min Scan# 1041

Delta R.T. -0.03 min

Lab File: BG022882.D

Acq: 6 Jul 2016 18:45

Instrument :

BNA_G

ClientSampleId :

LAR9943

Tgt Ion:105 Resp: 37514


Ion Ratio Lower Upper

105 100

71 208.1 2.6 3.8#

51 17.2 27.1 40.7#

120 0.0 15.1 22.7#



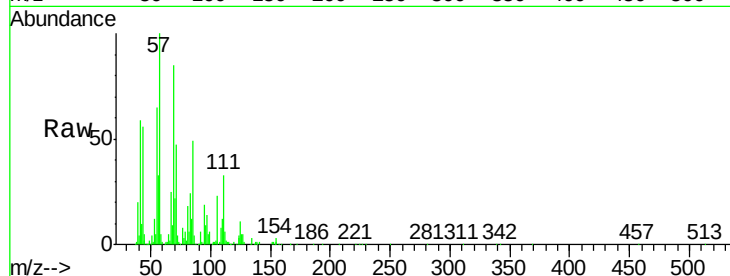


Abundance Ion 105.00 (104.70 to 105.70): E

Ion 71.00 (70.70 to 71.70): BGC

Ion 51.00 (50.70 to 51.70): BGC

Ion 120.00 (119.70 to 120.70): E

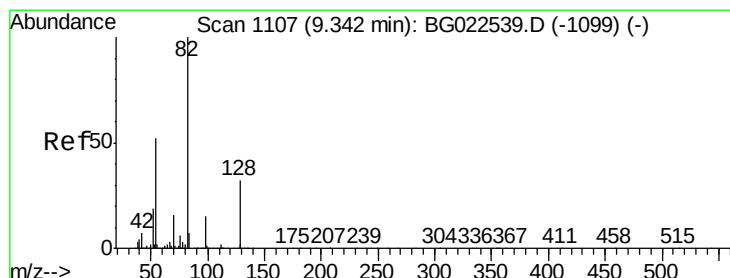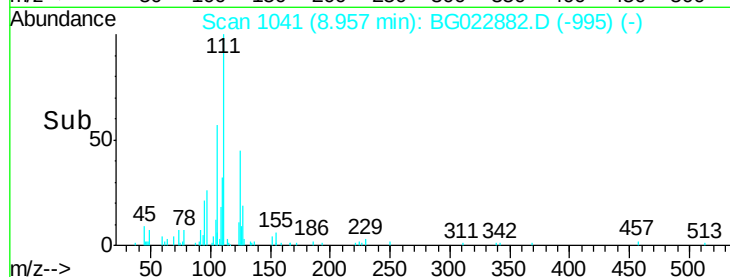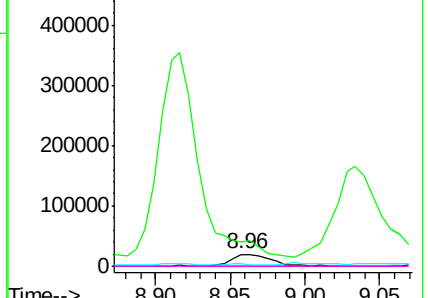

#23

Nitrobenzene-d5

Concen: 8.27 ng

RT: 9.32 min Scan# 1103

Delta R.T. -0.01 min

Lab File: BG022882.D

Acq: 6 Jul 2016 18:45


Tgt Ion: 82 Resp: 105271

Ion Ratio Lower Upper

82 100

128 7.7 24.4 36.6#



54 41.7 41.4 62.0

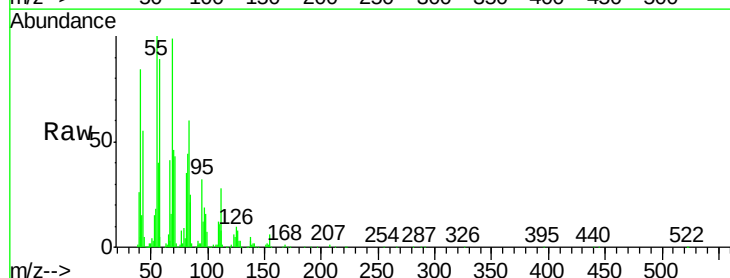


Abundance Ion 82.00 (81.70 to 82.70): BGC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BGC

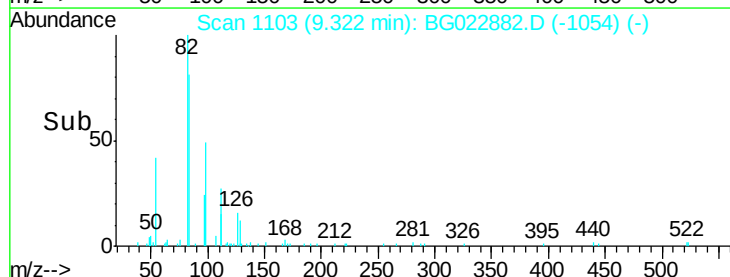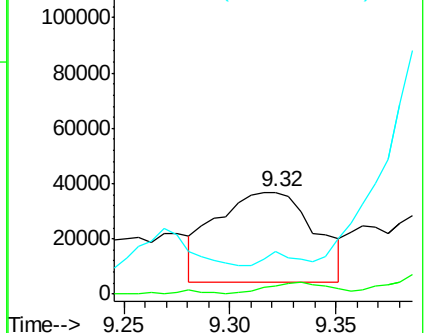

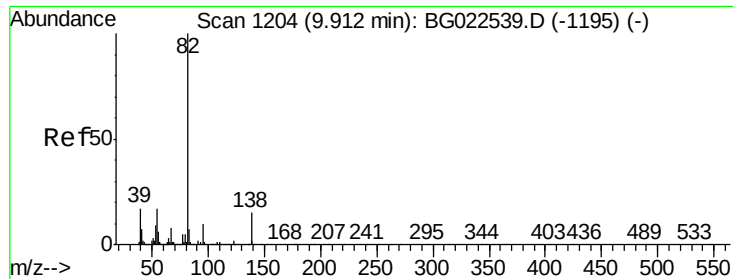

#25

Isophorone

Concen: 8.68 ng

RT: 9.90 min Scan# 1201

Delta R.T. -0.01 min

Lab File: BG022882.D

Acq: 6 Jul 2016 18:45

Instrument :

BNA_G

ClientSampleId :

LAR9943





Tgt Ion: 82 Resp: 214406

Ion Ratio Lower Upper

82 100

95 154.9 8.2 12.2#

138 6.8 10.7 16.1#

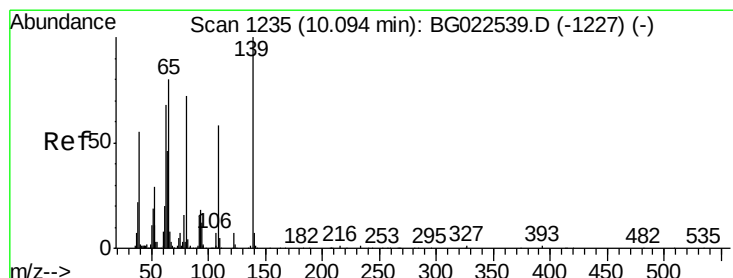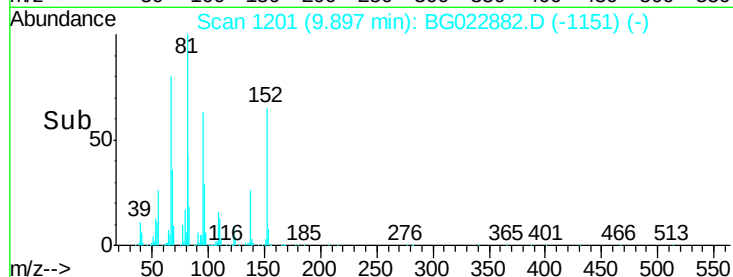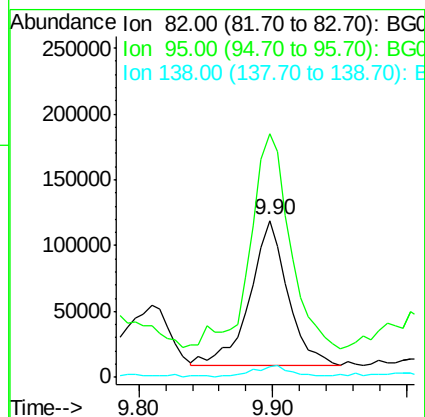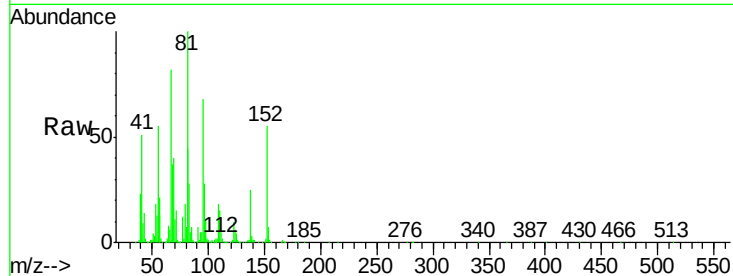

#26

2-Nitrophenol

Concen: 4.28 ng

RT: 10.09 min Scan# 1233

Delta R.T. -0.00 min

Lab File: BG022882.D

Acq: 6 Jul 2016 18:45




Tgt Ion: 139 Resp: 21679


Ion Ratio Lower Upper

139 100

109 162.0 43.5 65.3#

65 103.7 64.3 96.5#

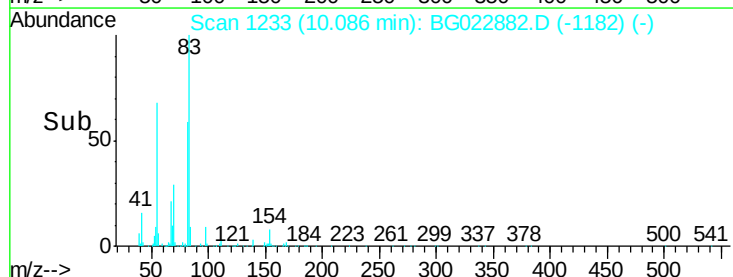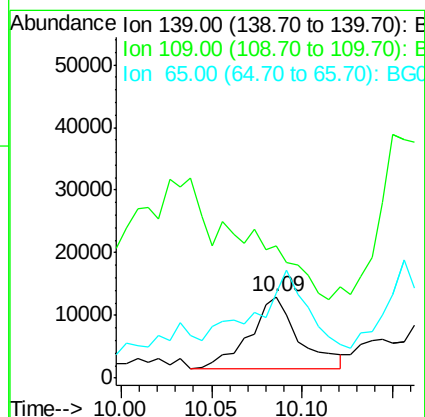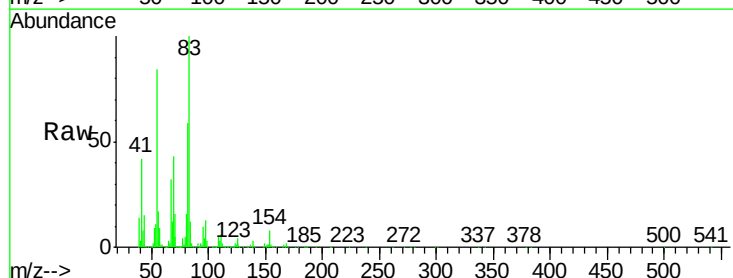

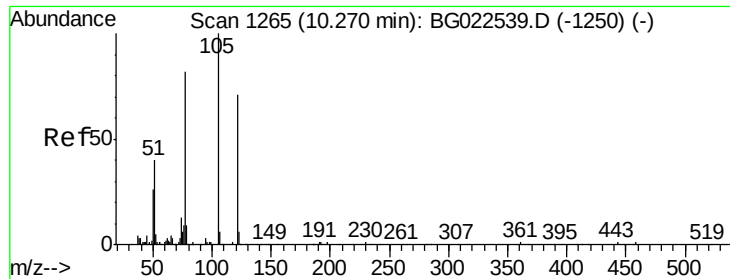

#32

Benzoic acid

Concen: 7.04 ng

RT: 10.20 min Scan# 1252

Delta R.T. -0.00 min

Lab File: BG022882.D

Acq: 6 Jul 2016 18:45

Instrument :

BNA_G

ClientSampleId :

LAR9943


Tgt Ion:122 Resp: 13645

Ion Ratio Lower Upper

122 100

105 20.7 117.2 157.2#




77 149.0 109.2 149.2

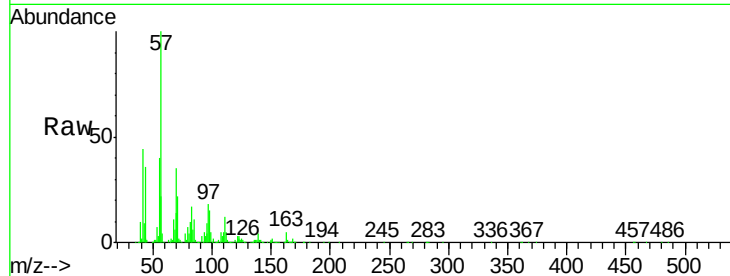

Abundance Ion 122.00 (121.70 to 122.70): E

Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BGC

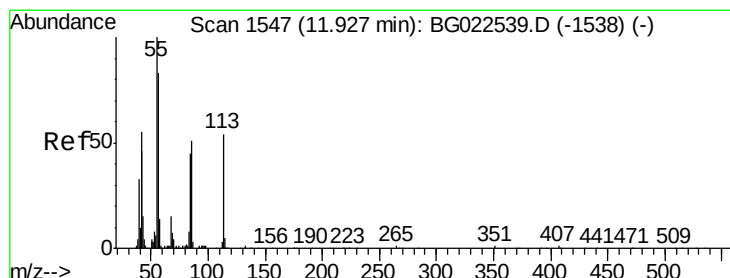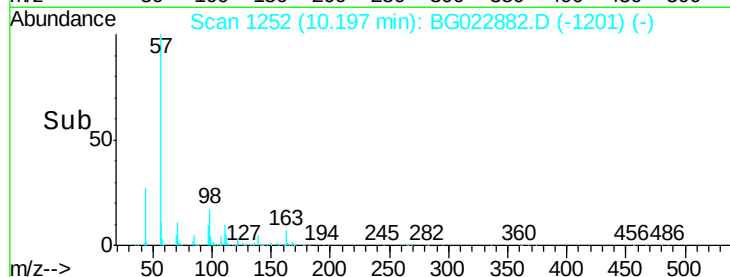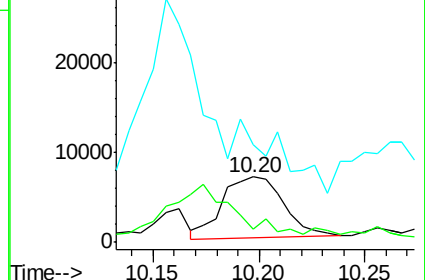

#35

Caprolactam

Concen: 3.22 ng

RT: 11.87 min Scan# 1537

Delta R.T. -0.03 min

Lab File: BG022882.D

Acq: 6 Jul 2016 18:45


Tgt Ion:113 Resp: 9554

Ion Ratio Lower Upper

113 100

55 699.3 154.5 194.5#



56 422.7 125.1 165.1#

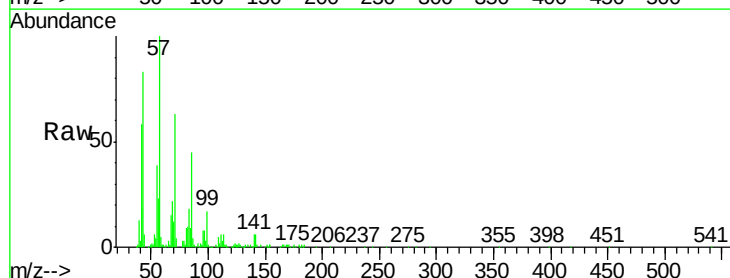


Abundance Ion 113.00 (112.70 to 113.70): E

Ion 55.00 (54.70 to 55.70): BGC

Ion 56.00 (55.70 to 56.70): BGC

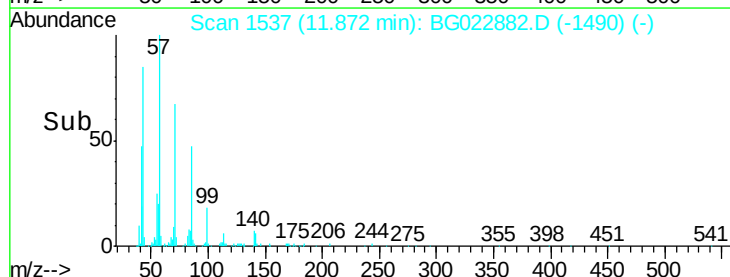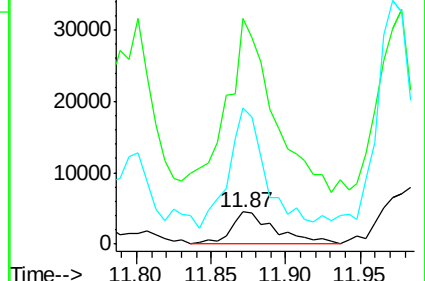

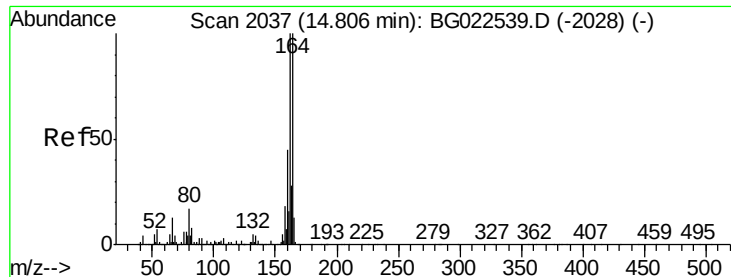

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 14.80 min Scan# 2035

Delta R.T. -0.00 min

Lab File: BG022882.D

Acq: 6 Jul 2016 18:45

Instrument :

BNA_G

ClientSampleId :

LAR9943


Tgt Ion:164 Resp: 407452

Ion Ratio Lower Upper

164 100

162 101.0 87.7 131.5




160 44.4 37.2 55.8

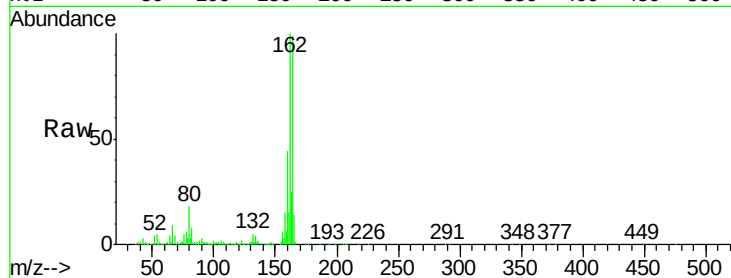

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

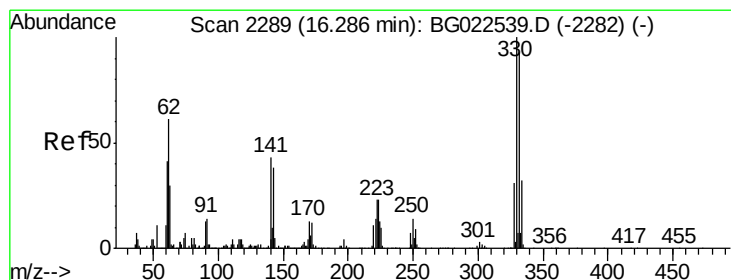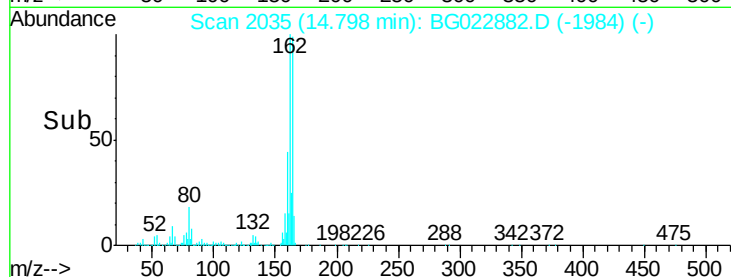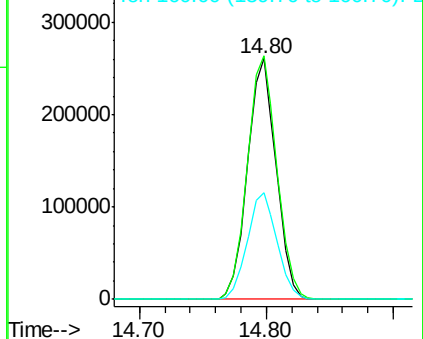

#41

2,4,6-Tribromophenol

Concen: 2.76 ng

RT: 16.28 min Scan# 2288

Delta R.T. -0.00 min

Lab File: BG022882.D

Acq: 6 Jul 2016 18:45


Tgt Ion:330 Resp: 17660

Ion Ratio Lower Upper

330 100

332 86.8 77.4 116.2



141 32.1 31.7 47.5

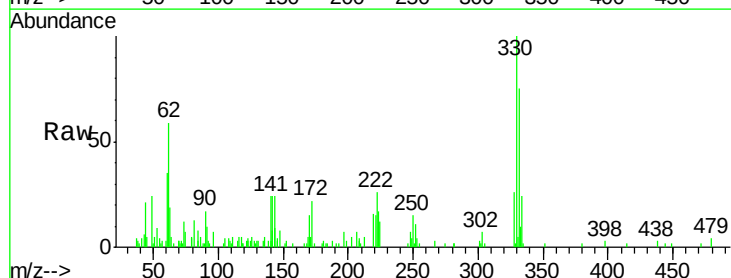


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



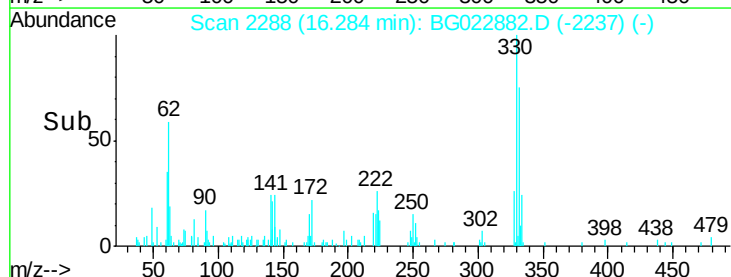
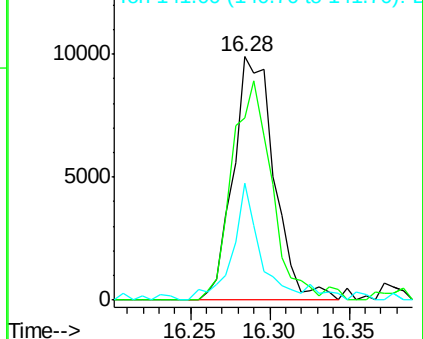


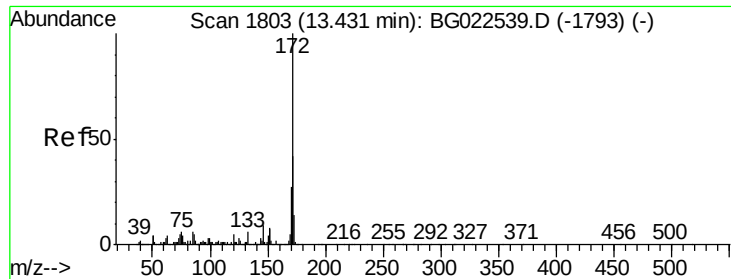

#44
2-Fluorobiphenyl
Concen: 2.37 ng
RT: 13.42 min Scan# 1800
Delta R.T. -0.01 min
Lab File: BG022882.D
Acq: 6 Jul 2016 18:45




Instrument :
BNA_G
ClientSampleId :
LAR9943


Tgt Ion:172 Resp: 61013
Ion Ratio Lower Upper
172 100
171 36.3 31.6 47.4
170 28.8 21.3 31.9

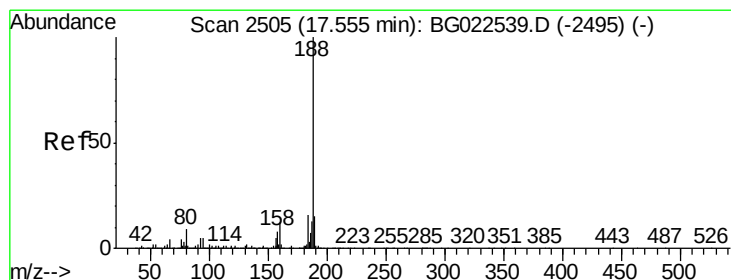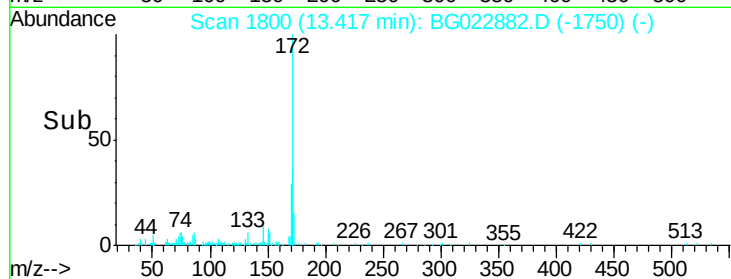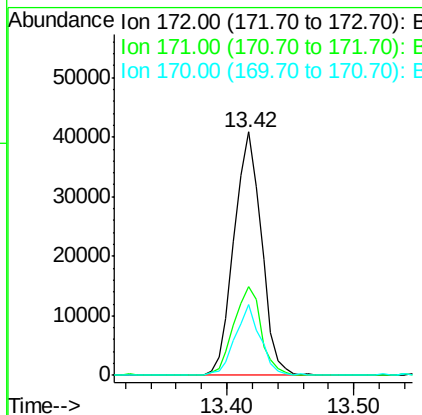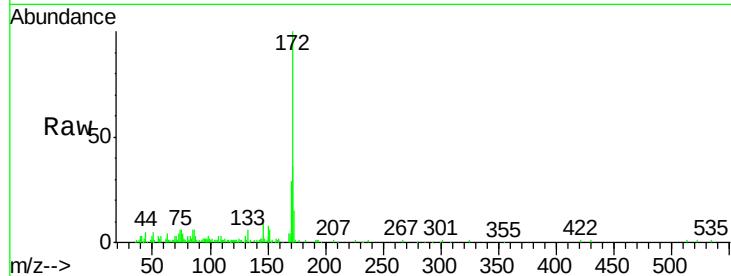

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.55 min Scan# 2503
Delta R.T. -0.00 min
Lab File: BG022882.D
Acq: 6 Jul 2016 18:45

Tgt Ion:188 Resp: 967716
Ion Ratio Lower Upper
188 100
94 7.0 5.2 7.8
80 8.5 7.2 10.8

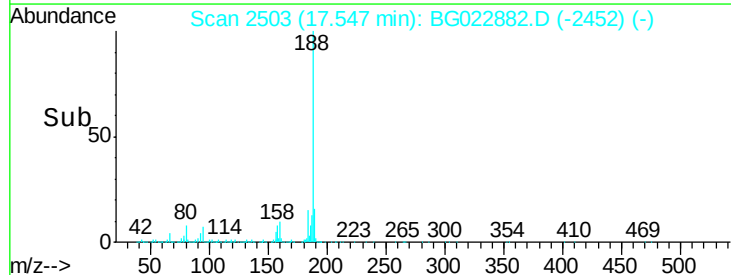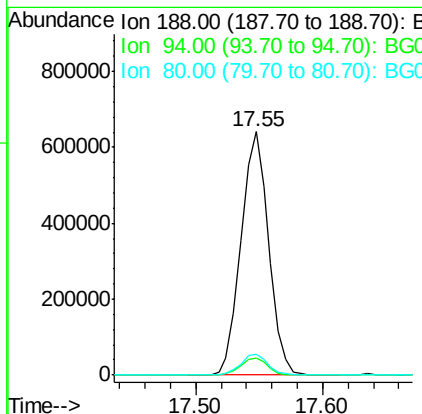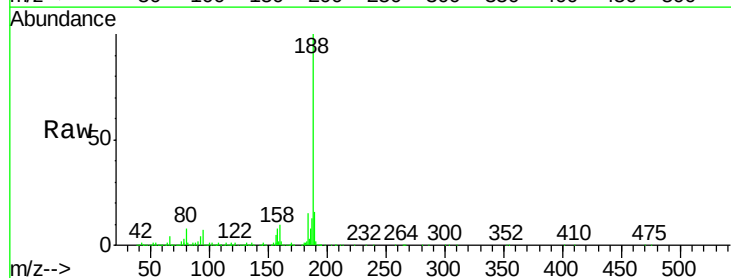

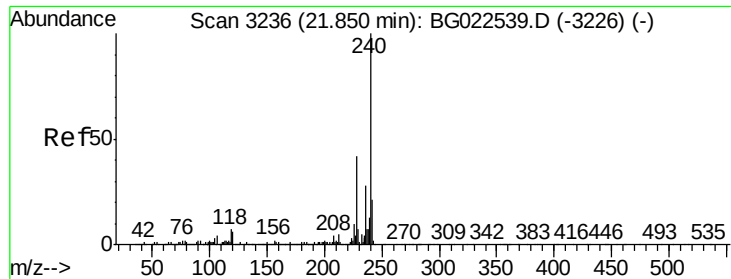

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.84 min Scan# 3234

Delta R.T. -0.00 min

Lab File: BG022882.D

Acq: 6 Jul 2016 18:45

Instrument :

BNA_G

ClientSampleId :

LAR9943


Tgt Ion:240 Resp: 1114380

Ion Ratio Lower Upper

240 100

120 5.4 4.1 6.1




236 29.2 21.1 31.7

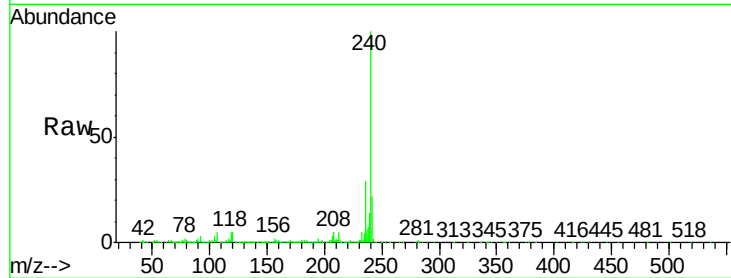

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

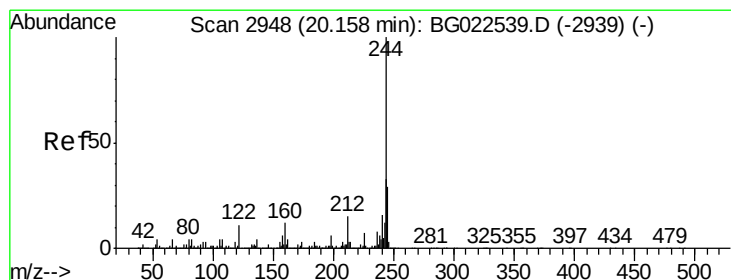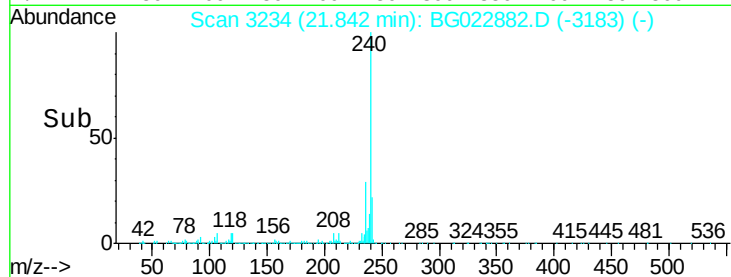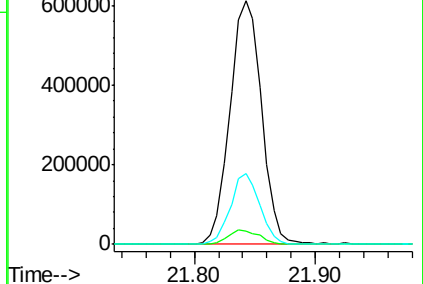

#78

Terphenyl-d14

Concen: 2.53 ng

RT: 20.14 min Scan# 2944

Delta R.T. -0.01 min

Lab File: BG022882.D

Acq: 6 Jul 2016 18:45


Tgt Ion:244 Resp: 106248

Ion Ratio Lower Upper

244 100

212 6.9 10.8 16.2#



122 5.6 8.0 12.0#

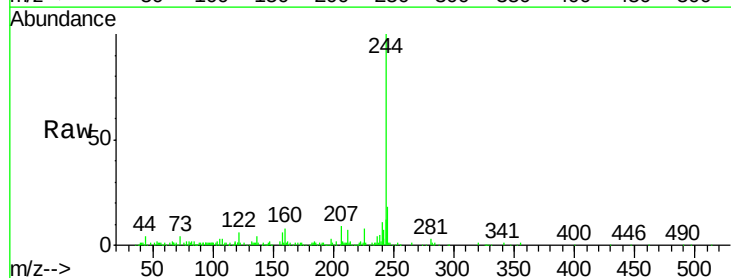


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

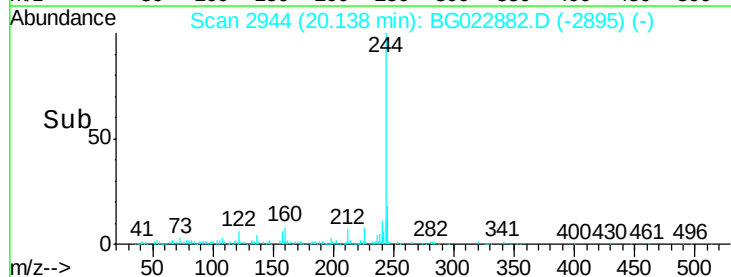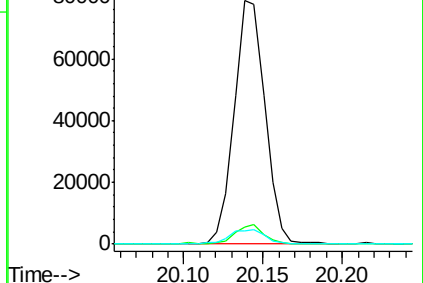

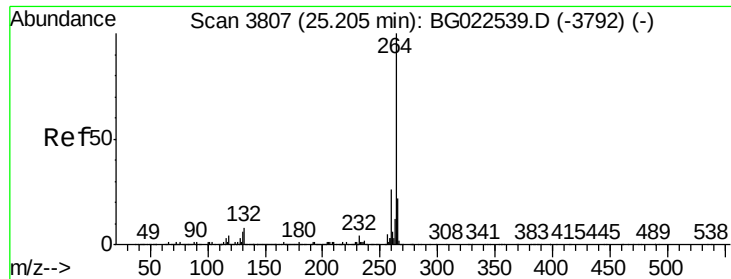

#86
Perylene-d12
Concen: 20.00 ng
RT: 25.21 min Scan# 3807
Delta R.T. 0.00 min
Lab File: BG022882.D
Acq: 6 Jul 2016 18:45

Instrument :
BNA_G
ClientSampleId :
LAR9943

Tgt Ion: 264 Resp: 1117114

Ion	Ratio	Lower	Upper
264	100		
260	26.5	18.4	27.6
265	22.5	18.9	28.3

