


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070716\
Data File : BG022872.D
Acq On : 6 Jul 2016 11:02
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\Methods\8270-BG062516.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 24 20:14:59 2016

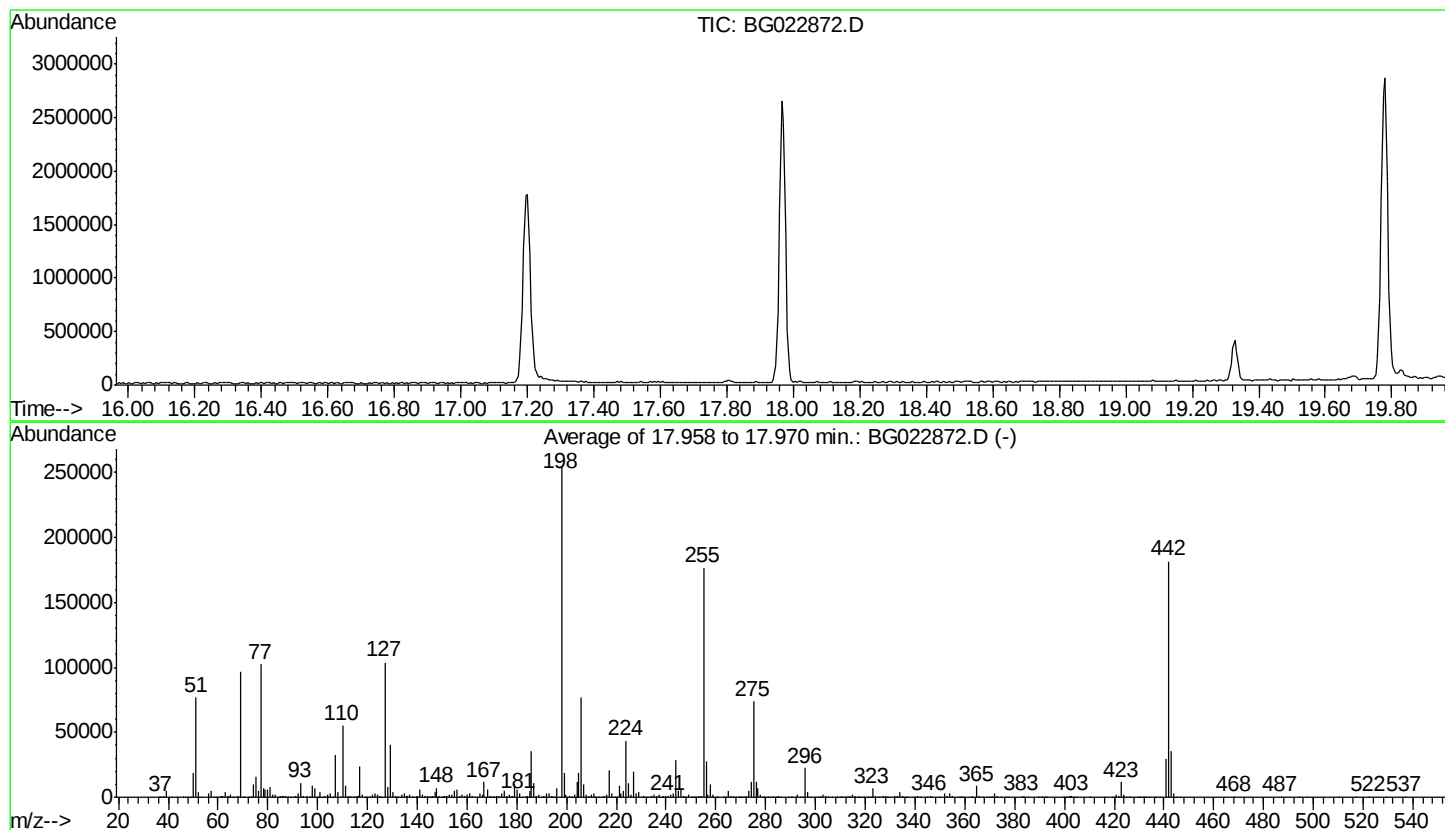

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2566

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.1	76772	PASS
68	69	0.00	2	0.9	918	PASS
69	198	0.00	100	38.0	97019	PASS
70	69	0.00	2	0.1	120	PASS
127	198	10	80	40.6	103810	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	255445	PASS
199	198	5	9	7.2	18503	PASS
275	198	10	60	28.9	73834	PASS
365	198	1	100	3.4	8786	PASS
441	442	0.01	24	16.4	29727	PASS
442	198	50	100	71.1	181568	PASS
443	442	15	24	19.8	35946	PASS