

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070717\
 Data File : BG027883.D
 Acq On : 8 Jul 2017 00:37
 Operator : SJ/JU
 Sample : I4072-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jul 08 02:14:14 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 07 17:43:21 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	33603	20.00	ng	0.00
21) Naphthalene-d8	11.25	136	145595	20.00	ng	0.00
38) Acenaphthene-d10	15.03	164	79305	20.00	ng	0.00
63) Phenanthrene-d10	17.77	188	211187	20.00	ng	0.00
75) Chrysene-d12	22.12	240	252198	20.00	ng	0.00
86) Perylene-d12	25.69	264	236890	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	6.01	112	278860	127.79	ng	0.00
7) Phenol-d6	7.58	99	347812	104.33	ng	0.00
23) Nitrobenzene-d5	9.59	82	214097	81.97	ng	0.00
41) 2,4,6-Tribromophenol	16.51	330	209892	192.96	ng	0.00
44) 2-Fluorobiphenyl	13.65	172	549161	98.90	ng	0.00
78) Terphenyl-d14	20.35	244	1208617	112.35	ng	0.00
Target Compounds						
76) Benzidine	20.01	184	64	3.23	ng	Qvalue # 64

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070717\
Data File : BG027883.D
Acq On : 8 Jul 2017 00:37
Operator : SJ/JU
Sample : I4072-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jul 08 02:14:14 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 17:43:21 2017
Response via : Initial Calibration

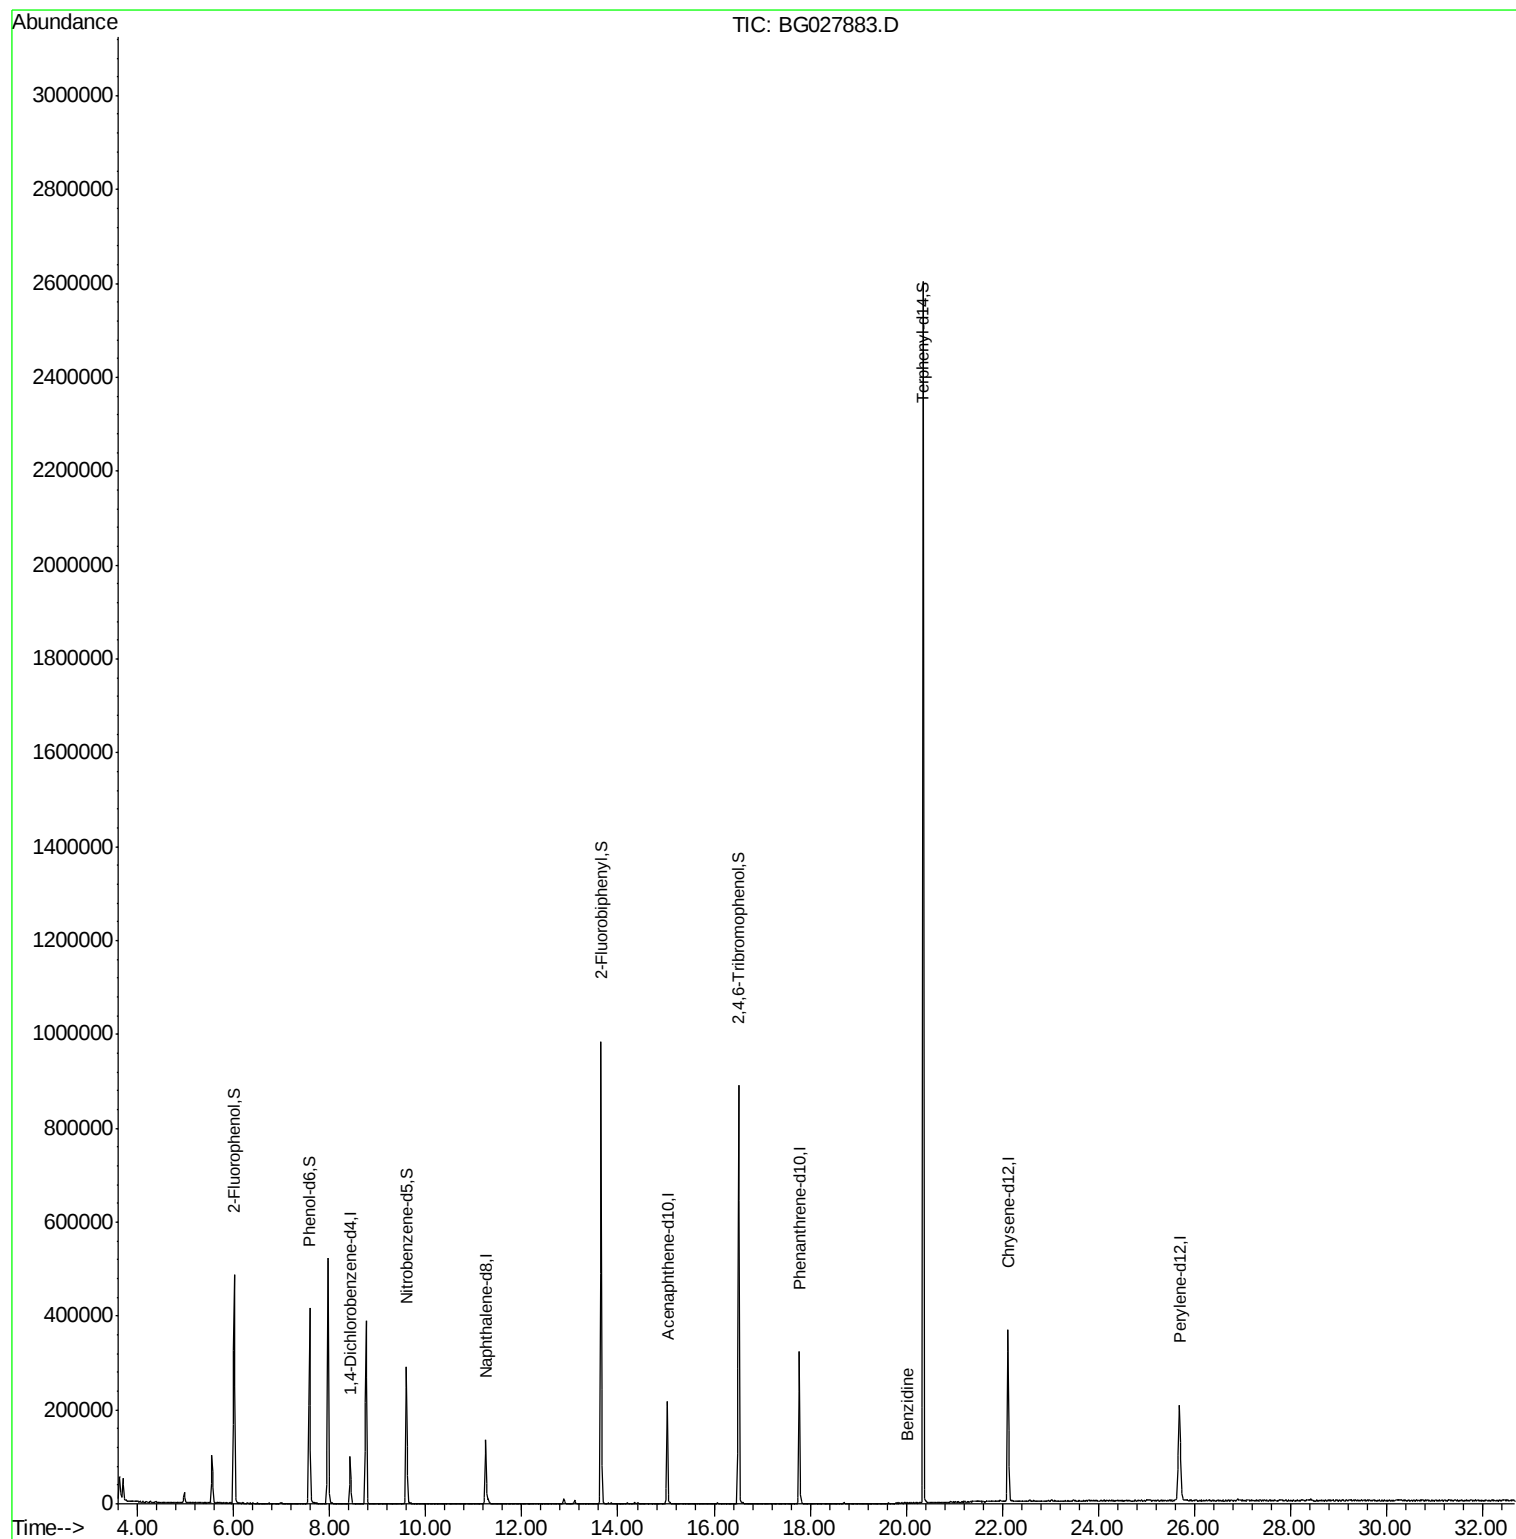




#1



1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.43 min Scan# 824
Delta R.T. 0.00 min
Lab File: BG027883.D
Acq: 8 Jul 2017 00:37

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 33603
Ion Ratio Lower Upper
152 100
150 148.2 114.0 171.0
115 55.0 48.1 72.1

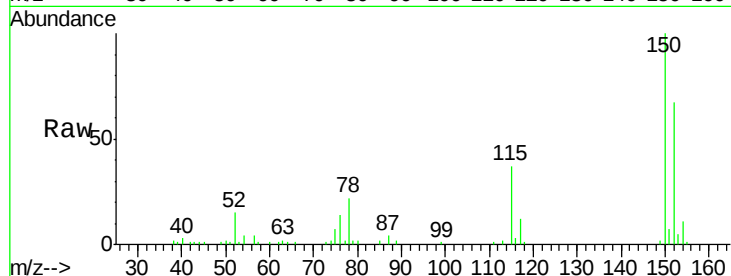


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

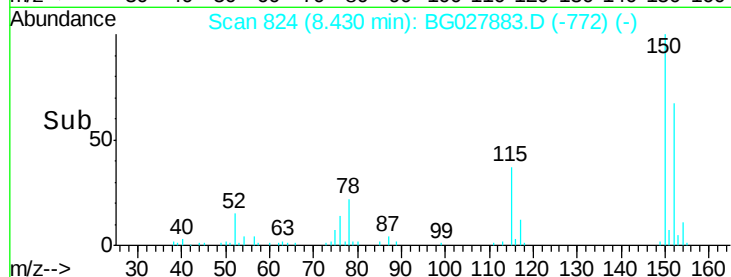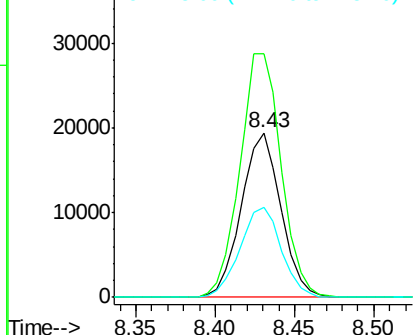



#5


2-Fluorophenol
Concen: 127.79 ng
RT: 6.01 min Scan# 412
Delta R.T. 0.00 min
Lab File: BG027883.D
Acq: 8 Jul 2017 00:37

Tgt Ion:112 Resp: 278860
Ion Ratio Lower Upper
112 100
64 53.6 61.8 92.6#
63 25.0 37.2 55.8#

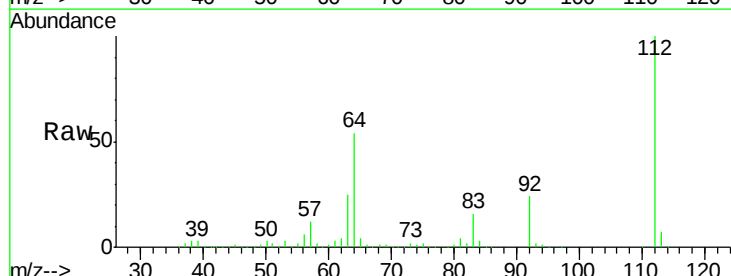

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

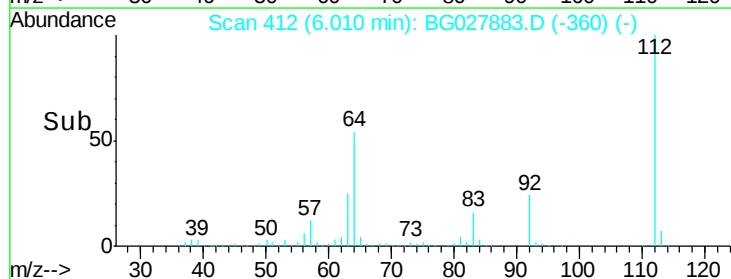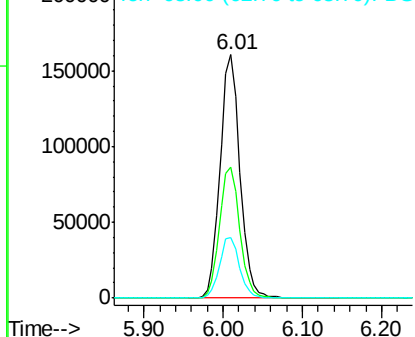

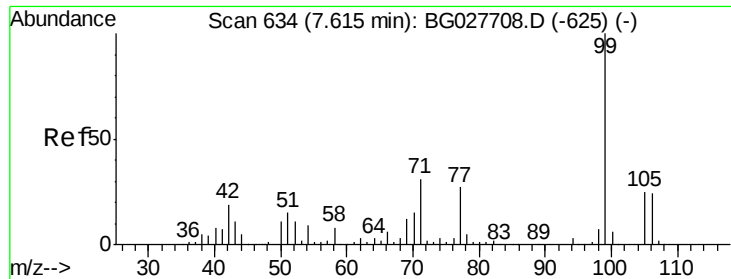

#7

Phenol-d6

Concen: 104.33 ng

RT: 7.58 min Scan# 679

Delta R.T. 0.00 min

Lab File: BG027883.D

Acq: 8 Jul 2017 00:37

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 347812

Ion Ratio Lower Upper




99 100

42 10.8 20.5 30.7#

71 24.6 37.6 56.4#

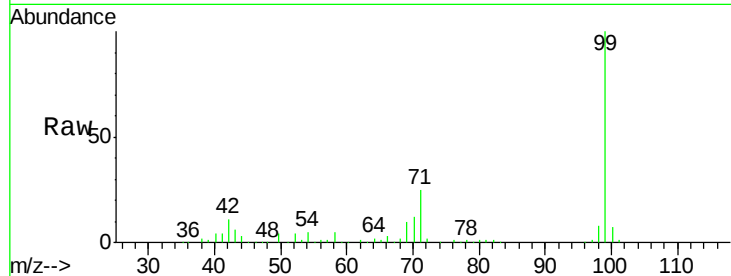

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

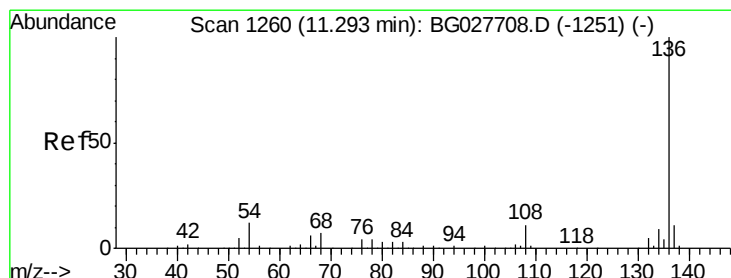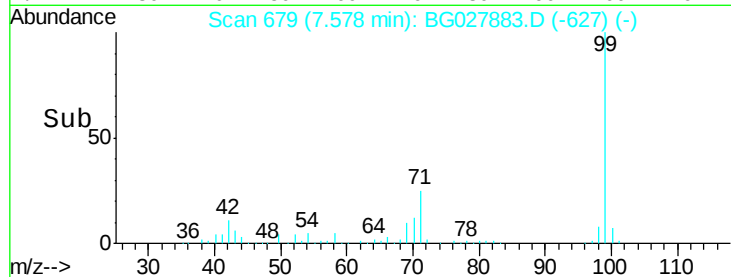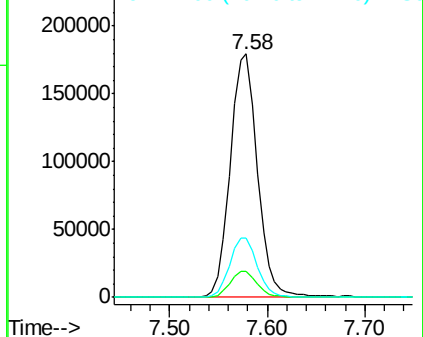

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.25 min Scan# 1304

Delta R.T. 0.00 min

Lab File: BG027883.D

Acq: 8 Jul 2017 00:37

Tgt Ion: 136 Resp: 145595


Ion Ratio Lower Upper

136 100



137 10.6 8.9 13.3

54 7.2 9.3 13.9#

68 7.2 5.1 7.7

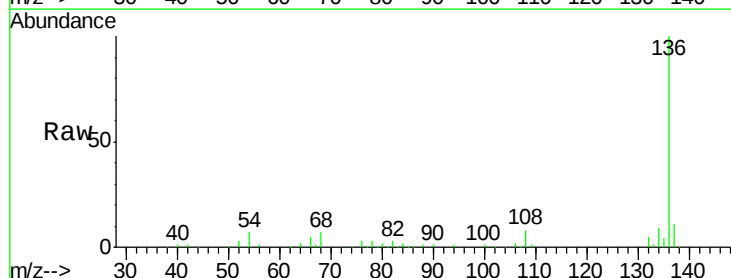

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

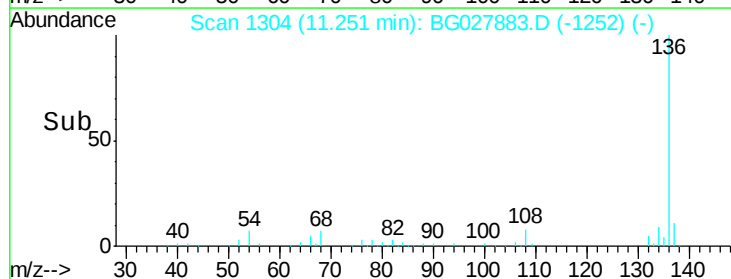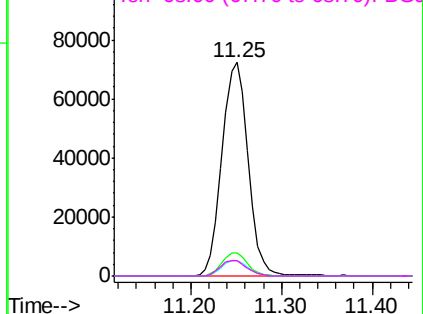







#23
 Nitrobenzene-d5
 Concen: 81.97 ng
 RT: 9.59 min Scan# 1022
 Delta R.T. -0.00 min
 Lab File: BG027883.D
 Acq: 8 Jul 2017 00:37

Instrument :
 BNA_G
 ClientSampled :

Tot Ion: 82 Resp: 214097
 Ion Ratio Lower Upper
 82 100
 128 47.8 26.4 39.6#
 54 38.5 49.4 74.2#

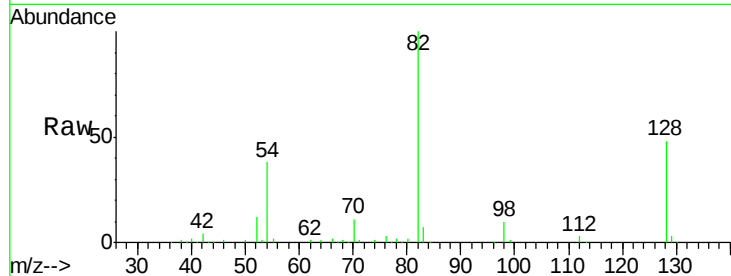


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

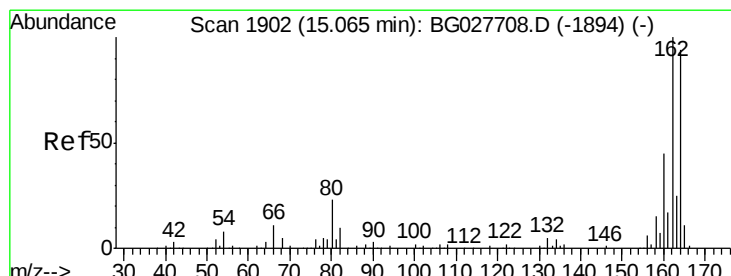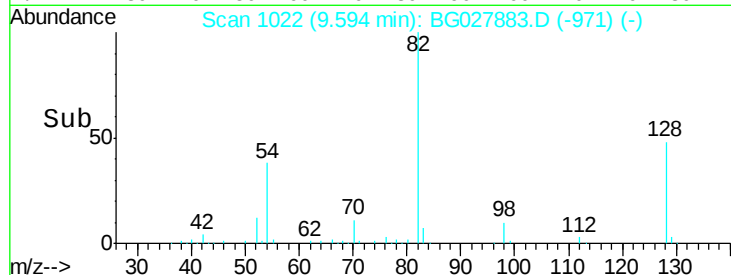
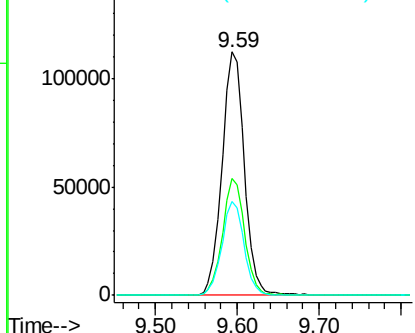



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 15.03 min Scan# 1947
 Delta R.T. 0.00 min
 Lab File: BG027883.D
 Acq: 8 Jul 2017 00:37

Tgt Ion:164 Resp: 79305
 Ion Ratio Lower Upper
 164 100
 162 108.5 85.1 127.7
 160 45.9 34.7 52.1

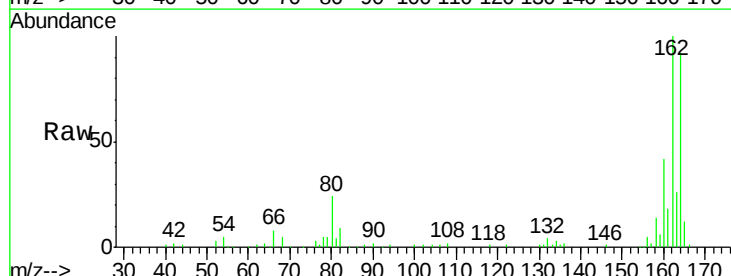

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC



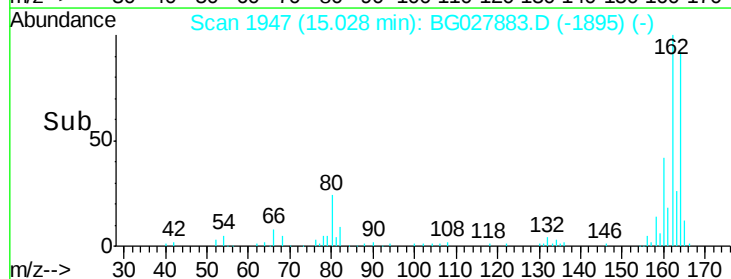
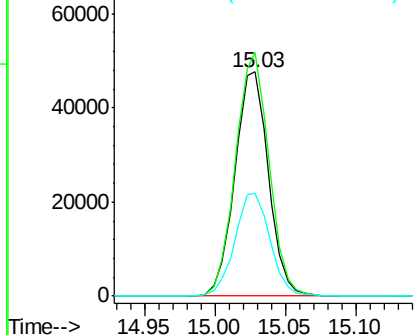


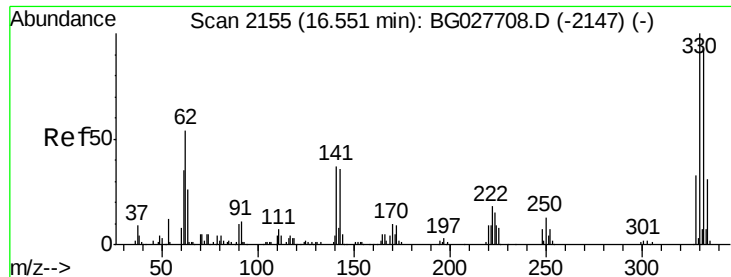

#41
 2,4,6-Tribromophenol
 Concen: 192.96 ng
 RT: 16.51 min Scan# 2200
 Delta R.T. -0.00 min
 Lab File: BG027883.D
 Acq: 8 Jul 2017 00:37




Instrument :
 BNA_G
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
330	100		
332	95.6	77.3	115.9
141	28.5	32.1	48.1#

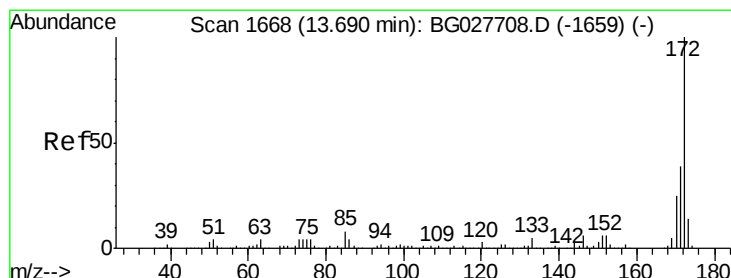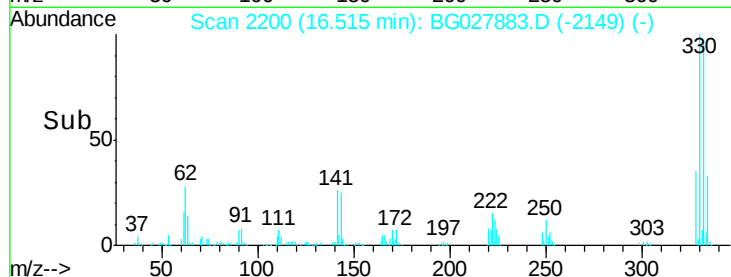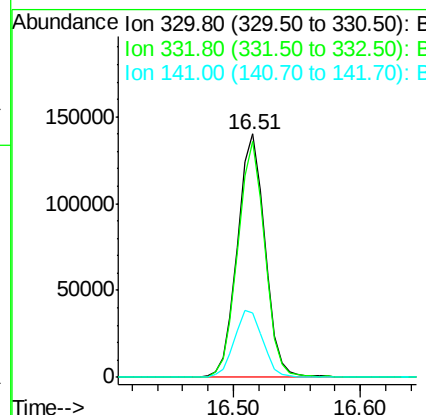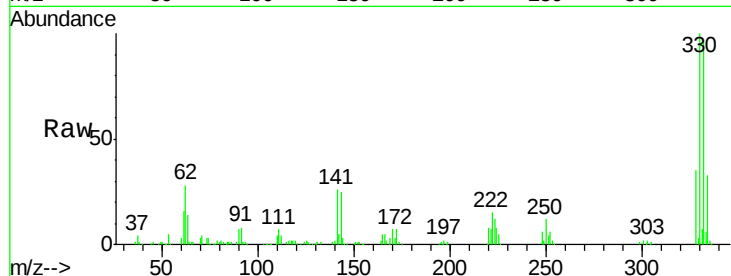

#44
 2-Fluorobiphenyl
 Concen: 98.90 ng
 RT: 13.65 min Scan# 1712
 Delta R.T. -0.00 min
 Lab File: BG027883.D
 Acq: 8 Jul 2017 00:37

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.4	32.2	48.2
170	23.9	21.8	32.6

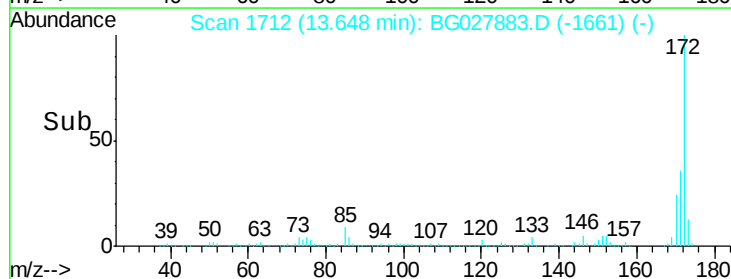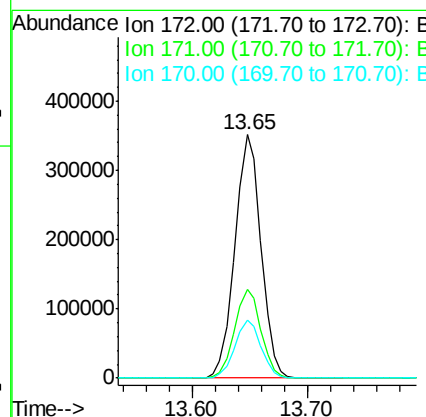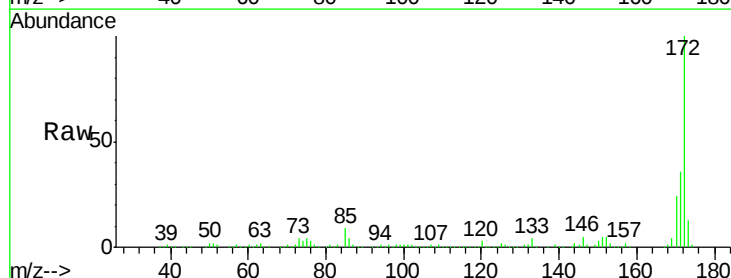


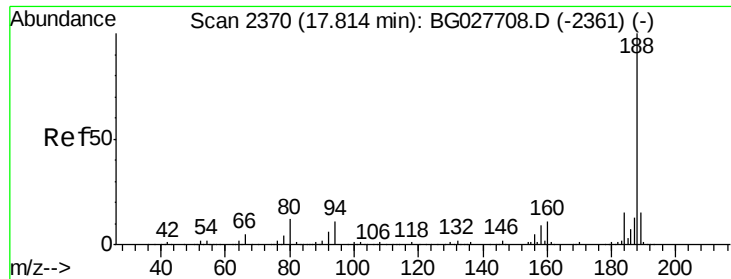




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.77 min Scan# 2414
Delta R.T. -0.00 min
Lab File: BG027883.D
Acq: 8 Jul 2017 00:37

Instrument :
BNA_G
ClientSampleId :

Tot Ion:188 Resp: 211187
Ion Ratio Lower Upper
188 100
94 12.7 5.8 8.8#
80 13.5 7.5 11.3#

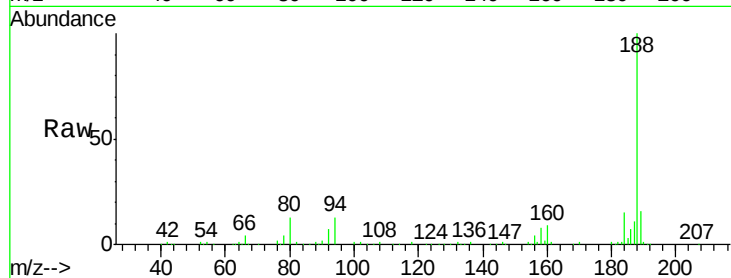


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

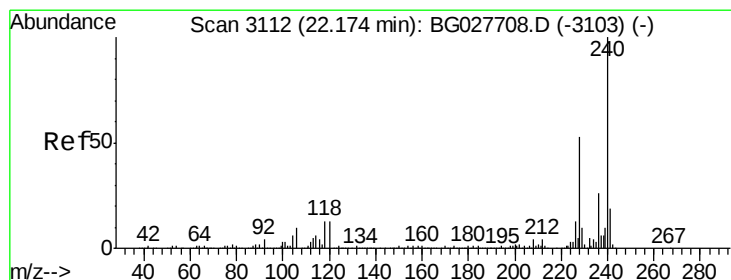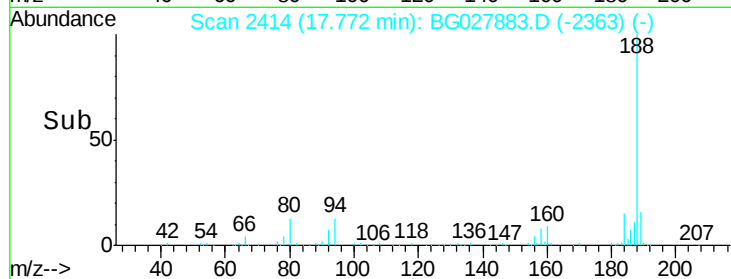
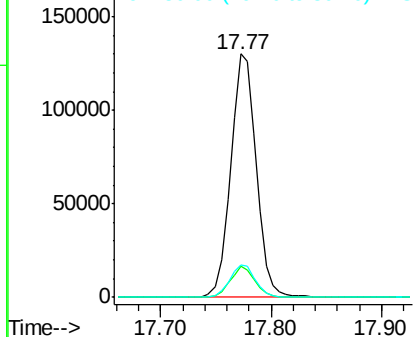



#75
Chrysene-d12
Concen: 20.00 ng
RT: 22.12 min Scan# 3154
Delta R.T. -0.01 min
Lab File: BG027883.D
Acq: 8 Jul 2017 00:37

Tgt Ion:240 Resp: 252198
Ion Ratio Lower Upper
240 100
120 14.1 5.7 8.5#
236 25.7 22.2 33.4

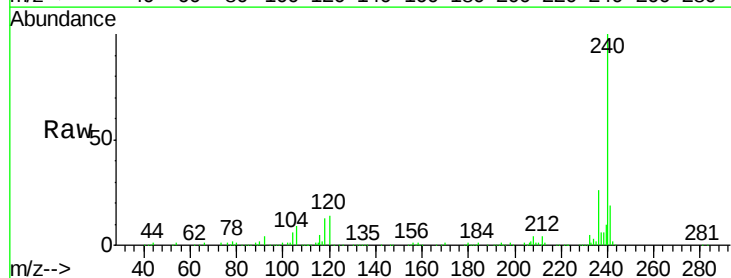

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

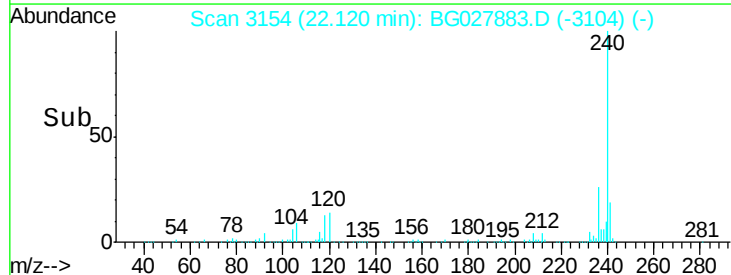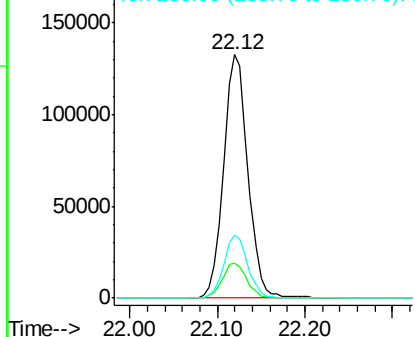

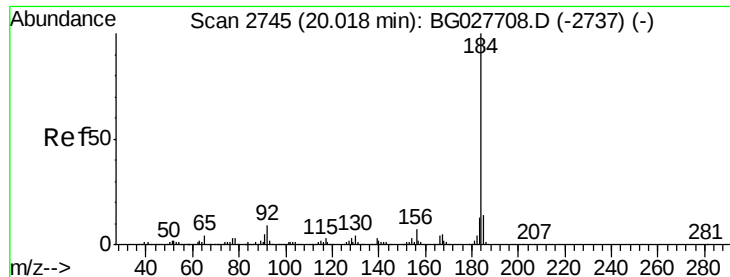

#76

Benzidine

Concen: 3.23 ng

RT: 20.01 min Scan# 2795

Delta R.T. 0.02 min

Lab File: BG027883.D

Acq: 8 Jul 2017 00:37

Instrument :

BNA_G

ClientSampled :


Tot Ion:184 Resp: 64

Ion Ratio Lower Upper

184 100

185 0.0 13.0 19.6#


183 0.0 11.0 16.6#

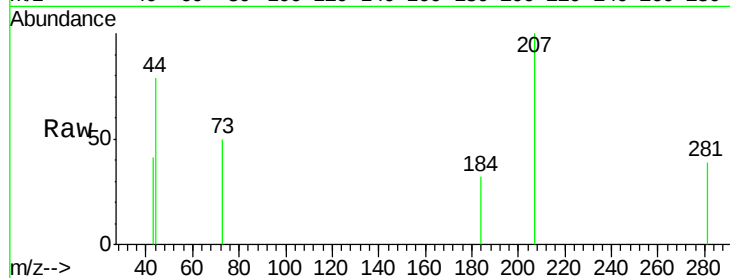



Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

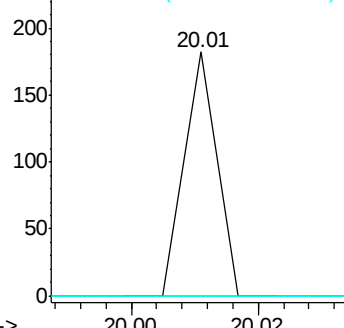

Time-->

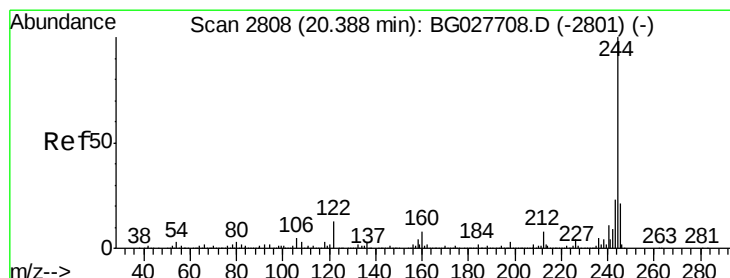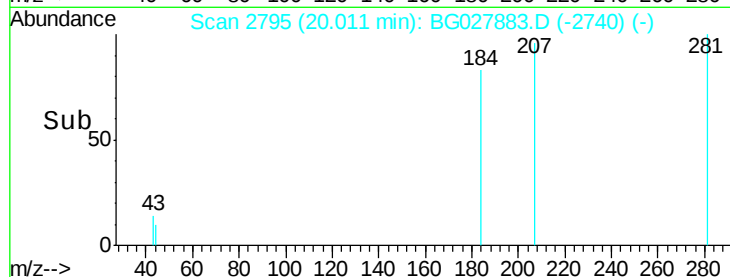

#78

Terphenyl-d14

Concen: 112.35 ng

RT: 20.35 min Scan# 2853

Delta R.T. -0.00 min

Lab File: BG027883.D

Acq: 8 Jul 2017 00:37


Tgt Ion:244 Resp: 1208617

Ion Ratio Lower Upper

244 100

212 6.5 10.0 15.0#


122 14.1 8.6 12.8#

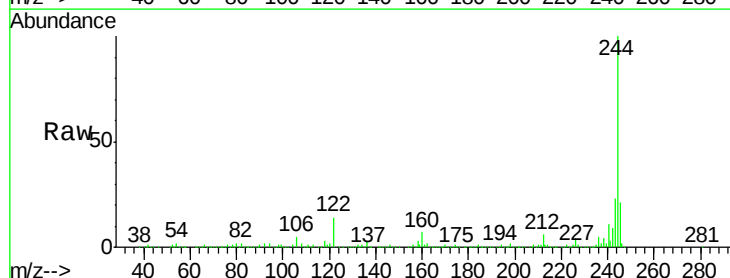


Abundance Ion 244.00 (243.70 to 244.70): E


Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

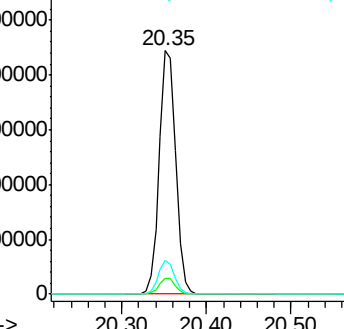

Time-->

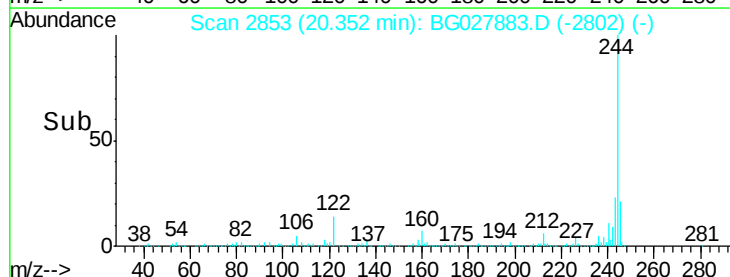

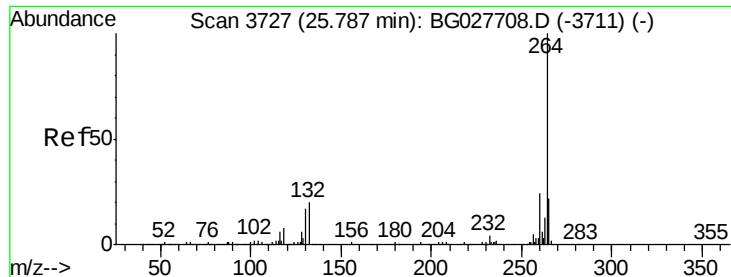

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 25.69 min Scan# 3761
 Delta R.T. -0.01 min
 Lab File: BG027883.D
 Acq: 8 Jul 2017 00:37

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.1	21.8	32.8
265	21.3	18.2	27.4

