
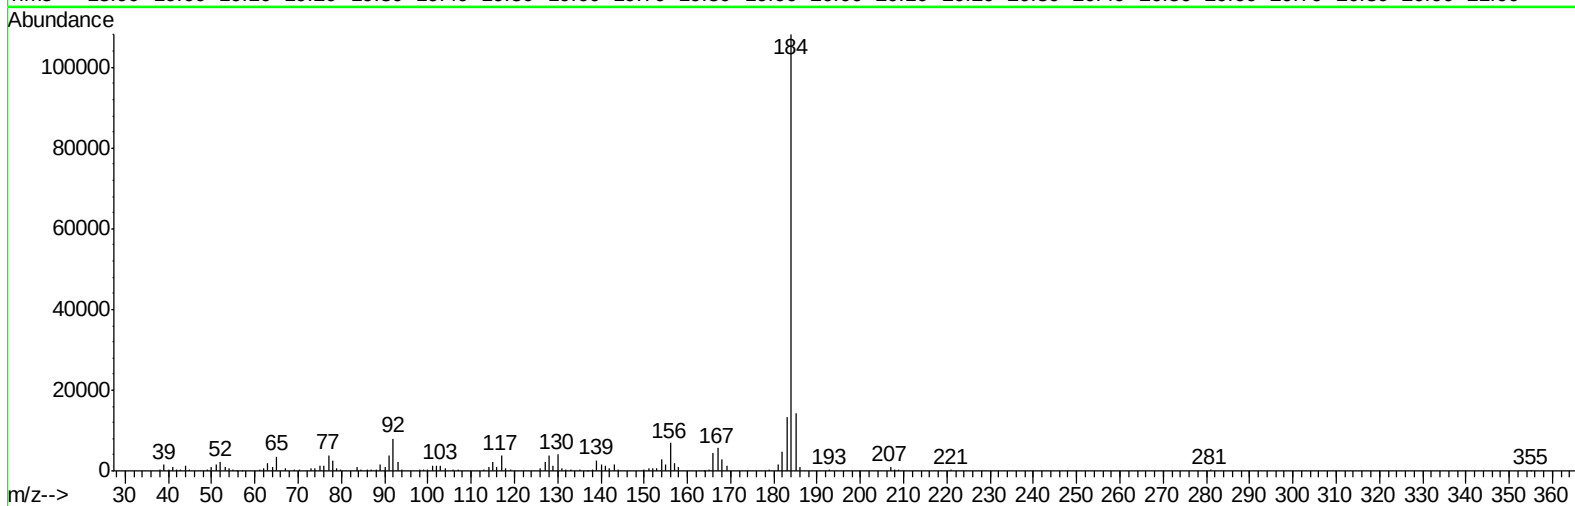


Data Path : Z:\HPCHEM1\BNA G\Data\BG070717\
Data File : BG027865.D
Acq On : 7 Jul 2017 10:48
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 03:31:29 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 17:43:21 2017
Response via : Initial Calibration

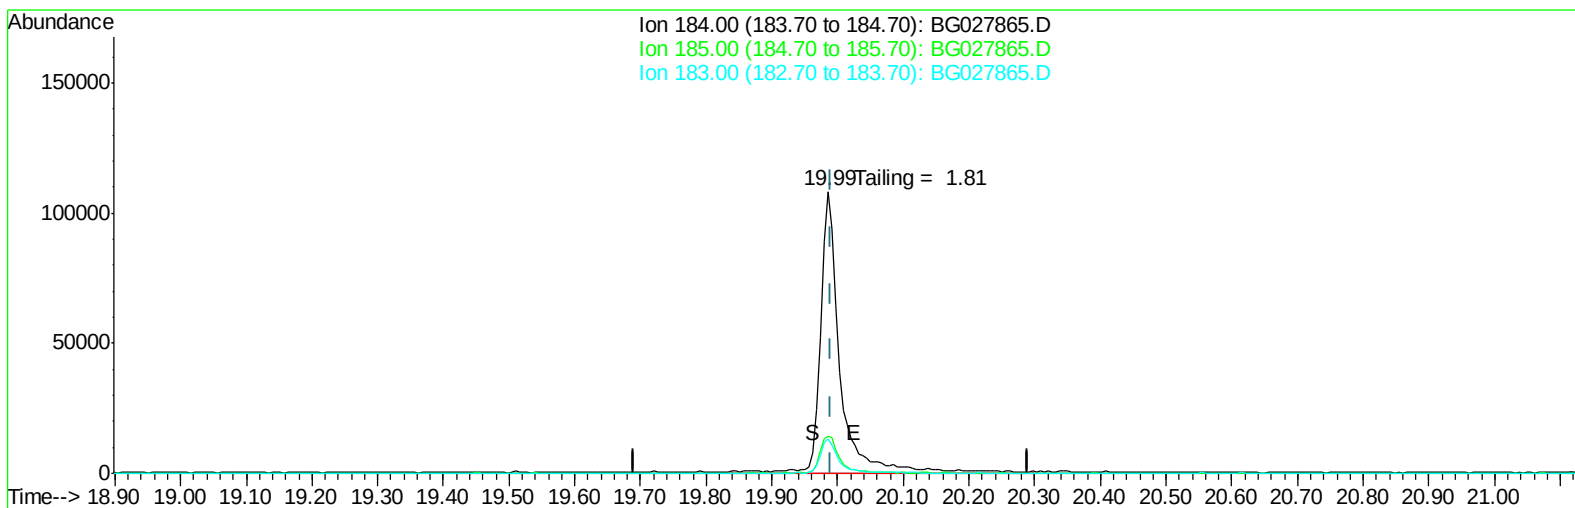

TIC: BG027865.D

(76) Benzidine



19.985min (-0.004) 0.00ng

response 209369

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	13.29
183.00	13.80	12.19
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG070717\
Data File : BG027865.D
Acq On : 7 Jul 2017 10:48
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 03:31:29 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 17:43:21 2017
Response via : Initial Calibration

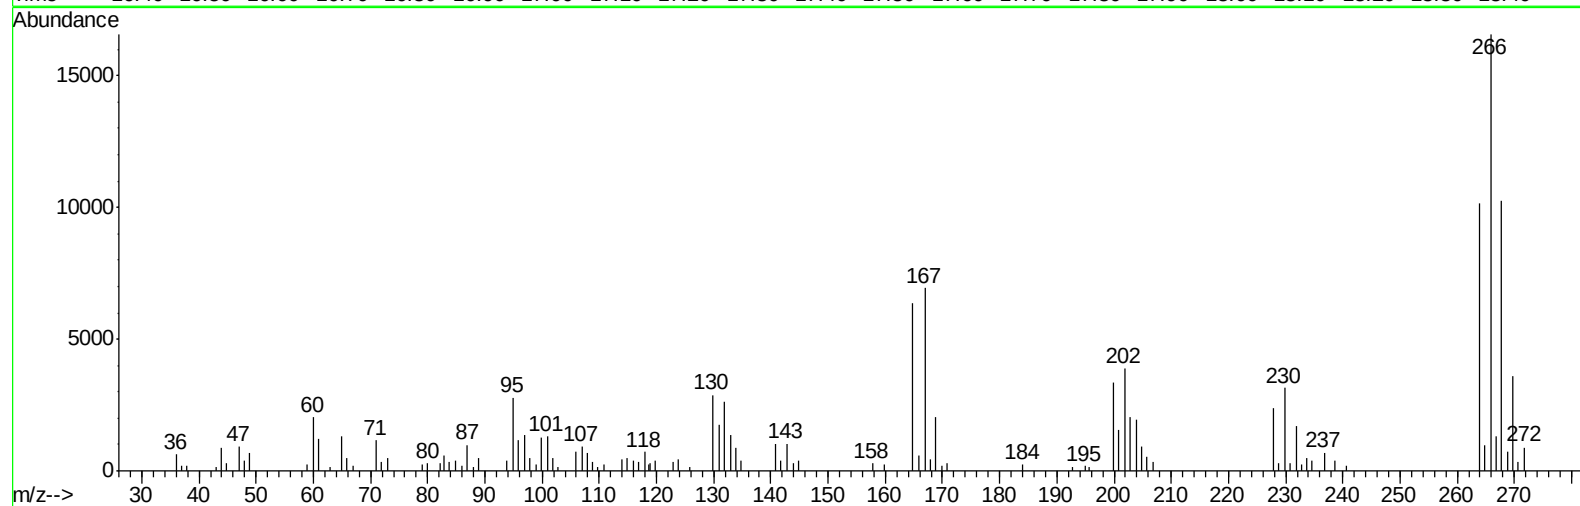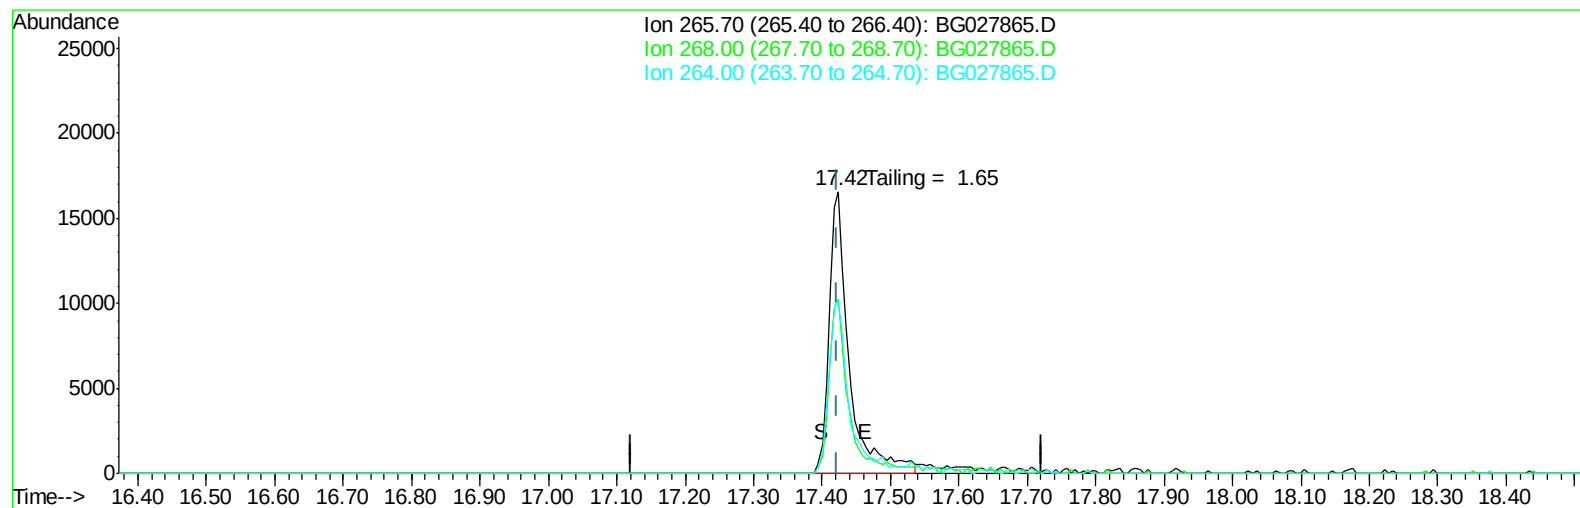

TIC: BG027865.D

(69) Pentachlorophenol (C)

17.424min (+0.002) 0.00ng

response 33073

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	61.78
264.00	62.60	61.18
0.00	0.00	0.00