
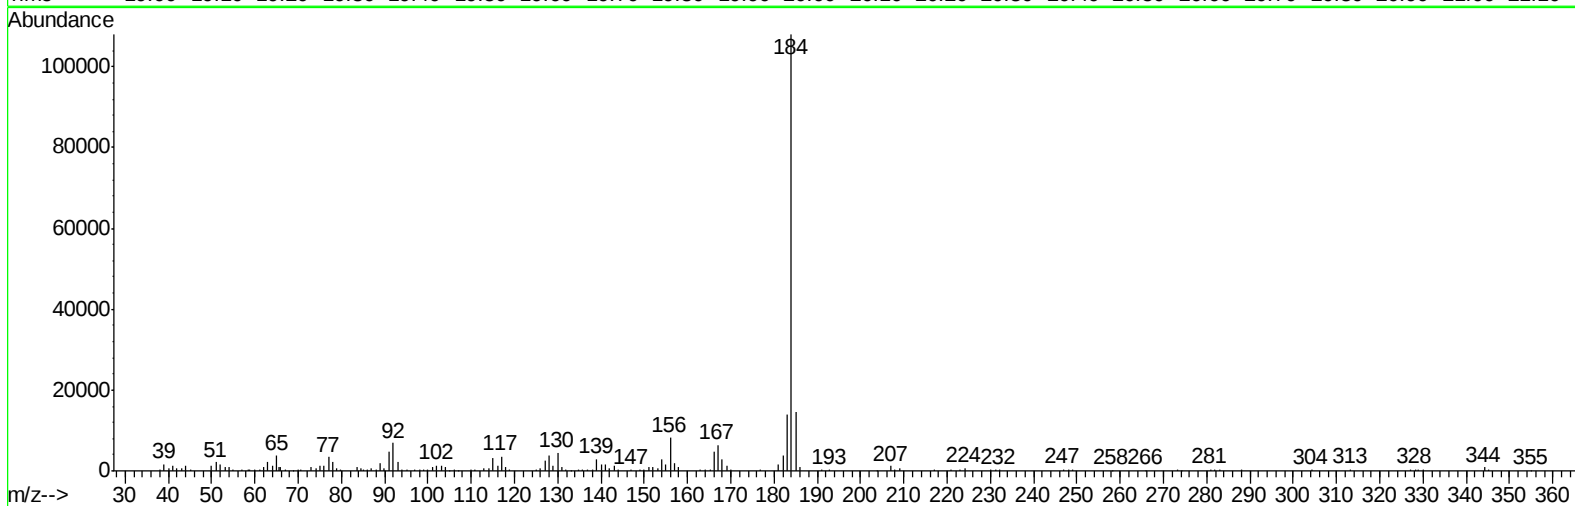


Data Path : Z:\HPCHEM1\BNA G\Data\BG070717\  
Data File : BG027869.D  
Acq On : 7 Jul 2017 15:21  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 03:35:55 2017  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062817.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jul 07 17:43:21 2017  
Response via : Initial Calibration

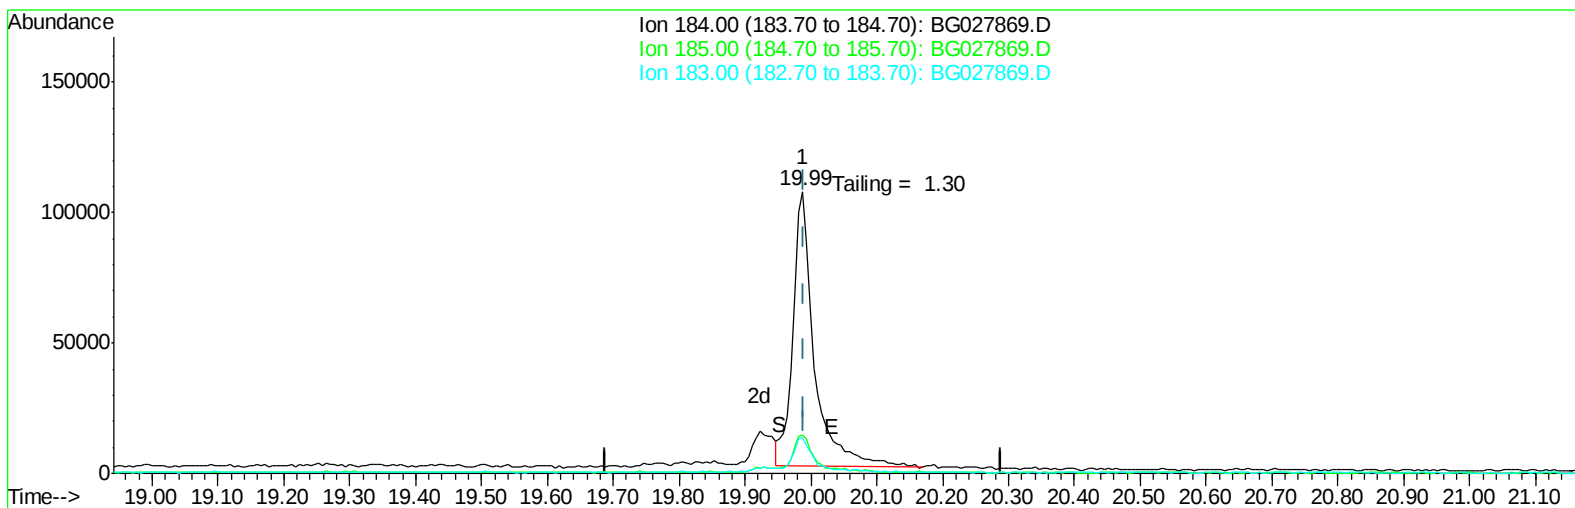

TIC: BG027869.D

(76) Benzidine



19.988min (-0.002) 178486.23ng

response 245904

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.30 | 13.64 |
| 183.00 | 13.80 | 12.79 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA G\Data\BG070717\  
Data File : BG027869.D  
Acq On : 7 Jul 2017 15:21  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 03:35:55 2017  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062817.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jul 07 17:43:21 2017  
Response via : Initial Calibration

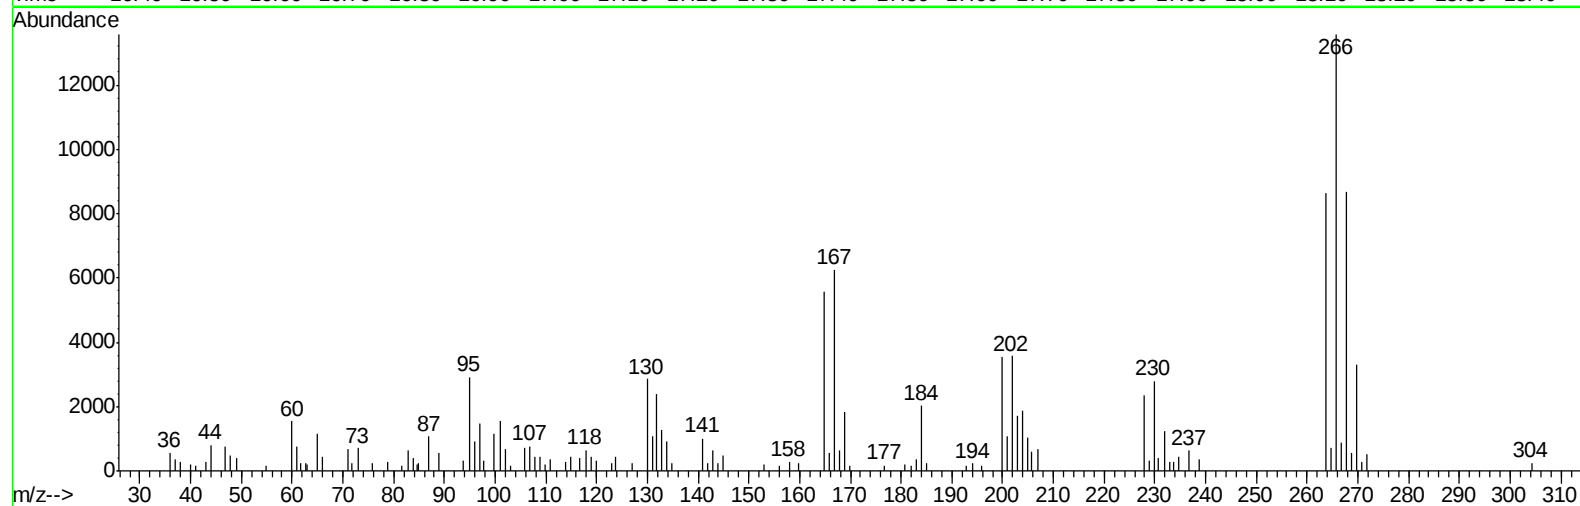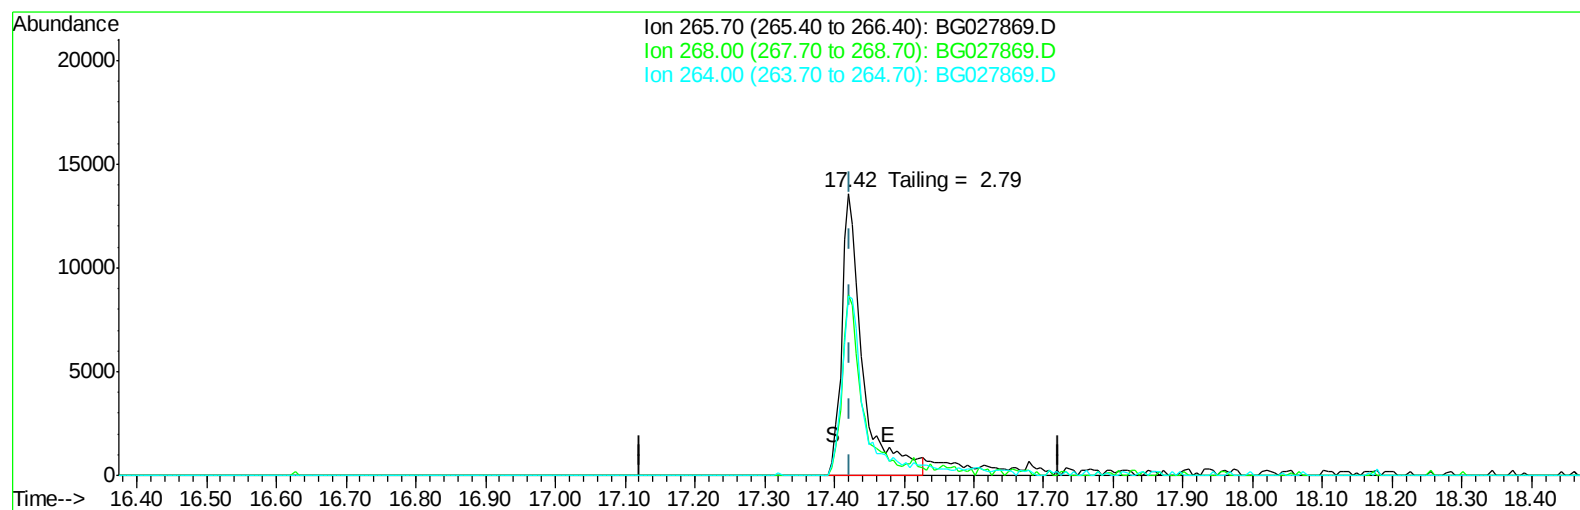

TIC: BG027869.D

(69) Pentachlorophenol (C)

17.420min (-0.002) 0.00ng

response 25498

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 60.70 | 68.17 |
| 264.00 | 62.60 | 63.75 |
| 0.00   | 0.00  | 0.00  |