


Data Path : Z:\HPCHEM1\BNA_G\Data\BG070717\
 Data File : BG027865.D
 Acq On : 7 Jul 2017 10:48
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 07 17:43:21 2017

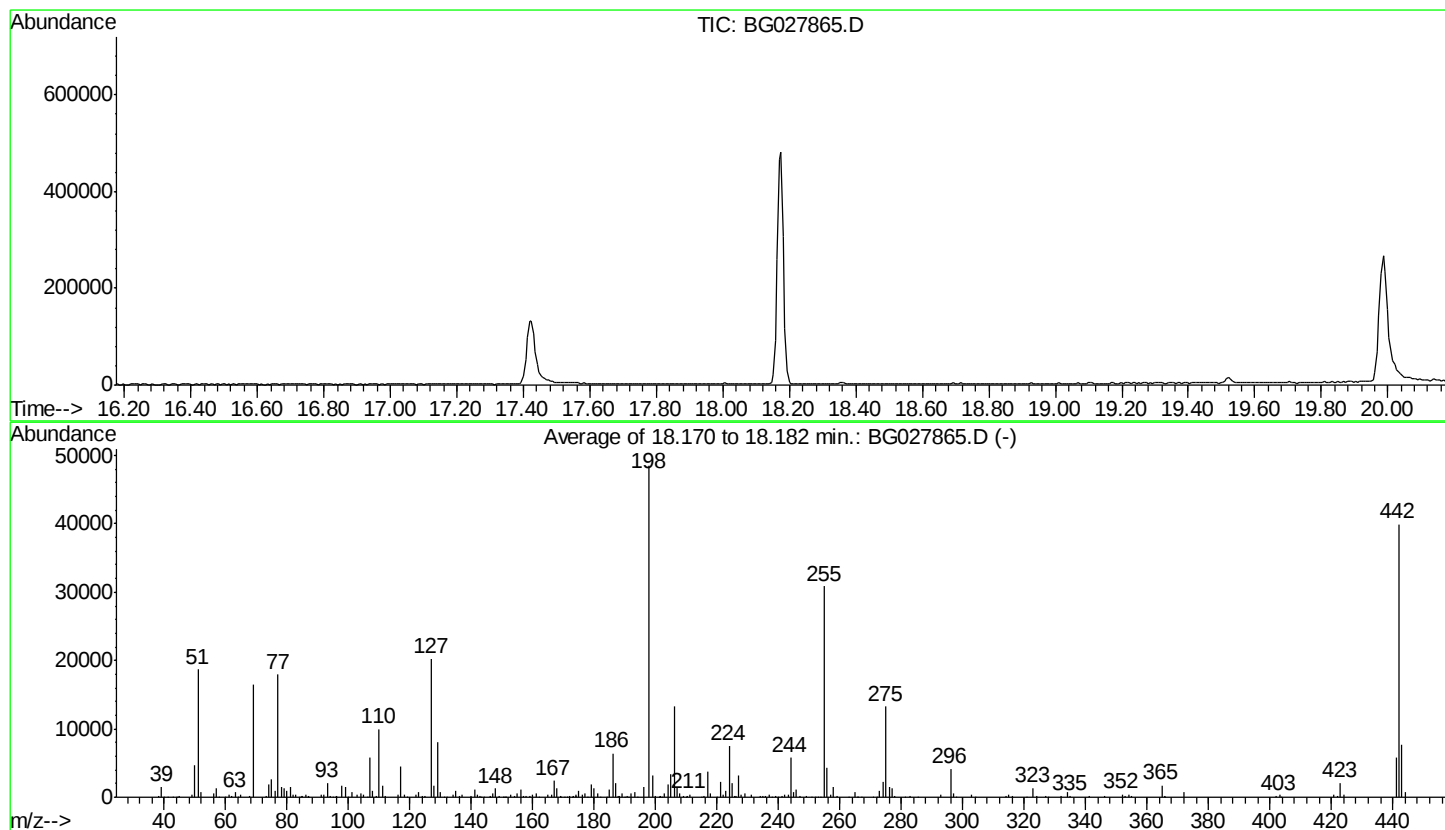

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	18725	PASS
68	69	0.00	2	1.1	175	PASS
69	198	0.00	100	34.0	16507	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.8	20254	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48512	PASS
199	198	5	9	6.6	3226	PASS
275	198	10	60	27.4	13270	PASS
365	198	1	100	3.5	1688	PASS
441	442	0.01	24	14.6	5821	PASS
442	198	50	100	82.2	39901	PASS
443	442	15	24	19.1	7611	PASS