


Data Path : Z:\HPCHEM1\BNA_G\Data\BG070717\
 Data File : BG027869.D
 Acq On : 7 Jul 2017 15:21
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 07 17:43:21 2017

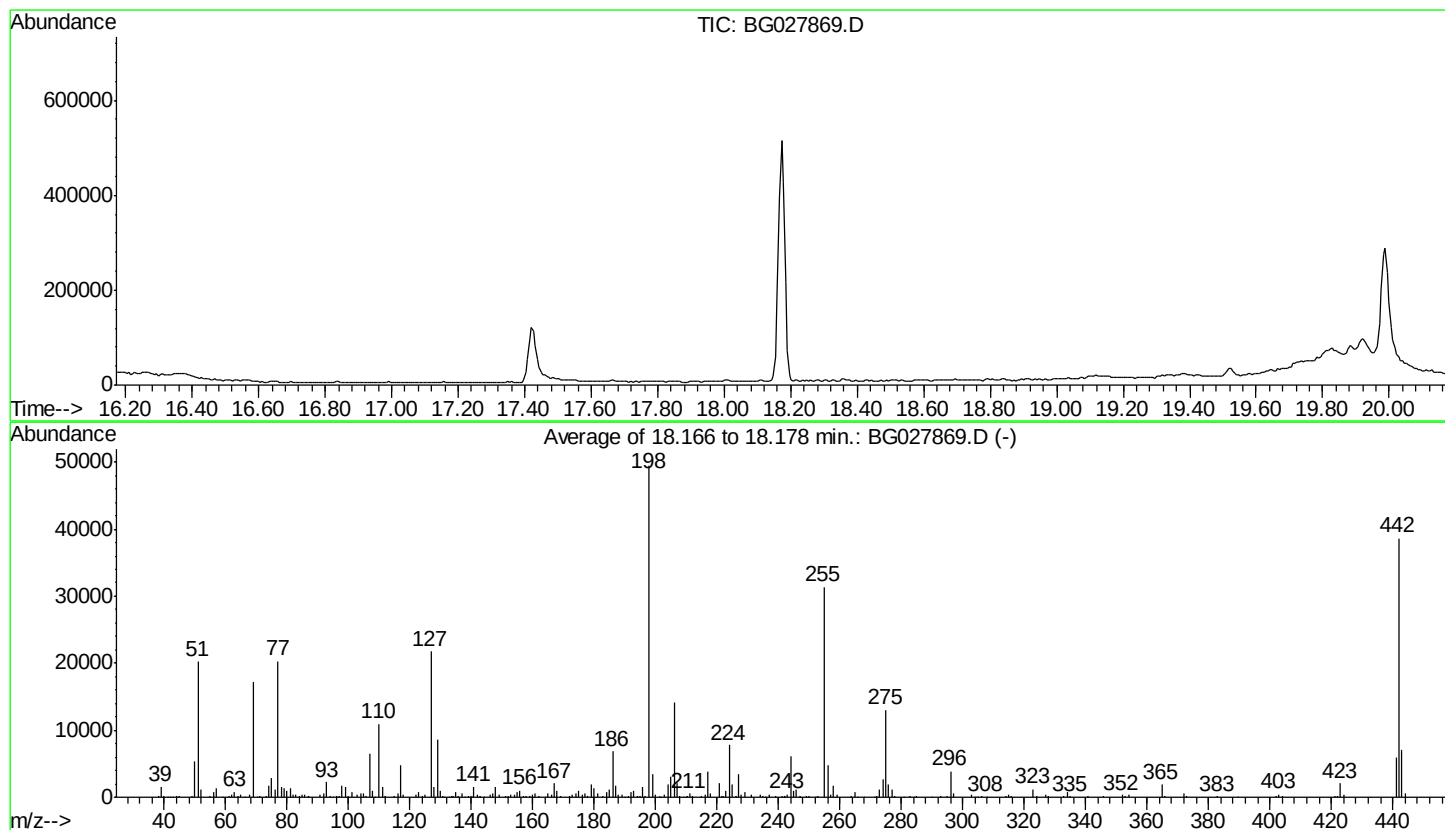

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.9	20228	PASS
68	69	0.00	2	2.0	344	PASS
69	198	0.00	100	34.9	17264	PASS
70	69	0.00	2	0.5	91	PASS
127	198	10	80	43.9	21740	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49469	PASS
199	198	5	9	7.0	3469	PASS
275	198	10	60	26.4	13079	PASS
365	198	1	100	3.8	1865	PASS
441	442	0.01	24	15.2	5861	PASS
442	198	50	100	78.0	38602	PASS
443	442	15	24	18.6	7164	PASS