
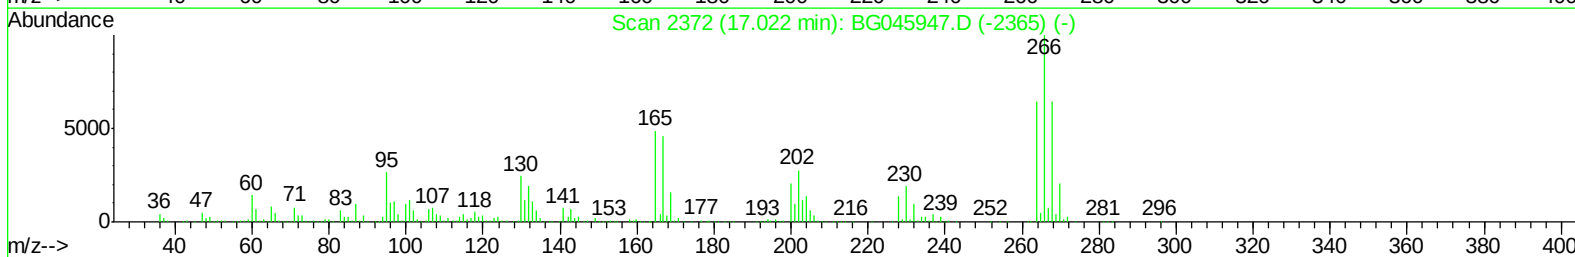
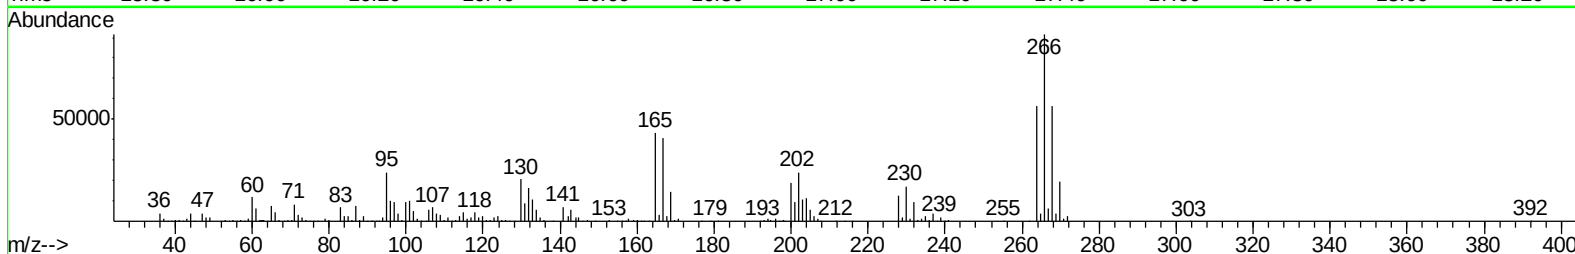


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070720\
 Data File : BG045952.D
 Acq On : 7 Jul 2020 8:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 07:03:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG070620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 07 09:58:42 2020
 Response via : Initial Calibration

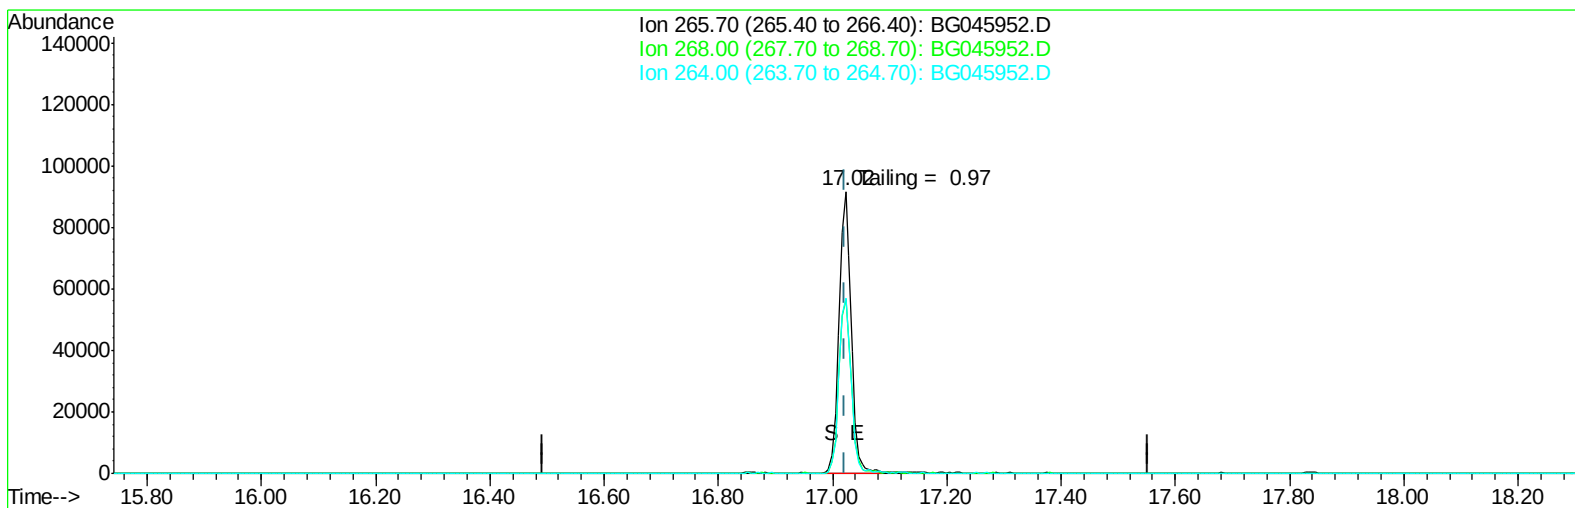

TIC: BG045952.D

(70) Pentachlorophenol (C)




17.022min (-0.000) 78780.20ng

response 134996

Ion	Exp%	Act%
265.70	100	100
268.00	64.80	61.95
264.00	64.20	62.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070720\
 Data File : BG045952.D
 Acq On : 7 Jul 2020 8:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 07:03:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG070620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 07 09:58:42 2020
 Response via : Initial Calibration

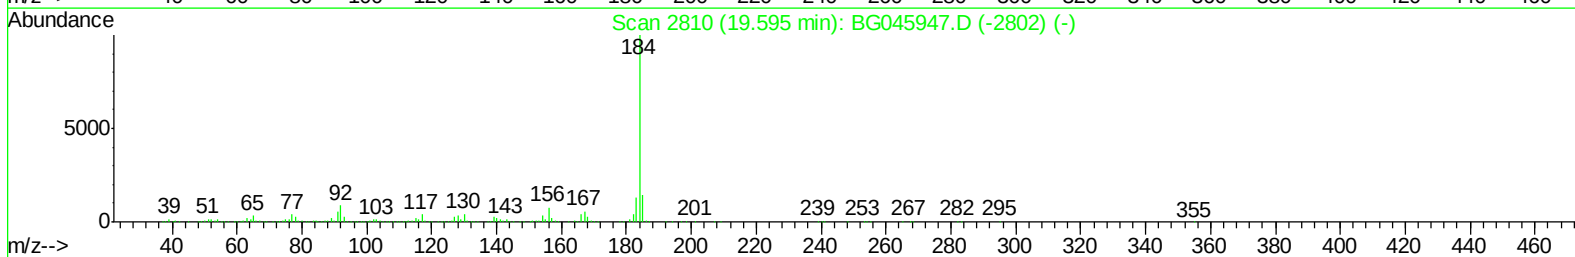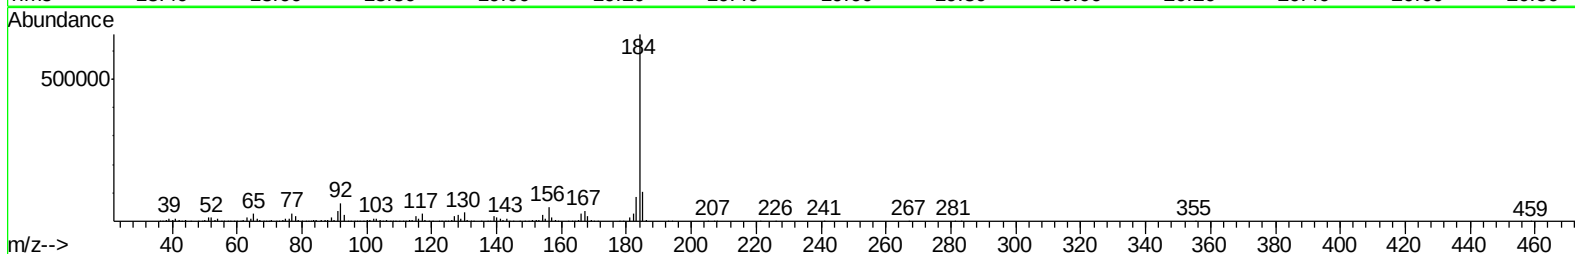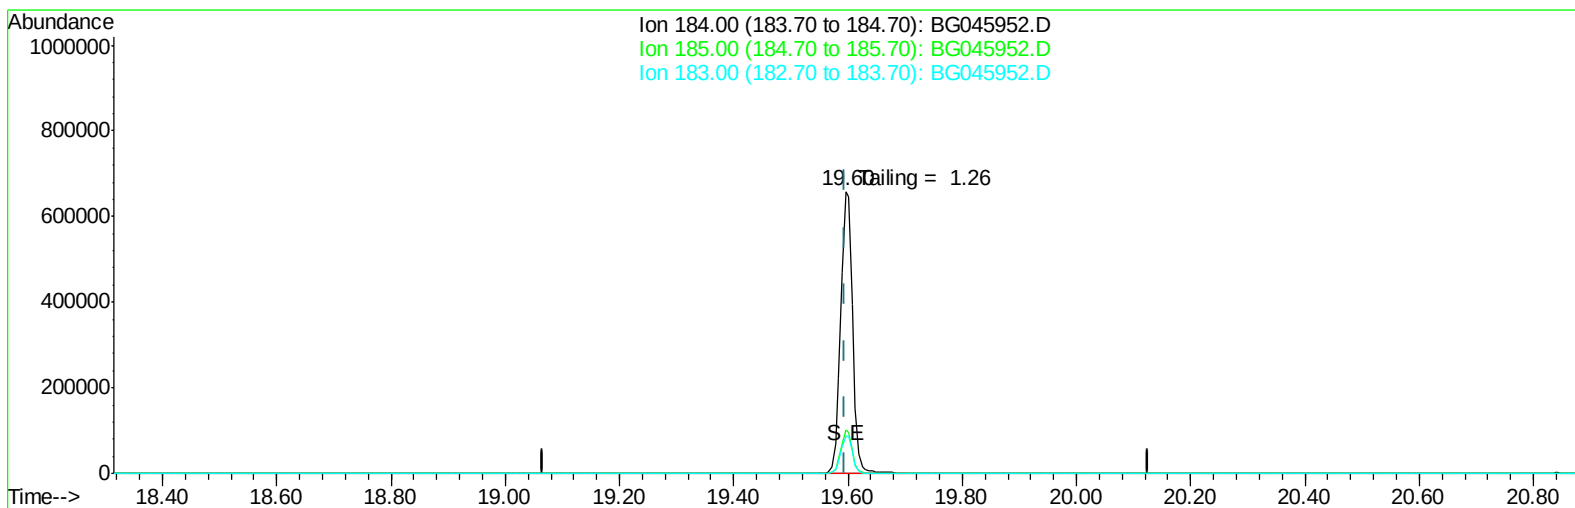

TIC: BG045952.D

(77) Benzidine

19.595min (-0.000) 2785.19ng

response 961522

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	15.66
183.00	13.00	13.32
0.00	0.00	0.00